


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090518\
Data File : VV007383.D
Acq On : 05 Sep 2018 14:45
Operator : SY/MD
Sample : BFB72
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB72

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Title : VOC Analysis
Last Update : Thu Sep 06 02:12:11 2018

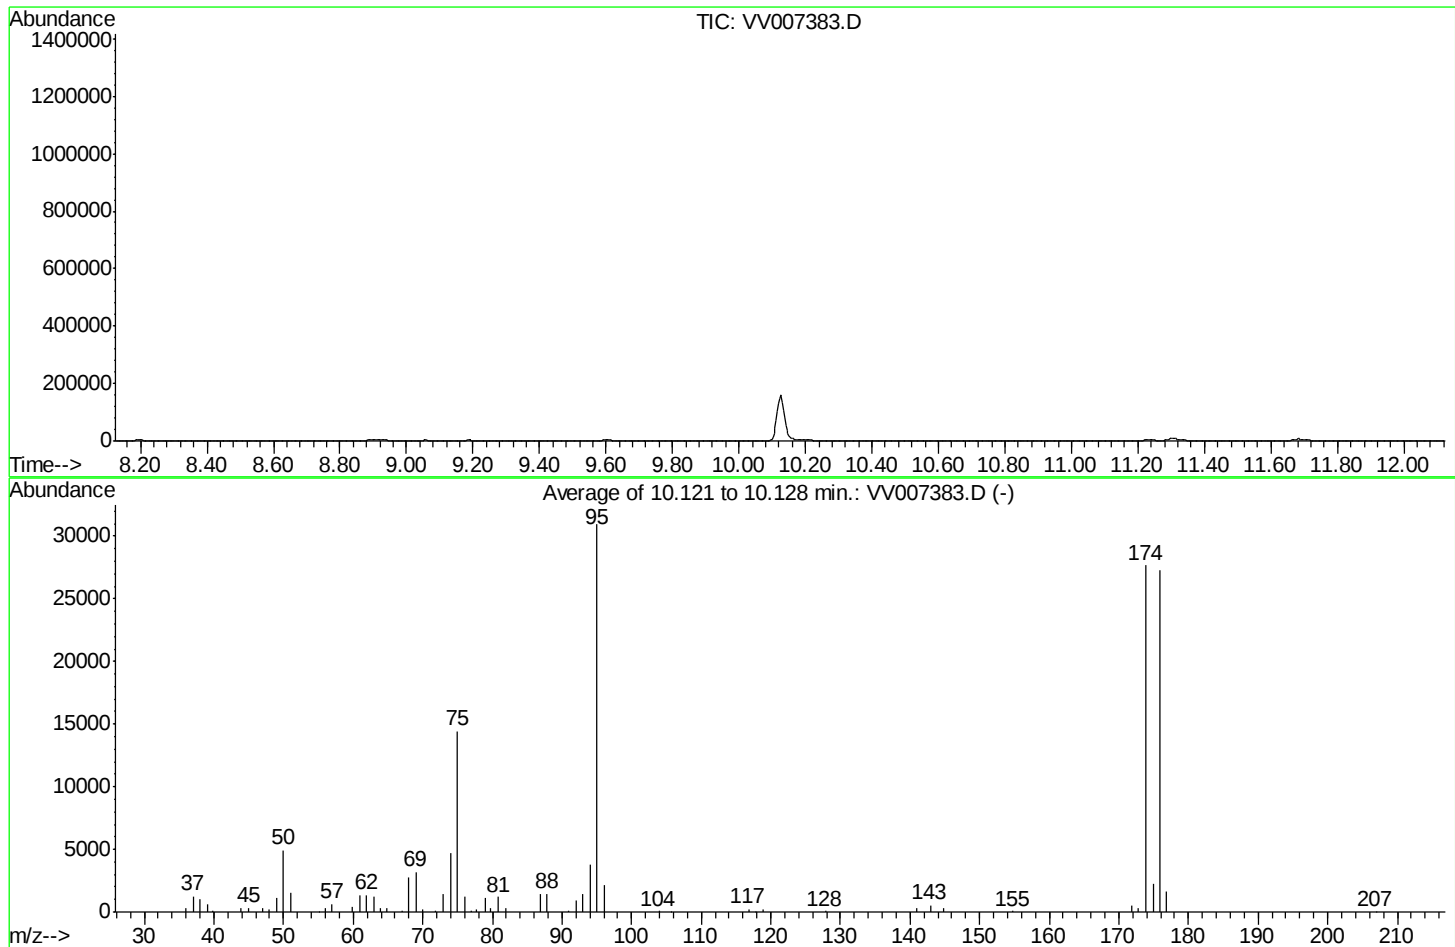

AutoFind: Scans 2871, 2872, 2873; Background Corrected with Scan 2859

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.9	4923	PASS
75	95	30	80	46.6	14427	PASS
95	95	100	100	100.0	30949	PASS
96	95	5	9	6.8	2102	PASS
173	174	0.00	2	1.3	355	PASS
174	95	50	120	89.4	27656	PASS
175	174	5	9	8.2	2273	PASS
176	174	95	101	98.7	27298	PASS
177	176	5	9	6.1	1664	PASS

Scan 2859 (10.083 min): VV007383.D
BFB72

m/z	Abundance
39.90	257.0
43.90	782.0

Instrument :
MSVOA_V
ClientSampleId :
BFB72

m/z	Abundance
35.90	341.0
37.00	1301.0
38.00	1025.0
39.10	626.0
39.90	379.0
43.90	1094.0
45.00	354.0
47.00	373.0
47.90	207.0
49.00	1077.0
50.00	4613.0
51.00	1489.0
56.00	348.0
57.00	701.0
59.90	379.0
61.00	1274.0
62.00	1317.0
63.00	1179.0
63.90	324.0
64.90	348.0
67.10	122.0
68.00	2741.0
69.00	2984.0
70.00	183.0
71.80	144.0
73.00	1248.0
74.00	4475.0
75.00	13674.0
76.00	1270.0
76.90	155.0
77.70	186.0
78.90	1191.0
79.80	266.0
80.90	1095.0
81.90	308.0
86.90	1394.0
87.90	1477.0
91.10	108.0
92.00	912.0
93.00	1408.0
94.00	3770.0
95.00	30832.0
96.00	2183.0
116.90	192.0
117.80	107.0
118.90	188.0
140.90	295.0
142.90	542.0
144.70	277.0
171.90	507.0
172.80	364.0
173.90	25864.0
174.90	2311.0
175.90	26208.0
176.90	1607.0

Instrument :
MSVOA_V
ClientSampleId :
BFB72

m/z	Abundance
35.90	331.0
37.00	1245.0
38.00	1022.0
39.10	659.0
39.90	417.0
43.90	1135.0
45.00	366.0
47.00	354.0
47.90	190.0
49.00	1161.0
50.00	5065.0
51.00	1550.0
55.00	109.0
56.00	314.0
57.00	671.0
59.90	437.0
61.10	1357.0
62.00	1376.0
63.00	1252.0
63.90	324.0
64.90	333.0
67.10	116.0
68.00	2872.0
69.00	3338.0
69.90	189.0
71.90	120.0
73.00	1464.0
74.00	4810.0
75.00	14938.0
76.00	1240.0
76.90	142.0
77.80	228.0
78.90	1197.0
79.80	299.0
80.90	1227.0
81.90	276.0
86.90	1465.0
87.90	1522.0
91.00	106.0
91.90	954.0
93.00	1414.0
94.00	3957.0
95.00	31856.0
96.00	2149.0
104.00	100.0
116.90	224.0
118.90	188.0
127.80	106.0
140.90	291.0
142.90	537.0
144.70	270.0
154.80	130.0
171.90	556.0
172.80	368.0
173.90	28584.0
174.90	2380.0
175.90	28464.0
176.90	1723.0

Instrument :
MSVOA_V
ClientSampleId :
BFB72

m/z	Abundance
35.90	316.0
37.00	1171.0
38.00	934.0
39.10	561.0
39.90	406.0
44.00	1097.0
45.00	329.0
46.90	323.0
47.90	214.0
49.00	1089.0
50.00	5093.0
51.00	1570.0
56.00	285.0
57.00	575.0
59.90	420.0
61.00	1324.0
61.90	1349.0
63.00	1236.0
64.00	228.0
64.90	315.0
68.00	2712.0
69.00	3343.0
69.90	163.0
71.90	120.0
73.00	1519.0
74.00	4846.0
75.00	14669.0
76.00	1136.0
77.00	143.0
77.80	270.0
78.90	1121.0
79.80	308.0
80.90	1254.0
81.90	249.0
86.90	1427.0
87.90	1422.0
90.90	102.0
91.90	893.0
93.00	1328.0
94.00	3668.0
95.00	30160.0
96.00	1974.0
103.90	135.0
105.70	108.0
116.70	235.0
118.90	174.0
127.90	130.0
140.90	263.0
142.90	476.0
144.80	276.0
154.80	125.0
171.90	510.0
172.80	333.0
173.90	28520.0
174.90	2130.0
175.90	27224.0
176.90	1663.0
206.90	158.0

Instrument :
MSVOA_V
ClientSampleId :
BFB72