


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV090519\
Data File : VV012579.D
Acq On : 05 Sep 2019 12:04
Operator : SY/MD
Sample : BFB31
Misc : 25mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB31

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR090519WMA.M
Title : TRACE VOA SOM01.0
Last Update : Mon Sep 09 12:56:16 2019

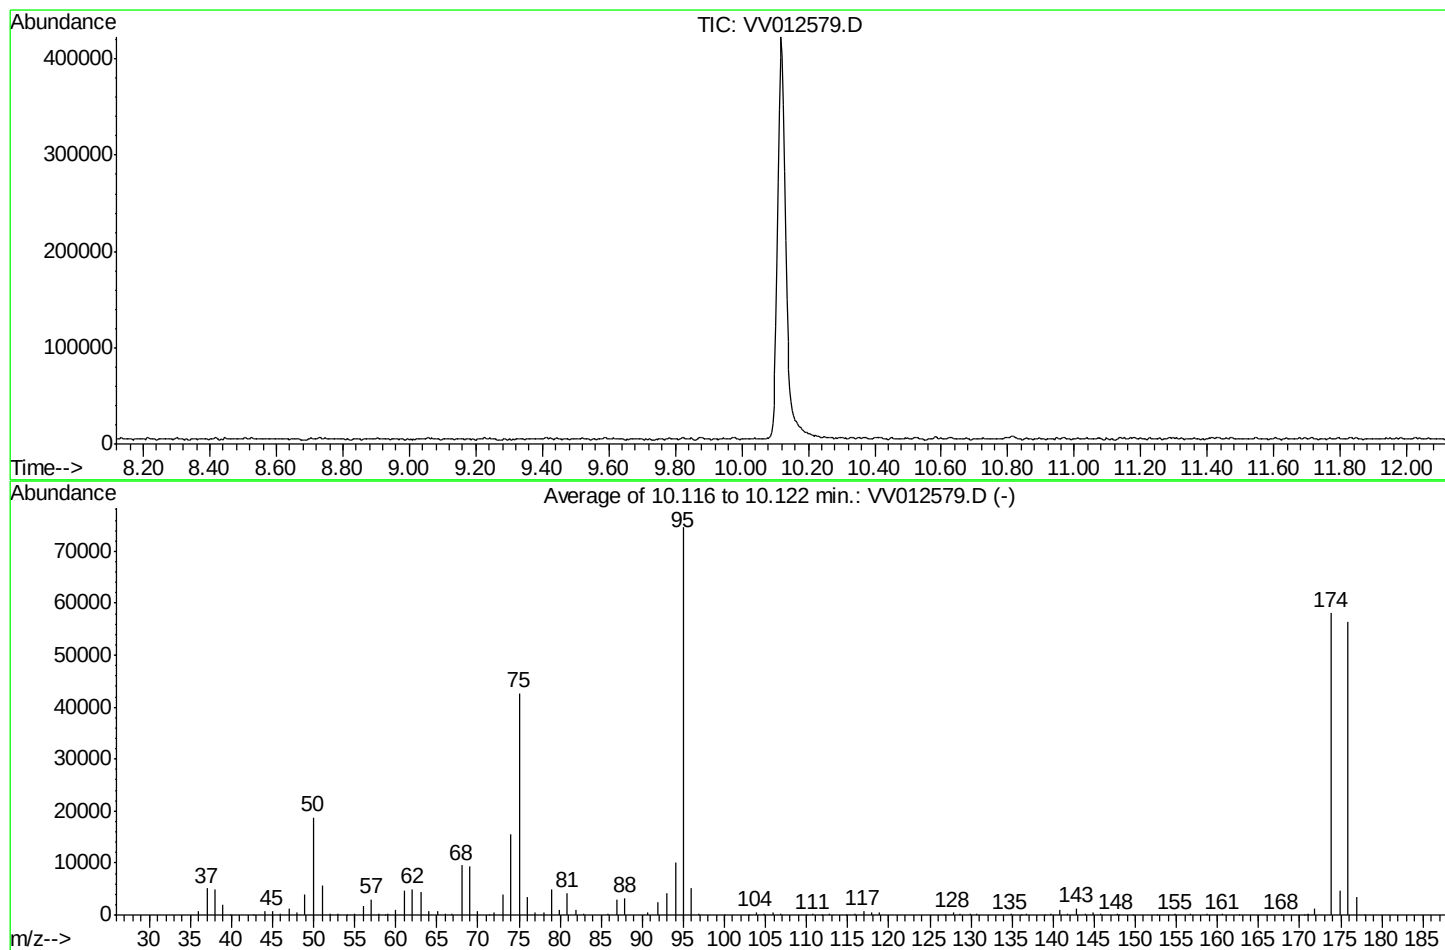

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	25.1	18761	PASS
75	95	30	80	57.2	42693	PASS
95	95	100	100	100.0	74608	PASS
96	95	5	9	7.1	5299	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	77.9	58141	PASS
175	174	5	9	8.2	4753	PASS
176	174	95	101	97.1	56432	PASS
177	176	5	9	6.2	3513	PASS

m/z	Abundance
36.00	1074.0
37.00	5170.0
38.00	5019.0
39.00	2188.0
40.00	773.0
42.70	135.0
44.00	1431.0
45.00	1124.0
45.90	299.0
47.00	1163.0
47.90	758.0
49.00	4248.0
50.00	19016.0
51.00	5985.0
52.00	278.0
52.90	185.0
54.10	245.0
55.00	328.0
56.00	1762.0
57.00	3017.0
58.00	165.0
58.70	108.0
59.10	142.0
60.00	1040.0
61.00	4521.0
62.00	4801.0
63.00	4644.0
63.90	706.0
65.10	956.0
66.00	249.0
67.10	292.0
68.00	9453.0
69.00	9555.0
70.00	865.0
71.30	123.0
72.00	481.0
73.00	4145.0
74.00	15465.0
75.00	42296.0
76.00	3498.0
76.90	509.0
78.00	431.0
78.90	4814.0
79.90	1101.0
80.90	4402.0
81.90	927.0
82.80	140.0
85.80	178.0
86.90	2897.0
87.90	3315.0
90.70	509.0
91.90	2633.0
93.00	3971.0
94.00	10009.0
95.00	73360.0
96.00	5367.0
97.00	243.0
99.90	119.0
103.80	531.0
104.80	233.0
105.80	544.0
106.90	145.0
109.90	184.0
110.80	202.0
111.80	115.0
112.80	127.0
115.80	343.0
116.90	635.0
117.80	442.0
118.80	588.0
126.80	130.0
127.70	365.0
128.70	139.0
129.80	365.0
130.80	198.0
134.90	176.0
136.20	110.0
136.80	154.0
139.00	130.0
139.70	156.0
140.80	928.0
141.80	227.0
142.90	1312.0
143.90	160.0
144.80	388.0
145.80	171.0
147.80	252.0
152.60	121.0
154.90	202.0
156.70	187.0
158.60	111.0
160.60	223.0

Instrument :
MSVOA_V
ClientSampleId :
BFB31

170.80	350.0
171.80	1078.0
173.90	55968.0
174.90	4352.0
175.90	53840.0
176.90	3492.0
177.90	128.0

Instrument :
MSVOA_V
ClientSampleId :
BFB31

m/z	Abundance
36.00	1078.0
37.00	5319.0
38.00	5182.0
39.00	2274.0
40.00	755.0
41.90	123.0
42.70	131.0
44.00	1507.0
45.00	1065.0
45.90	302.0
47.10	1222.0
48.00	714.0
49.00	4334.0
50.00	19424.0
51.00	6021.0
52.10	268.0
52.90	203.0
54.10	209.0
55.00	332.0
56.00	1891.0
57.00	3129.0
57.90	173.0
58.90	128.0
59.10	134.0
60.00	1130.0
61.00	4661.0
62.00	5220.0
63.00	4616.0
63.90	809.0
65.10	894.0
66.00	219.0
66.90	288.0
68.00	9847.0
69.00	9785.0
70.00	869.0
72.00	543.0
73.00	4109.0
74.00	16191.0
75.00	44008.0
76.00	3513.0
76.90	580.0
77.90	440.0
78.90	5024.0
79.90	1030.0
80.90	4421.0
81.90	1041.0
82.80	183.0
85.80	196.0
86.90	3076.0
87.90	3427.0
90.70	582.0
91.90	2621.0
93.00	4225.0
94.00	10366.0
95.00	77104.0
96.00	5614.0
97.00	248.0
99.90	125.0
103.00	151.0
103.80	579.0
104.80	198.0
105.90	583.0
106.90	154.0
109.90	129.0
110.70	193.0
111.80	134.0
112.70	140.0
114.80	130.0
115.80	408.0
116.90	768.0
117.80	391.0
118.80	509.0
126.80	113.0
127.80	382.0
128.70	146.0
129.80	355.0
130.70	162.0
134.80	179.0
136.80	148.0
139.00	145.0
139.80	162.0
140.80	1144.0
141.80	273.0
142.90	1431.0
144.00	184.0
144.80	444.0
145.80	202.0
147.80	195.0
149.70	121.0
154.80	236.0
156.80	213.0
158.60	169.0

Instrument :
MSVOA_V
ClientSampleId :
BFB31

160.60	212.0
162.60	124.0
171.00	313.0
171.90	1342.0
173.90	59952.0
174.90	4924.0
175.90	58480.0
176.90	3657.0
177.90	127.0

Instrument :
MSVOA_V
ClientSampleId :
BFB31

m/z	Abundance
36.00	1005.0
37.00	5019.0
38.00	5009.0
39.00	2161.0
39.90	757.0
41.90	177.0
42.60	114.0
44.00	1350.0
45.00	958.0
45.90	284.0
47.10	1225.0
48.00	610.0
49.00	4054.0
50.00	18312.0
51.00	5470.0
52.10	253.0
52.90	210.0
54.00	192.0
55.00	305.0
56.00	1696.0
57.00	2830.0
57.90	166.0
58.80	133.0
60.00	1021.0
61.00	4696.0
62.00	5081.0
63.00	4247.0
64.00	825.0
65.10	862.0
66.00	165.0
66.90	288.0
68.00	9206.0
69.00	9303.0
70.00	776.0
72.00	555.0
73.00	3809.0
74.00	15286.0
75.00	41776.0
76.00	3310.0
77.00	605.0
77.90	369.0
78.90	4624.0
79.90	983.0
80.90	3974.0
81.90	1011.0
82.80	193.0
85.80	186.0
86.90	3102.0
87.90	3124.0
90.70	554.0
91.90	2353.0
93.00	4098.0
94.00	9970.0
95.00	73360.0
96.00	5362.0
96.90	206.0
100.00	109.0
103.00	139.0
103.90	580.0
104.90	194.0
105.90	535.0
106.80	139.0
110.70	176.0
111.80	144.0
112.70	158.0
114.80	132.0
115.80	418.0
116.90	850.0
117.90	366.0
118.80	458.0
127.90	418.0
128.70	168.0
129.90	314.0
130.60	148.0
134.80	171.0
136.80	164.0
139.80	146.0
140.90	1188.0
141.70	242.0
142.90	1270.0
144.00	150.0
144.80	426.0
145.80	223.0
148.00	199.0
149.80	123.0
154.80	243.0
156.80	184.0
158.70	221.0
160.70	150.0
162.50	128.0
167.80	105.0
170.50	207.0

Instrument :
MSVOA_V
ClientSampleId :
BFB31

171.00	234.0
171.90	1410.0
173.90	58504.0
174.90	4983.0
175.90	56976.0
176.90	3392.0
177.80	133.0

Instrument :
MSVOA_V
ClientSampleId :
BFB31

m/z	Abundance
35.50	154.0
36.00	267.0
36.70	128.0
37.80	211.0
38.80	180.0
39.90	700.0
41.10	106.0
41.90	167.0
42.40	143.0
44.00	655.0
45.20	215.0
45.90	125.0
46.50	146.0
47.90	110.0
48.80	138.0
49.80	156.0
51.00	109.0
52.00	113.0
52.60	121.0
53.90	101.0
54.30	125.0
55.70	121.0
58.30	101.0
63.00	136.0
64.90	105.0
66.80	151.0
69.20	121.0
69.80	103.0
70.20	109.0
75.60	104.0
77.00	132.0
96.00	148.0
98.70	108.0
116.00	102.0
132.20	105.0

Instrument :
MSVOA_V
ClientSampleId :
BFB31