

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090618\
 Data File : VV007452.D
 Acq On : 07 Sep 2018 05:32
 Operator : SY/MD
 Sample : J4751-10
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Sep 07 07:39:46 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Sep 07 03:09:50 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	531280	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	529252	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	192776	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	170437	44.91	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	89.82%
7) Chloroethane-d5	1.56	69	129773	52.20	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	104.40%
11) 1,1-Dichloroethene-d2	2.13	63	225742	33.77	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	67.54%
21) 2-Butanone-d5	3.96	46	156299	50.64	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	50.64%
24) Chloroform-d	4.41	84	337436	42.99	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	85.98%
26) 1,2-Dichloroethane-d4	5.09	65	214538	45.30	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.60%
32) Benzene-d6	5.10	84	688137	43.14	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	86.28%
36) 1,2-Dichloropropane-d6	6.12	67	227254	42.51	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	85.02%
41) Toluene-d8	7.36	98	554117	40.35	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	80.70%
43) trans-1,3-Dichloropropene-	7.67	79	84728	37.21	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	74.42%
47) 2-Hexanone-d5	8.14	63	141410	67.48	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	67.48%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	306095	41.92	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	83.84%
64) 1,2-Dichlorobenzene-d4	11.68	152	202904	48.97	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	97.94%


Target Compounds					Ovalue
59) 1,2,3-Trichloropropane	11.30	75	21758	3.932 ug/L	# 88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV090618\
Data File : VV007452.D
Acq On : 07 Sep 2018 05:32
Operator : SY/MD
Sample : J4751-10
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Sep 07 07:39:46 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Sep 07 03:09:50 2018
Response via : Initial Calibration

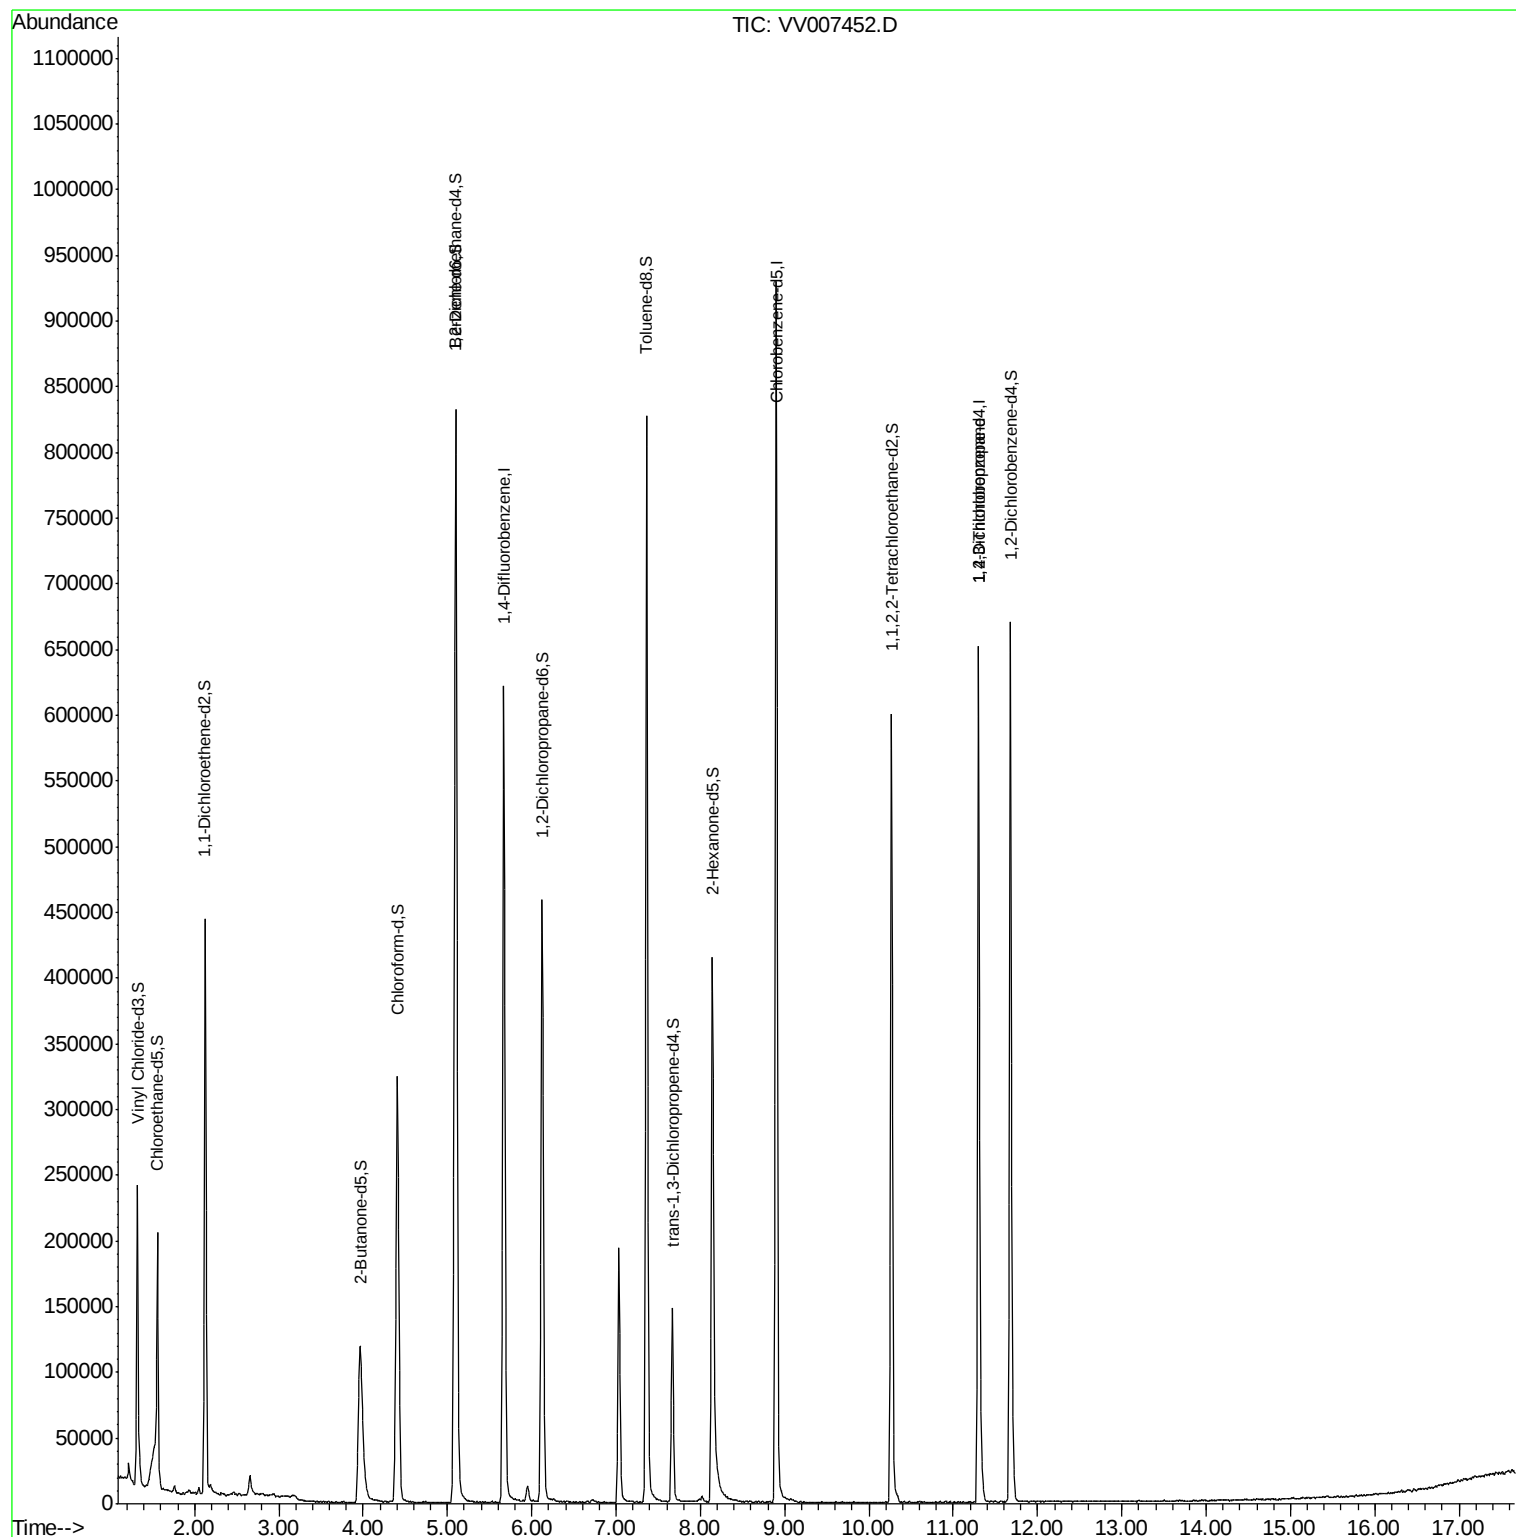

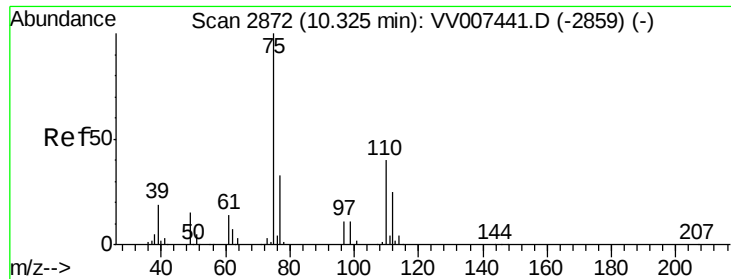

#59

1,2,3-Trichloropropane

Concen: 3.932 ug/L

RT: 11.30 min Scan# 3175

Delta R.T. 0.97 min

Lab File: VV007452.D

Acq: 07 Sep 2018 05:32

Instrument :

MSVOA_V

ClientSampleId :

Tot Ion: 75 Resp: 21758

Ion Ratio Lower Upper

75 100

77 38.7 25.5 38.3#

