

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090618\
 Data File : VV007420.D
 Acq On : 06 Sep 2018 15:09
 Operator : SY/MD
 Sample : VV0906WBL01
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK76

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.322	64	72	87	rVB	234079	258698	13.28%	1.777%
2	1.579	145	152	170	rVB	198435	239446	12.29%	1.645%
3	2.132	314	324	335	rBV	414575	590732	30.32%	4.058%
4	3.495	746	748	753	rBV3	492	326	0.02%	0.002%
5	3.521	753	756	760	rVB2	639	525	0.03%	0.004%
6	3.814	844	847	852	rBV3	537	542	0.03%	0.004%
7	3.843	853	856	860	rBV3	380	281	0.01%	0.002%
8	3.888	867	870	873	rVB2	359	280	0.01%	0.002%
9	3.955	873	891	934	rBV2	155799	491258	25.22%	3.374%
10	4.280	989	992	995	rVB3	712	431	0.02%	0.003%
11	4.319	1001	1004	1006	rBV3	647	404	0.02%	0.003%
12	4.405	1012	1031	1062	rBV	322213	782076	40.14%	5.372%
13	4.663	1109	1111	1115	rVB2	642	319	0.02%	0.002%
14	4.692	1115	1120	1122	rBV3	583	512	0.03%	0.004%
15	4.711	1122	1126	1129	rBV3	654	580	0.03%	0.004%
16	4.823	1156	1161	1163	rBV2	606	422	0.02%	0.003%
17	4.942	1194	1198	1201	rBV4	327	282	0.01%	0.002%
18	5.016	1216	1221	1224	rBV3	313	270	0.01%	0.002%
19	5.097	1227	1246	1276	rBV2	825565	1948266	100.00%	13.382%
20	5.306	1307	1311	1312	rVB3	440	297	0.02%	0.002%
21	5.322	1313	1316	1320	rVB4	606	343	0.02%	0.002%
22	5.421	1344	1347	1353	rBV3	625	471	0.02%	0.003%
23	5.447	1353	1355	1359	rBV3	661	475	0.02%	0.003%
24	5.550	1385	1387	1391	rVB2	661	315	0.02%	0.002%
25	5.579	1391	1396	1402	rBV4	489	680	0.03%	0.005%
26	5.669	1402	1424	1458	rBV	635561	1276453	65.52%	8.768%
27	5.949	1499	1511	1526	rVB4	13946	28303	1.45%	0.194%
28	6.122	1549	1565	1597	rBV	449736	926484	47.55%	6.364%
29	6.444	1661	1665	1668	rBV3	518	362	0.02%	0.002%
30	6.470	1668	1673	1675	rBV3	580	477	0.02%	0.003%
31	6.566	1701	1703	1707	rVV3	907	600	0.03%	0.004%
32	6.650	1722	1729	1730	rBV4	1128	1167	0.06%	0.008%
33	6.714	1743	1749	1750	rBV5	561	517	0.03%	0.004%
34	6.765	1763	1765	1768	rVB2	481	278	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090618\
 Data File : VV007420.D
 Acq On : 06 Sep 2018 15:09
 Operator : SY/MD
 Sample : VV0906WBL01
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK76

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

35	6.820	1779	1782	1785	rVB3	590	345	0.02%	0.002%
36	6.843	1785	1789	1790	rBV3	428	292	0.01%	0.002%
37	6.875	1795	1799	1801	rBV2	476	330	0.02%	0.002%
38	6.907	1806	1809	1812	rVB4	456	358	0.02%	0.002%
39	7.032	1833	1848	1869	rBV2	213010	390206	20.03%	2.680%
40	7.277	1918	1924	1932	rBV8	1287	2030	0.10%	0.014%
41	7.363	1936	1951	1987	rBV	813947	1442183	74.02%	9.906%
42	7.666	2032	2045	2068	rBV	158819	278857	14.31%	1.915%
43	7.958	2133	2136	2138	rBV2	749	477	0.02%	0.003%
44	7.987	2138	2145	2148	rBV3	1829	2147	0.11%	0.015%
45	8.055	2163	2166	2171	rVB3	630	489	0.03%	0.003%
46	8.142	2180	2193	2237	rBV2	434221	956561	49.10%	6.570%
47	8.640	2347	2348	2349	rBV	1032	320	0.02%	0.002%
48	8.650	2349	2351	2352	rVV2	682	344	0.02%	0.002%
49	8.775	2384	2390	2393	rBV2	347	345	0.02%	0.002%
50	8.900	2413	2429	2460	rBV	923649	1542613	79.18%	10.596%
51	9.183	2511	2517	2526	rVB6	2288	3247	0.17%	0.022%
52	9.241	2531	2535	2539	rVV4	565	434	0.02%	0.003%
53	9.273	2539	2545	2548	rBV2	469	402	0.02%	0.003%
54	9.418	2586	2590	2593	rVB3	376	281	0.01%	0.002%
55	9.453	2595	2601	2602	rBV3	370	312	0.02%	0.002%
56	9.518	2617	2621	2625	rVB4	487	351	0.02%	0.002%
57	9.560	2631	2634	2638	rVB2	708	408	0.02%	0.003%
58	9.598	2638	2646	2647	rBV4	1760	1711	0.09%	0.012%
59	9.672	2666	2669	2671	rBV	407	294	0.02%	0.002%
60	9.707	2677	2680	2683	rVB3	434	281	0.01%	0.002%
61	9.743	2688	2691	2696	rVB3	434	346	0.02%	0.002%
62	9.826	2714	2717	2721	rBV2	435	365	0.02%	0.003%
63	9.913	2741	2744	2749	rBV4	488	400	0.02%	0.003%
64	9.978	2760	2764	2773	rVB5	874	1274	0.07%	0.009%
65	10.093	2797	2800	2802	rBV2	463	322	0.02%	0.002%
66	10.125	2807	2810	2815	rVV2	452	403	0.02%	0.003%
67	10.267	2841	2854	2888	rBV	601627	988503	50.74%	6.790%
68	10.431	2896	2905	2912	rBV5	1118	1887	0.10%	0.013%
69	10.469	2915	2917	2920	rVB	494	270	0.01%	0.002%
70	10.550	2940	2942	2948	rBV2	501	496	0.03%	0.003%
71	10.621	2961	2964	2966	rBV2	575	371	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090618\
 Data File : VV007420.D
 Acq On : 06 Sep 2018 15:09
 Operator : SY/MD
 Sample : VV0906WBL01
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK76

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

72	10.733	2997	2999	3005	rVB3	500	365	0.02%	0.003%
73	10.772	3009	3011	3015	rVB3	537	430	0.02%	0.003%
74	10.820	3022	3026	3031	rVB3	674	664	0.03%	0.005%
75	10.904	3048	3052	3055	rBV4	507	482	0.02%	0.003%
76	10.965	3067	3071	3073	rBV	396	276	0.01%	0.002%
77	11.016	3084	3087	3090	rBV3	462	314	0.02%	0.002%
78	11.032	3090	3092	3099	rVB4	373	343	0.02%	0.002%
79	11.116	3113	3118	3121	rBV2	283	292	0.01%	0.002%
80	11.190	3137	3141	3143	rBV2	355	281	0.01%	0.002%
81	11.235	3147	3155	3162	rBV3	3126	4300	0.22%	0.030%
82	11.299	3162	3175	3201	rBV	678955	1157057	59.39%	7.947%
83	11.421	3211	3213	3216	rVB2	726	422	0.02%	0.003%
84	11.566	3256	3258	3261	rBV	364	279	0.01%	0.002%
85	11.678	3279	3293	3318	rBV	690179	1181885	60.66%	8.118%
86	11.781	3322	3325	3329	rBV2	499	451	0.02%	0.003%
87	11.891	3356	3359	3363	rBV3	491	327	0.02%	0.002%
88	12.231	3463	3465	3468	rBV2	437	308	0.02%	0.002%
89	12.408	3517	3520	3523	rBV2	317	268	0.01%	0.002%
90	12.485	3542	3544	3548	rBV2	399	365	0.02%	0.003%
91	12.540	3558	3561	3565	rVB3	604	477	0.02%	0.003%
92	12.701	3603	3611	3622	rVB5	3157	5187	0.27%	0.036%
93	12.932	3680	3683	3687	rBV3	830	678	0.03%	0.005%
94	12.984	3696	3699	3700	rBV3	499	316	0.02%	0.002%
95	13.321	3796	3804	3813	rBV6	4566	7217	0.37%	0.050%
96	13.418	3832	3834	3838	rVB3	780	496	0.03%	0.003%
97	13.460	3845	3847	3849	rBV2	621	363	0.02%	0.002%
98	13.563	3870	3879	3891	rBV2	7874	14119	0.72%	0.097%
99	13.804	3948	3954	3963	rVB5	4840	7347	0.38%	0.050%
100	14.312	4109	4112	4113	rBV3	717	396	0.02%	0.003%


Sum of corrected areas: 14558832

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV090618\
Data File : VV007420.D
Acq On : 06 Sep 2018 15:09
Operator : SY/MD
Sample : VV0906WBL01
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK76

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

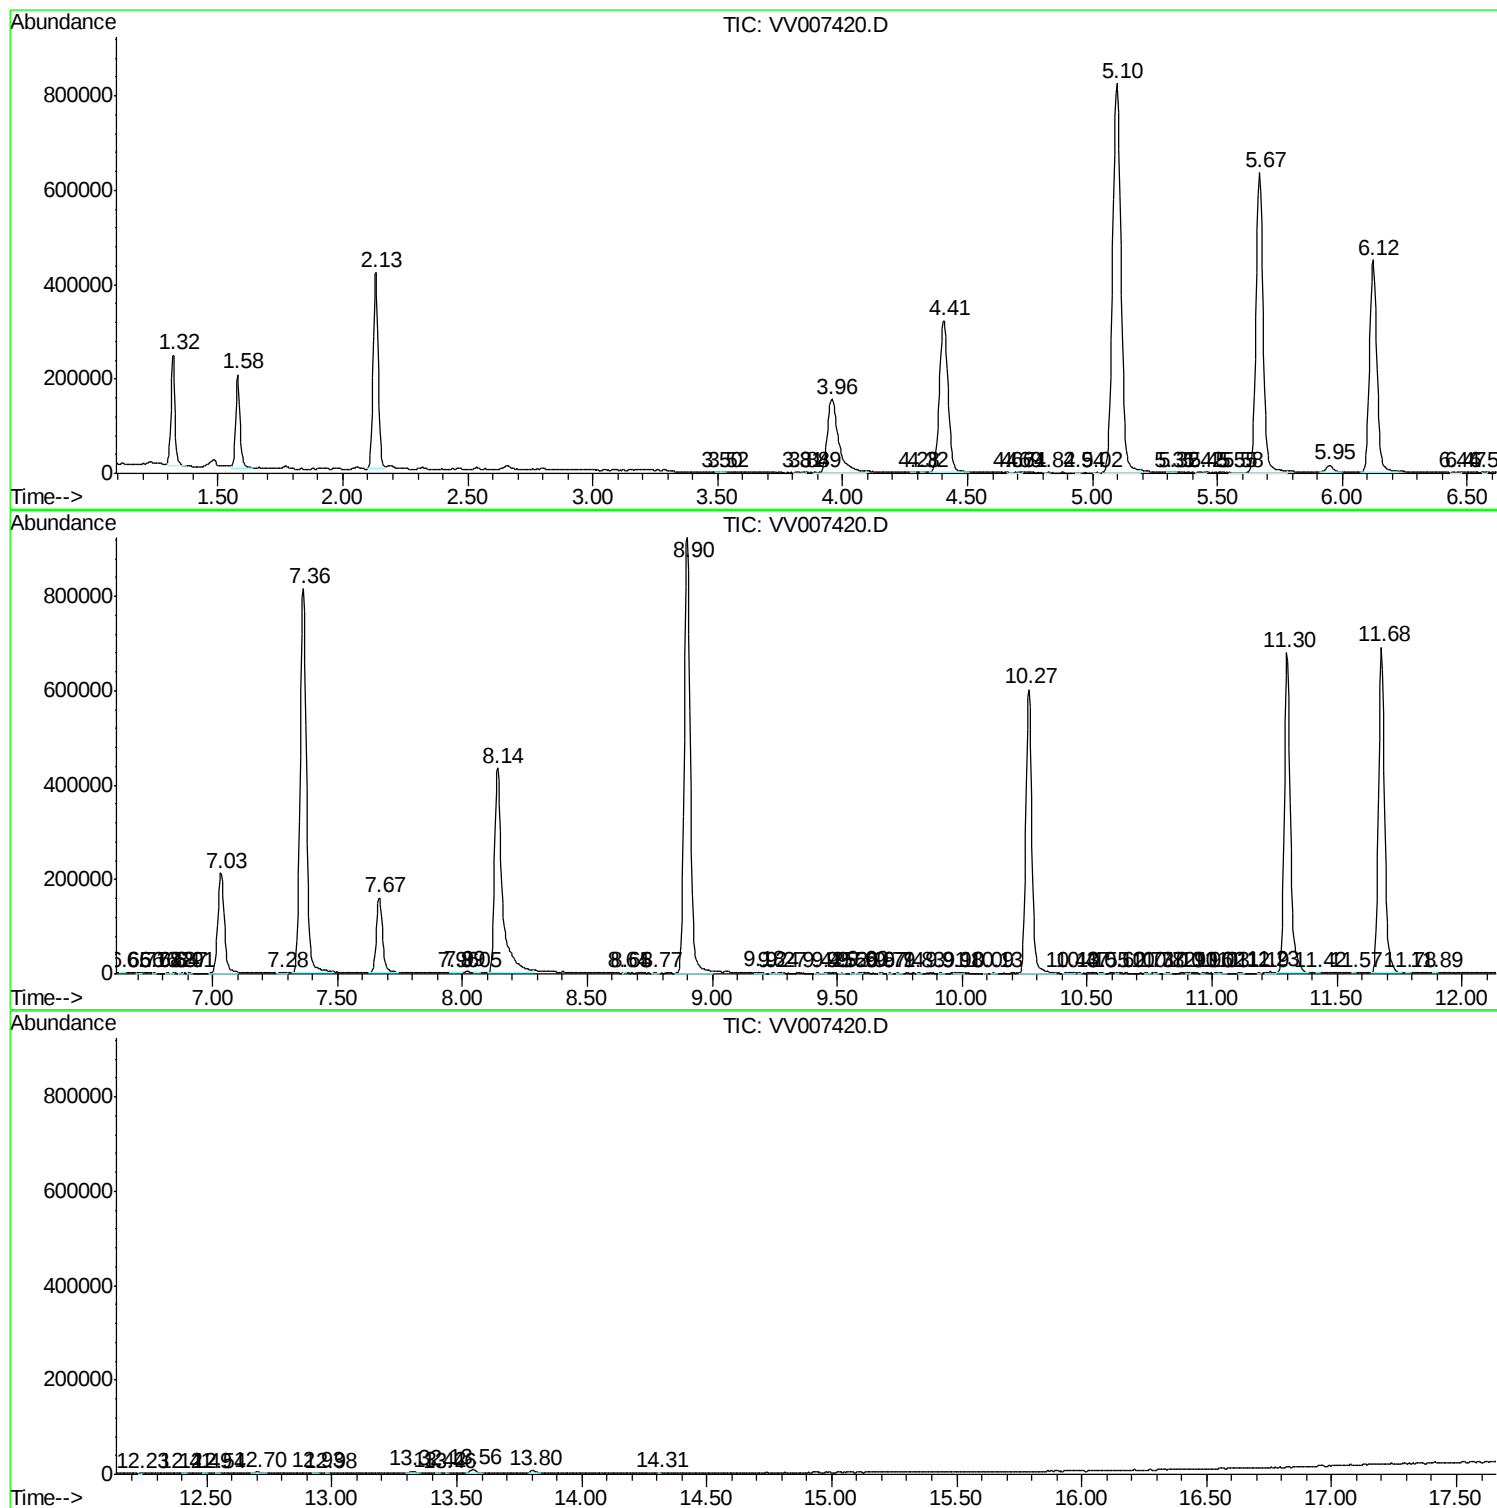

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV090618\
Data File : VV007420.D
Acq On : 06 Sep 2018 15:09
Operator : SY/MD
Sample : VV0906WBL01
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK76

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV090618\
Data File : VV007420.D
Acq On : 06 Sep 2018 15:09
Operator : SY/MD
Sample : VV0906WBL01
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK76

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc