

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090618\
 Data File : VV007422.D
 Acq On : 06 Sep 2018 16:11
 Operator : SY/MD
 Sample : J4719-01
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGD7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	63	71	88	rVB	216236	258370	13.68%	1.795%
2	1.560	140	146	162	rVB	183688	229459	12.15%	1.594%
3	2.126	312	322	334	rBV	405900	568574	30.09%	3.950%
4	2.193	335	343	353	rVB	84762	126860	6.71%	0.881%
5	3.489	743	746	749	rBV2	577	352	0.02%	0.002%
6	3.537	756	761	764	rBV3	1051	797	0.04%	0.006%
7	3.595	777	779	785	rVB2	532	477	0.03%	0.003%
8	3.630	785	790	793	rBV	697	598	0.03%	0.004%
9	3.727	816	820	824	rVB2	296	287	0.02%	0.002%
10	3.830	849	852	857	rVB4	699	613	0.03%	0.004%
11	3.859	857	861	863	rBV	399	278	0.01%	0.002%
12	3.962	876	893	936	rBV3	157940	490457	25.96%	3.407%
13	4.289	992	995	1000	rBV3	709	736	0.04%	0.005%
14	4.405	1014	1031	1060	rBV	324989	779125	41.24%	5.412%
15	4.640	1100	1104	1107	rVB3	395	314	0.02%	0.002%
16	4.714	1120	1127	1128	rBV6	1045	1040	0.06%	0.007%
17	4.778	1145	1147	1152	rBV3	514	377	0.02%	0.003%
18	5.096	1227	1246	1286	rBV2	803334	1889284	100.00%	13.124%
19	5.347	1320	1324	1326	rBV2	616	462	0.02%	0.003%
20	5.402	1339	1341	1344	rVB3	669	336	0.02%	0.002%
21	5.421	1344	1347	1349	rBV2	603	363	0.02%	0.003%
22	5.450	1353	1356	1360	rVB4	636	465	0.02%	0.003%
23	5.466	1360	1361	1369	rVB3	411	332	0.02%	0.002%
24	5.511	1371	1375	1376	rBV2	377	276	0.01%	0.002%
25	5.579	1391	1396	1398	rBV2	595	547	0.03%	0.004%
26	5.669	1407	1424	1456	rBV	622932	1246593	65.98%	8.659%
27	5.958	1504	1514	1525	rVB7	11169	24733	1.31%	0.172%
28	6.122	1550	1565	1586	rBV	440807	892433	47.24%	6.199%
29	6.402	1649	1652	1657	rVB3	856	784	0.04%	0.005%
30	6.563	1700	1702	1707	rBV3	357	345	0.02%	0.002%
31	6.614	1715	1718	1720	rBV3	591	414	0.02%	0.003%
32	6.643	1721	1727	1739	rVB6	2529	4768	0.25%	0.033%
33	6.720	1747	1751	1760	rVV4	2120	2947	0.16%	0.020%
34	6.788	1770	1772	1776	rVB4	532	340	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090618\
 Data File : VV007422.D
 Acq On : 06 Sep 2018 16:11
 Operator : SY/MD
 Sample : J4719-01
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGD7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

35	6.836	1784	1787	1789	rBV3	512	306	0.02%	0.002%
36	6.875	1797	1799	1803	rBV	590	335	0.02%	0.002%
37	6.936	1816	1818	1821	rBV3	505	343	0.02%	0.002%
38	7.035	1835	1849	1863	rBV	210264	369996	19.58%	2.570%
39	7.164	1885	1889	1890	rBV3	629	488	0.03%	0.003%
40	7.293	1924	1929	1936	rVB4	1027	1265	0.07%	0.009%
41	7.363	1936	1951	1978	rBV	796846	1377107	72.89%	9.566%
42	7.592	2020	2022	2027	rVB5	667	382	0.02%	0.003%
43	7.669	2034	2046	2064	rBV	155476	264153	13.98%	1.835%
44	7.820	2090	2093	2100	rVV3	695	545	0.03%	0.004%
45	7.987	2136	2145	2148	rBV2	6016	8370	0.44%	0.058%
46	8.022	2149	2156	2167	rVB3	19067	32100	1.70%	0.223%
47	8.071	2167	2171	2174	rBV2	462	418	0.02%	0.003%
48	8.141	2179	2193	2238	rBV2	442905	927696	49.10%	6.444%
49	8.415	2271	2278	2294	rVB4	6887	14426	0.76%	0.100%
50	8.611	2337	2339	2342	rVB2	701	297	0.02%	0.002%
51	8.646	2348	2350	2354	rBV3	575	438	0.02%	0.003%
52	8.739	2377	2379	2381	rVB2	661	282	0.01%	0.002%
53	8.900	2413	2429	2459	rBV	935960	1540710	81.55%	10.703%
54	9.190	2510	2519	2521	rBV5	1334	1516	0.08%	0.011%
55	9.247	2529	2537	2538	rBV5	2157	2464	0.13%	0.017%
56	9.389	2577	2581	2584	rBV3	483	365	0.02%	0.003%
57	9.463	2602	2604	2607	rVV2	468	299	0.02%	0.002%
58	9.479	2607	2609	2613	rVB2	860	494	0.03%	0.003%
59	9.501	2613	2616	2619	rBV2	416	355	0.02%	0.002%
60	9.559	2632	2634	2638	rVB2	552	339	0.02%	0.002%
61	9.601	2641	2647	2650	rBV5	879	977	0.05%	0.007%
62	9.707	2673	2680	2683	rVB3	403	495	0.03%	0.003%
63	9.739	2686	2690	2691	rBV	536	373	0.02%	0.003%
64	9.862	2726	2728	2730	rVB2	580	282	0.01%	0.002%
65	9.891	2733	2737	2740	rBV3	303	278	0.01%	0.002%
66	9.939	2749	2752	2754	rBV2	484	278	0.01%	0.002%
67	9.971	2760	2762	2764	rBV	506	290	0.02%	0.002%
68	9.984	2764	2766	2772	rVB3	917	655	0.03%	0.005%
69	10.125	2807	2810	2814	rBV3	675	532	0.03%	0.004%
70	10.267	2842	2854	2889	rBV	602765	979107	51.82%	6.801%
71	10.427	2894	2904	2917	rBV2	5834	9693	0.51%	0.067%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090618\
 Data File : VV007422.D
 Acq On : 06 Sep 2018 16:11
 Operator : SY/MD
 Sample : J4719-01
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGD7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

72	10.511	2926	2930	2932	rVB	426	273	0.01%	0.002%
73	10.862	3037	3039	3041	rBV	562	345	0.02%	0.002%
74	10.887	3044	3047	3048	rVV2	568	318	0.02%	0.002%
75	10.900	3049	3051	3058	rVB5	645	541	0.03%	0.004%
76	11.119	3114	3119	3121	rBV3	461	457	0.02%	0.003%
77	11.231	3149	3154	3160	rVB5	1154	1440	0.08%	0.010%
78	11.302	3162	3176	3205	rBV	686325	1160122	61.41%	8.059%
79	11.402	3205	3207	3209	rBV3	796	481	0.03%	0.003%
80	11.546	3248	3252	3254	rBV3	474	343	0.02%	0.002%
81	11.588	3259	3265	3267	rBV5	938	695	0.04%	0.005%
82	11.678	3280	3293	3318	rBV	679812	1158374	61.31%	8.047%
83	11.858	3344	3349	3351	rBV4	423	397	0.02%	0.003%
84	11.929	3368	3371	3375	rVB4	498	404	0.02%	0.003%
85	11.952	3375	3378	3381	rBV3	439	290	0.02%	0.002%
86	12.009	3393	3396	3398	rBV3	643	389	0.02%	0.003%
87	12.054	3407	3410	3415	rVB2	483	328	0.02%	0.002%
88	12.746	3622	3625	3628	rBV4	576	326	0.02%	0.002%
89	12.845	3653	3656	3659	rBV	596	449	0.02%	0.003%
90	12.926	3678	3681	3684	rBV4	951	736	0.04%	0.005%
91	13.206	3764	3768	3771	rVB3	657	523	0.03%	0.004%
92	13.225	3771	3774	3776	rBV4	757	577	0.03%	0.004%
93	13.427	3833	3837	3839	rBV2	813	681	0.04%	0.005%
94	13.469	3847	3850	3852	rBV2	546	298	0.02%	0.002%
95	13.559	3876	3878	3883	rVB5	1403	963	0.05%	0.007%
96	13.620	3894	3897	3900	rVB4	840	573	0.03%	0.004%
97	13.640	3900	3903	3908	rBV7	752	830	0.04%	0.006%
98	13.906	3984	3986	3988	rBV3	691	343	0.02%	0.002%
99	14.501	4169	4171	4177	rBV4	1009	901	0.05%	0.006%
100	14.826	4269	4272	4273	rBV2	1335	784	0.04%	0.005%


Sum of corrected areas: 14395766

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV090618\
Data File : VV007422.D
Acq On : 06 Sep 2018 16:11
Operator : SY/MD
Sample : J4719-01
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGD7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

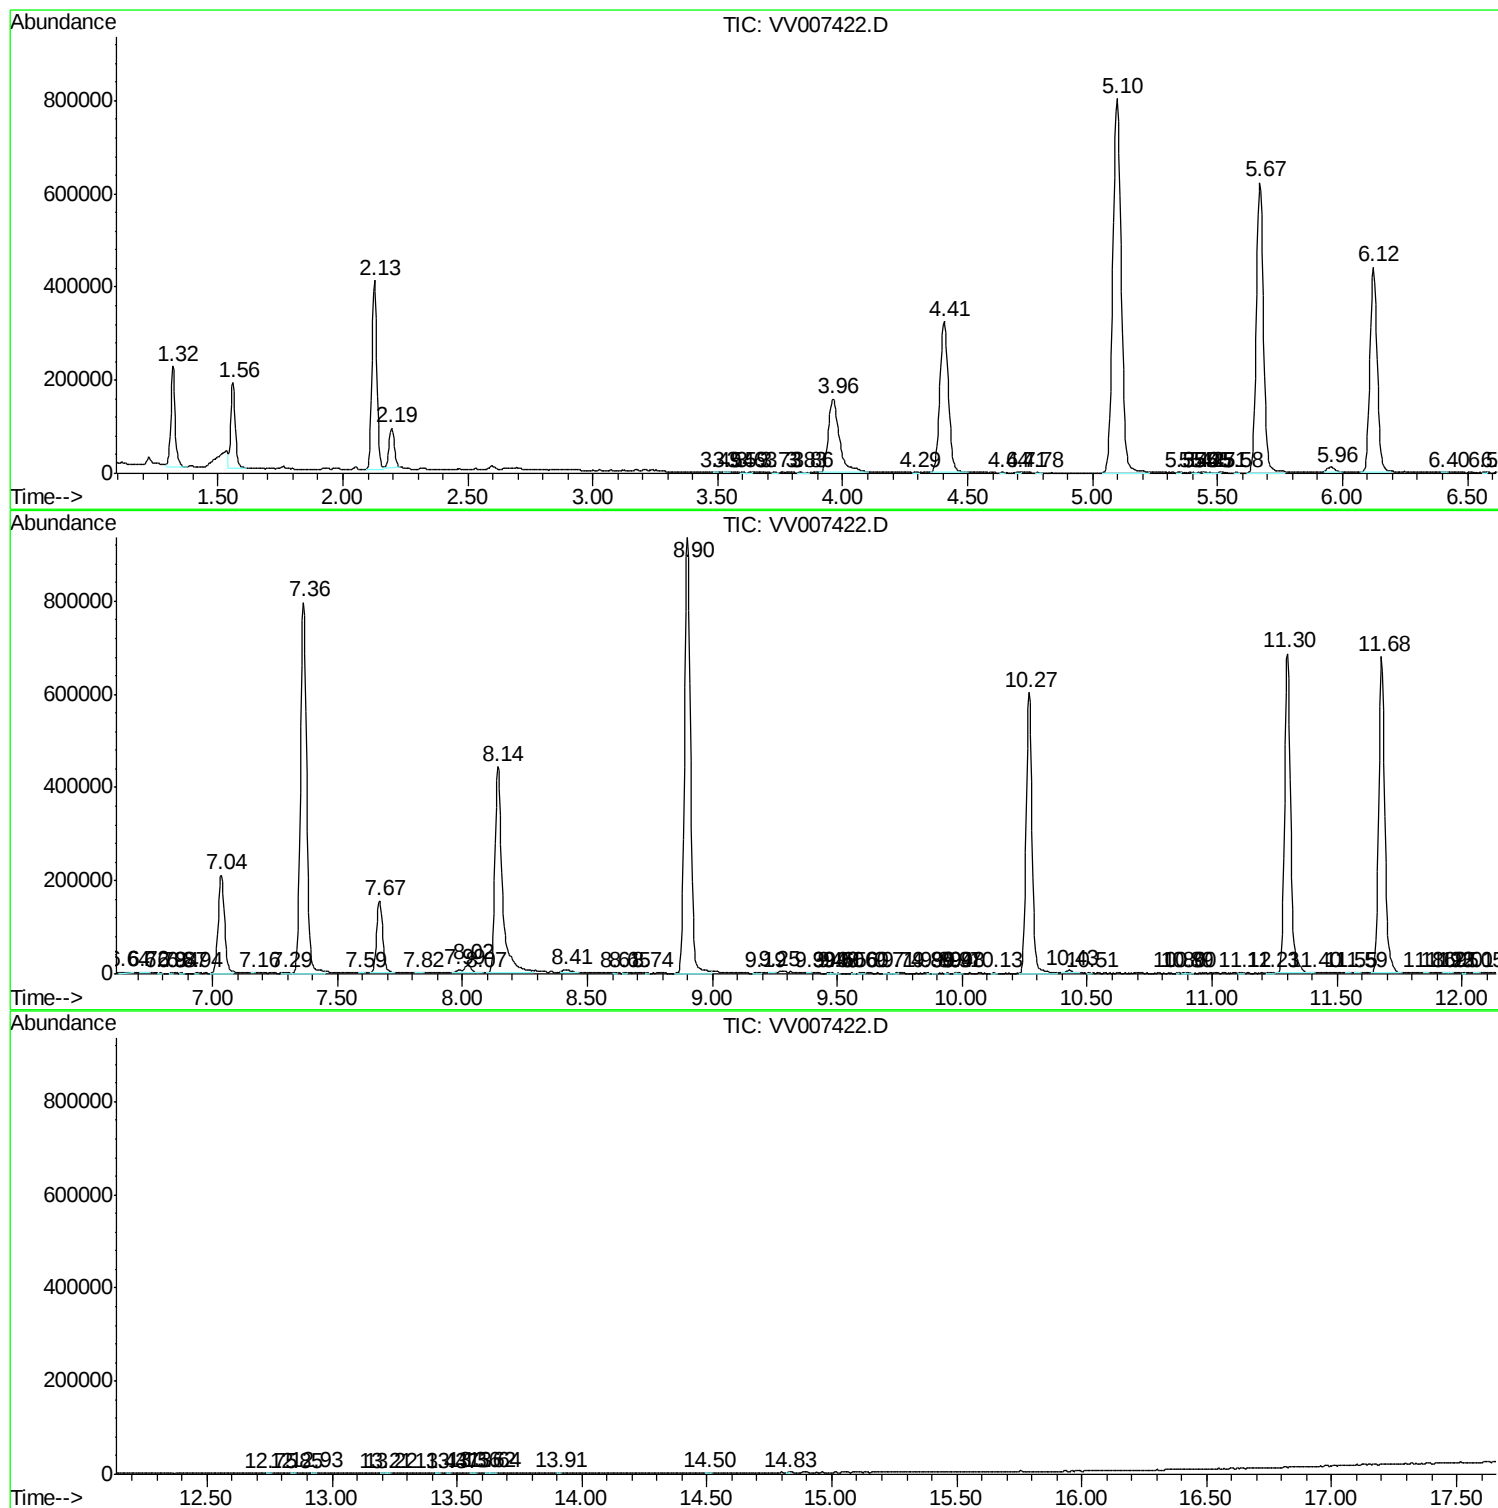

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV090618\
Data File : VV007422.D
Acq On : 06 Sep 2018 16:11
Operator : SY/MD
Sample : J4719-01
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGD7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV090618\
Data File : VV007422.D
Acq On : 06 Sep 2018 16:11
Operator : SY/MD
Sample : J4719-01
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGD7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc