

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090618\
 Data File : VV007426.D
 Acq On : 06 Sep 2018 17:52
 Operator : SY/MD
 Sample : J4719-06
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGE2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.322	64	72	90	rVB	221159	275727	14.22%	1.944%
2	1.560	141	146	162	rVB	187923	231258	11.92%	1.631%
3	2.126	312	322	335	rBV	433919	614868	31.70%	4.336%
4	3.434	726	729	733	rVB	450	343	0.02%	0.002%
5	3.576	770	773	777	rVB2	788	524	0.03%	0.004%
6	3.595	777	779	782	rBV2	489	283	0.01%	0.002%
7	3.679	803	805	811	rVB2	469	510	0.03%	0.004%
8	3.714	811	816	821	rBV3	500	504	0.03%	0.004%
9	3.823	845	850	853	rVB3	410	329	0.02%	0.002%
10	3.962	874	893	924	rBV3	134465	418562	21.58%	2.951%
11	4.296	994	997	999	rBV	562	355	0.02%	0.003%
12	4.405	1014	1031	1056	rBV	321862	772697	39.84%	5.448%
13	4.605	1091	1093	1097	rVB	465	333	0.02%	0.002%
14	4.634	1097	1102	1104	rBV2	477	419	0.02%	0.003%
15	4.682	1114	1117	1118	rBV2	817	455	0.02%	0.003%
16	4.724	1118	1130	1140	rVV10	5005	10615	0.55%	0.075%
17	4.820	1156	1160	1162	rBV2	433	322	0.02%	0.002%
18	4.878	1173	1178	1181	rBV2	328	282	0.01%	0.002%
19	4.926	1189	1193	1197	rVB4	514	434	0.02%	0.003%
20	4.975	1204	1208	1212	rVB3	273	269	0.01%	0.002%
21	5.100	1226	1247	1286	rBV2	822440	1939685	100.00%	13.677%
22	5.331	1316	1319	1323	rVB4	619	443	0.02%	0.003%
23	5.354	1323	1326	1330	rVB2	358	289	0.01%	0.002%
24	5.373	1330	1332	1334	rBV2	490	270	0.01%	0.002%
25	5.463	1351	1360	1365	rBV5	617	868	0.04%	0.006%
26	5.579	1392	1396	1398	rBV2	493	272	0.01%	0.002%
27	5.598	1398	1402	1404	rVB3	455	274	0.01%	0.002%
28	5.669	1408	1424	1451	rBV	631761	1248667	64.37%	8.805%
29	5.881	1486	1490	1493	rBV5	944	659	0.03%	0.005%
30	5.949	1501	1511	1522	rBV5	9937	19123	0.99%	0.135%
31	6.071	1546	1549	1550	rBV2	633	393	0.02%	0.003%
32	6.126	1551	1566	1592	rVV	442874	895824	46.18%	6.317%
33	6.344	1630	1634	1636	rBV3	534	342	0.02%	0.002%
34	6.483	1674	1677	1681	rBV2	343	270	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090618\
 Data File : VV007426.D
 Acq On : 06 Sep 2018 17:52
 Operator : SY/MD
 Sample : J4719-06
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGE2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

35	6.502	1681	1683	1690	rVB2	699	771	0.04%	0.005%
36	6.537	1690	1694	1698	rBV3	613	643	0.03%	0.005%
37	6.569	1701	1704	1706	rBV2	520	347	0.02%	0.002%
38	6.598	1709	1713	1719	rVB3	605	660	0.03%	0.005%
39	6.627	1719	1722	1724	rBV	492	295	0.02%	0.002%
40	6.717	1741	1750	1752	rBV5	2018	2157	0.11%	0.015%
41	6.804	1776	1777	1781	rVB2	658	325	0.02%	0.002%
42	6.820	1781	1782	1788	rVB4	536	416	0.02%	0.003%
43	6.868	1794	1797	1799	rBV	416	336	0.02%	0.002%
44	6.926	1813	1815	1820	rVB3	661	496	0.03%	0.003%
45	7.036	1835	1849	1876	rBV	214284	382978	19.74%	2.700%
46	7.158	1884	1887	1891	rBV5	635	564	0.03%	0.004%
47	7.209	1899	1903	1905	rBV3	478	297	0.02%	0.002%
48	7.235	1908	1911	1914	rVB3	451	266	0.01%	0.002%
49	7.296	1927	1930	1932	rBV2	401	278	0.01%	0.002%
50	7.364	1936	1951	1968	rBV	816096	1410547	72.72%	9.946%
51	7.585	2017	2020	2023	rBV3	729	576	0.03%	0.004%
52	7.669	2033	2046	2066	rBV	160613	269843	13.91%	1.903%
53	7.778	2076	2080	2083	rBV4	689	532	0.03%	0.004%
54	7.849	2100	2102	2106	rBV3	596	458	0.02%	0.003%
55	7.900	2115	2118	2120	rBV3	519	391	0.02%	0.003%
56	7.984	2138	2144	2149	rBV4	3021	4241	0.22%	0.030%
57	8.142	2181	2193	2225	rBV2	413466	843689	43.50%	5.949%
58	8.547	2315	2319	2323	rVB3	497	536	0.03%	0.004%
59	8.627	2339	2344	2346	rBV3	594	518	0.03%	0.004%
60	8.656	2348	2353	2356	rBV4	707	619	0.03%	0.004%
61	8.708	2365	2369	2370	rBV2	649	323	0.02%	0.002%
62	8.794	2392	2396	2398	rBV2	483	271	0.01%	0.002%
63	8.900	2414	2429	2452	rBV	944531	1543470	79.57%	10.883%
64	9.190	2514	2519	2523	rVB6	765	704	0.04%	0.005%
65	9.238	2528	2534	2535	rBV3	2020	1725	0.09%	0.012%
66	9.495	2611	2614	2617	rBV3	526	421	0.02%	0.003%
67	9.569	2632	2637	2639	rVB2	307	295	0.02%	0.002%
68	9.589	2639	2643	2646	rBV2	562	563	0.03%	0.004%
69	9.730	2685	2687	2692	rBV2	330	276	0.01%	0.002%
70	9.855	2722	2726	2727	rBV3	402	289	0.01%	0.002%
71	9.913	2742	2744	2749	rVV3	391	340	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090618\
 Data File : VV007426.D
 Acq On : 06 Sep 2018 17:52
 Operator : SY/MD
 Sample : J4719-06
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGE2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

72	9.936	2749	2751	2755	rVB2	632	416	0.02%	0.003%
73	9.965	2755	2760	2763	rBV2	424	367	0.02%	0.003%
74	10.109	2802	2805	2809	rBV3	458	270	0.01%	0.002%
75	10.219	2833	2839	2840	rBV2	320	287	0.01%	0.002%
76	10.267	2841	2854	2891	rVV	580815	946922	48.82%	6.677%
77	10.425	2896	2903	2917	rVV3	2610	5197	0.27%	0.037%
78	10.476	2917	2919	2924	rVV3	370	334	0.02%	0.002%
79	10.502	2924	2927	2935	rVB3	490	465	0.02%	0.003%
80	10.566	2945	2947	2950	rBV2	453	303	0.02%	0.002%
81	10.617	2961	2963	2970	rVB2	749	637	0.03%	0.004%
82	10.688	2982	2985	2989	rBV2	594	494	0.03%	0.003%
83	10.846	3031	3034	3039	rVB3	418	378	0.02%	0.003%
84	10.891	3043	3048	3049	rBV3	439	384	0.02%	0.003%
85	11.228	3149	3153	3156	rBV3	636	522	0.03%	0.004%
86	11.299	3163	3175	3203	rBV	685109	1158093	59.71%	8.166%
87	11.450	3218	3222	3225	rVB2	620	502	0.03%	0.004%
88	11.678	3280	3293	3318	rBV	669010	1151972	59.39%	8.123%
89	11.791	3326	3328	3330	rBV4	521	268	0.01%	0.002%
90	11.977	3382	3386	3392	rBV5	708	728	0.04%	0.005%
91	12.106	3423	3426	3428	rBV2	422	310	0.02%	0.002%
92	12.141	3434	3437	3439	rBV2	420	280	0.01%	0.002%
93	12.463	3532	3537	3542	rBV4	621	671	0.03%	0.005%
94	12.698	3608	3610	3611	rBV	781	319	0.02%	0.002%
95	12.939	3680	3685	3690	rBV7	1084	1291	0.07%	0.009%
96	13.215	3769	3771	3775	rBV2	470	307	0.02%	0.002%
97	13.556	3874	3877	3880	rBV3	579	439	0.02%	0.003%
98	13.785	3946	3948	3951	rBV	645	329	0.02%	0.002%
99	13.990	4010	4012	4016	rVB2	806	450	0.02%	0.003%
100	14.855	4278	4281	4284	rBV2	1178	1048	0.05%	0.007%


Sum of corrected areas: 14181907

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV090618\
Data File : VV007426.D
Acq On : 06 Sep 2018 17:52
Operator : SY/MD
Sample : J4719-06
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGE2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

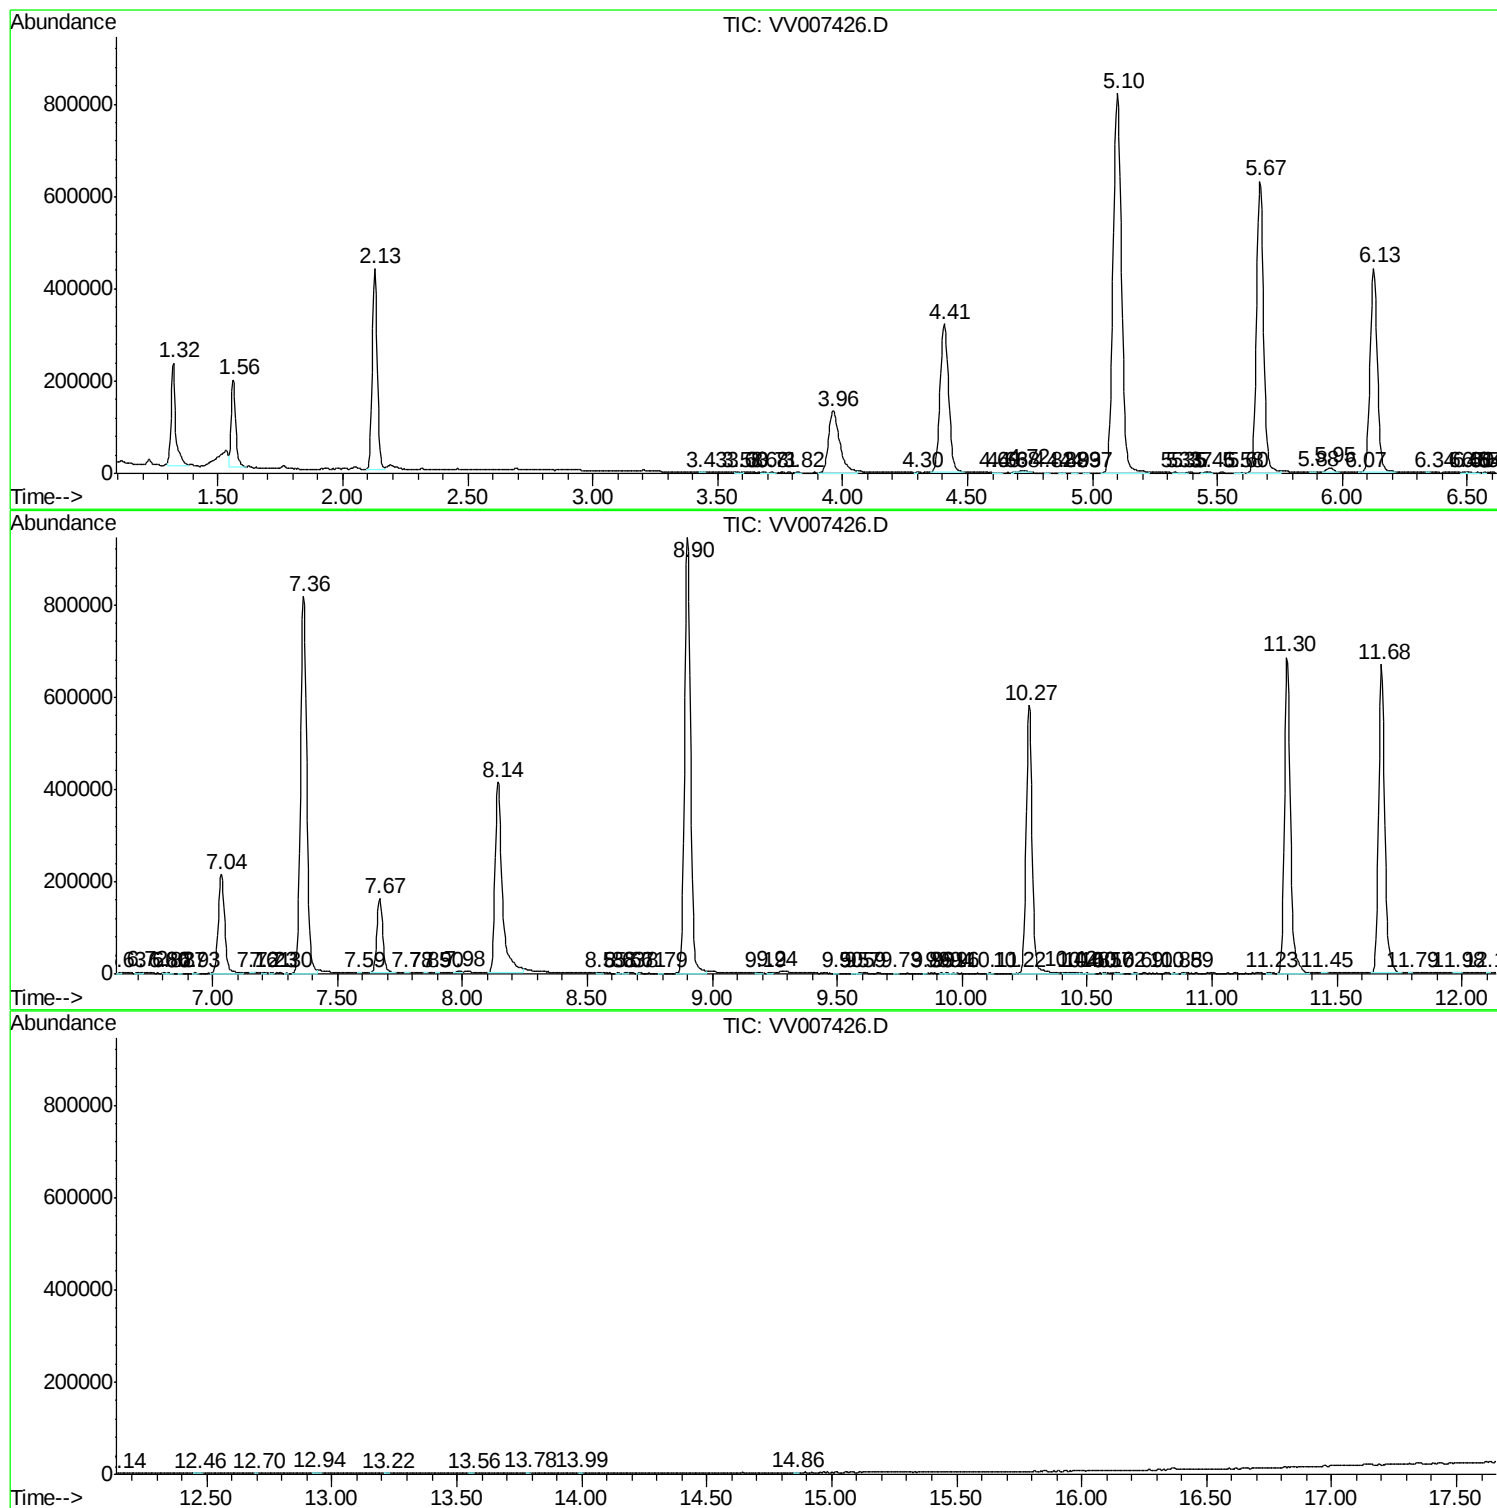

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV090618\
Data File : VV007426.D
Acq On : 06 Sep 2018 17:52
Operator : SY/MD
Sample : J4719-06
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGE2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV090618\
Data File : VV007426.D
Acq On : 06 Sep 2018 17:52
Operator : SY/MD
Sample : J4719-06
Misc : 5.0 mL/MSV0A_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
BEGE2

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc