

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090618\
 Data File : VV007429.D
 Acq On : 06 Sep 2018 19:07
 Operator : SY/MD
 Sample : J4719-10
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGE6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	63	71	89	rVB	247549	302474	15.48%	2.127%
2	1.560	140	146	162	rVB	195053	242049	12.38%	1.702%
3	2.126	312	322	334	rBV	434299	614068	31.42%	4.318%
4	3.614	782	785	788	rVB2	688	448	0.02%	0.003%
5	3.704	810	813	817	rVB3	396	304	0.02%	0.002%
6	3.727	817	820	823	rBV4	804	651	0.03%	0.005%
7	3.756	823	829	836	rVV7	1214	2087	0.11%	0.015%
8	3.807	842	845	848	rBV2	805	609	0.03%	0.004%
9	3.891	865	871	873	rBV4	1392	1465	0.07%	0.010%
10	3.958	877	892	914	rBV2	136768	388324	19.87%	2.731%
11	4.293	994	996	999	rVB2	594	325	0.02%	0.002%
12	4.405	1012	1031	1059	rBV	322370	768623	39.32%	5.405%
13	4.627	1098	1100	1104	rVB	520	426	0.02%	0.003%
14	4.650	1104	1107	1111	rVB3	652	472	0.02%	0.003%
15	4.724	1111	1130	1145	rBV4	14245	33338	1.71%	0.234%
16	4.782	1145	1148	1151	rBV3	542	448	0.02%	0.003%
17	4.904	1184	1186	1191	rBV3	364	290	0.01%	0.002%
18	5.100	1227	1247	1279	rBV2	811555	1954557	100.00%	13.744%
19	5.318	1312	1315	1319	rVB4	621	344	0.02%	0.002%
20	5.364	1325	1329	1330	rBV3	1446	1024	0.05%	0.007%
21	5.383	1330	1335	1338	rBV6	2347	2414	0.12%	0.017%
22	5.566	1382	1392	1395	rBV7	2216	3352	0.17%	0.024%
23	5.669	1409	1424	1444	rBV	637610	1236396	63.26%	8.694%
24	5.949	1503	1511	1526	rVB6	7704	15191	0.78%	0.107%
25	6.126	1551	1566	1589	rBV	443970	889826	45.53%	6.257%
26	6.476	1672	1675	1679	rBV3	630	682	0.03%	0.005%
27	6.589	1705	1710	1713	rBV3	770	715	0.04%	0.005%
28	6.605	1713	1715	1717	rVB3	683	306	0.02%	0.002%
29	6.637	1722	1725	1729	rVV2	705	629	0.03%	0.004%
30	6.727	1745	1753	1764	rVB3	2117	4086	0.21%	0.029%
31	6.804	1772	1777	1783	rVB5	505	647	0.03%	0.005%
32	6.849	1788	1791	1793	rBV2	500	365	0.02%	0.003%
33	6.894	1802	1805	1812	rVB5	700	788	0.04%	0.006%
34	6.929	1812	1816	1820	rBV3	479	366	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090618\
 Data File : VV007429.D
 Acq On : 06 Sep 2018 19:07
 Operator : SY/MD
 Sample : J4719-10
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGE6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

35	7.035	1829	1849	1867	rBV	210673	371496	19.01%	2.612%
36	7.167	1888	1890	1893	rBV3	574	331	0.02%	0.002%
37	7.209	1898	1903	1904	rBV	662	399	0.02%	0.003%
38	7.280	1922	1925	1927	rBV2	1256	842	0.04%	0.006%
39	7.363	1937	1951	1968	rBV	809902	1396208	71.43%	9.818%
40	7.595	2021	2023	2025	rBV3	548	298	0.02%	0.002%
41	7.669	2032	2046	2066	rBV	154749	265543	13.59%	1.867%
42	7.817	2089	2092	2097	rVB4	914	798	0.04%	0.006%
43	7.904	2116	2119	2122	rBV2	788	619	0.03%	0.004%
44	7.987	2136	2145	2147	rBV6	3298	4551	0.23%	0.032%
45	8.023	2150	2156	2166	rVB2	19883	30078	1.54%	0.212%
46	8.142	2180	2193	2228	rBV2	408824	830470	42.49%	5.840%
47	8.617	2340	2341	2345	rVB	719	315	0.02%	0.002%
48	8.643	2345	2349	2350	rBV3	608	506	0.03%	0.004%
49	8.695	2362	2365	2370	rVV3	556	491	0.03%	0.003%
50	8.759	2380	2385	2386	rBV3	788	525	0.03%	0.004%
51	8.900	2415	2429	2458	rBV	952200	1551772	79.39%	10.912%
52	9.187	2515	2518	2525	rVB5	1037	1076	0.06%	0.008%
53	9.248	2527	2537	2539	rBV4	3537	4977	0.25%	0.035%
54	9.550	2628	2631	2635	rVB	630	530	0.03%	0.004%
55	9.588	2635	2643	2645	rBV5	773	1042	0.05%	0.007%
56	9.653	2656	2663	2669	rBV5	1121	1490	0.08%	0.010%
57	9.678	2669	2671	2675	rVB3	523	295	0.02%	0.002%
58	9.759	2692	2696	2699	rBV2	428	343	0.02%	0.002%
59	9.855	2723	2726	2727	rBV2	690	367	0.02%	0.003%
60	9.910	2741	2743	2750	rVB5	697	785	0.04%	0.006%
61	9.945	2750	2754	2757	rBV3	809	661	0.03%	0.005%
62	9.981	2761	2765	2770	rBV4	640	602	0.03%	0.004%
63	10.109	2801	2805	2806	rBV2	547	437	0.02%	0.003%
64	10.186	2826	2829	2833	rBV2	463	329	0.02%	0.002%
65	10.219	2835	2839	2841	rBV2	543	438	0.02%	0.003%
66	10.267	2842	2854	2884	rVB	577650	944058	48.30%	6.638%
67	10.428	2892	2904	2912	rBV5	2395	3734	0.19%	0.026%
68	10.627	2959	2966	2967	rBV4	817	838	0.04%	0.006%
69	10.714	2990	2993	2996	rVB2	427	294	0.02%	0.002%
70	10.855	3033	3037	3043	rVB3	518	555	0.03%	0.004%
71	10.907	3049	3053	3057	rBV5	790	696	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090618\
 Data File : VV007429.D
 Acq On : 06 Sep 2018 19:07
 Operator : SY/MD
 Sample : J4719-10
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGE6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

72	10.974	3067	3074	3078	rBV4	1276	1723	0.09%	0.012%
73	11.141	3123	3126	3129	rBV3	519	387	0.02%	0.003%
74	11.157	3129	3131	3137	rBV4	633	533	0.03%	0.004%
75	11.299	3163	3175	3200	rBV	690862	1165218	59.62%	8.194%
76	11.428	3210	3215	3218	rBV3	835	729	0.04%	0.005%
77	11.498	3235	3237	3241	rVB3	556	378	0.02%	0.003%
78	11.579	3260	3262	3263	rVV2	739	358	0.02%	0.003%
79	11.595	3263	3267	3269	rVV5	1460	1346	0.07%	0.009%
80	11.620	3269	3275	3280	rVV10	2551	3689	0.19%	0.026%
81	11.678	3280	3293	3315	rVB	670661	1150648	58.87%	8.091%
82	11.833	3338	3341	3344	rBV4	488	333	0.02%	0.002%
83	11.945	3373	3376	3378	rBV2	615	330	0.02%	0.002%
84	12.093	3420	3422	3426	rVB	586	352	0.02%	0.002%
85	12.122	3428	3431	3434	rBV2	415	301	0.02%	0.002%
86	12.219	3458	3461	3463	rBV2	380	298	0.02%	0.002%
87	12.254	3469	3472	3475	rBV2	495	295	0.02%	0.002%
88	12.476	3538	3541	3547	rBV4	863	847	0.04%	0.006%
89	12.553	3561	3565	3567	rBV	477	394	0.02%	0.003%
90	12.723	3616	3618	3621	rVB2	1093	547	0.03%	0.004%
91	12.746	3621	3625	3627	rBV2	639	419	0.02%	0.003%
92	13.064	3722	3724	3731	rVB3	732	766	0.04%	0.005%
93	13.289	3790	3794	3796	rBV2	525	485	0.02%	0.003%
94	13.418	3830	3834	3837	rBV2	756	614	0.03%	0.004%
95	13.473	3849	3851	3855	rBV4	565	387	0.02%	0.003%
96	13.813	3955	3957	3962	rBV3	813	702	0.04%	0.005%
97	13.939	3992	3996	3997	rBV3	543	411	0.02%	0.003%
98	14.157	4062	4064	4067	rVB3	865	411	0.02%	0.003%
99	14.302	4107	4109	4111	rBV2	762	452	0.02%	0.003%
100	14.482	4162	4165	4168	rBV3	1089	888	0.05%	0.006%


Sum of corrected areas: 14221119

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV090618\
Data File : VV007429.D
Acq On : 06 Sep 2018 19:07
Operator : SY/MD
Sample : J4719-10
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGE6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

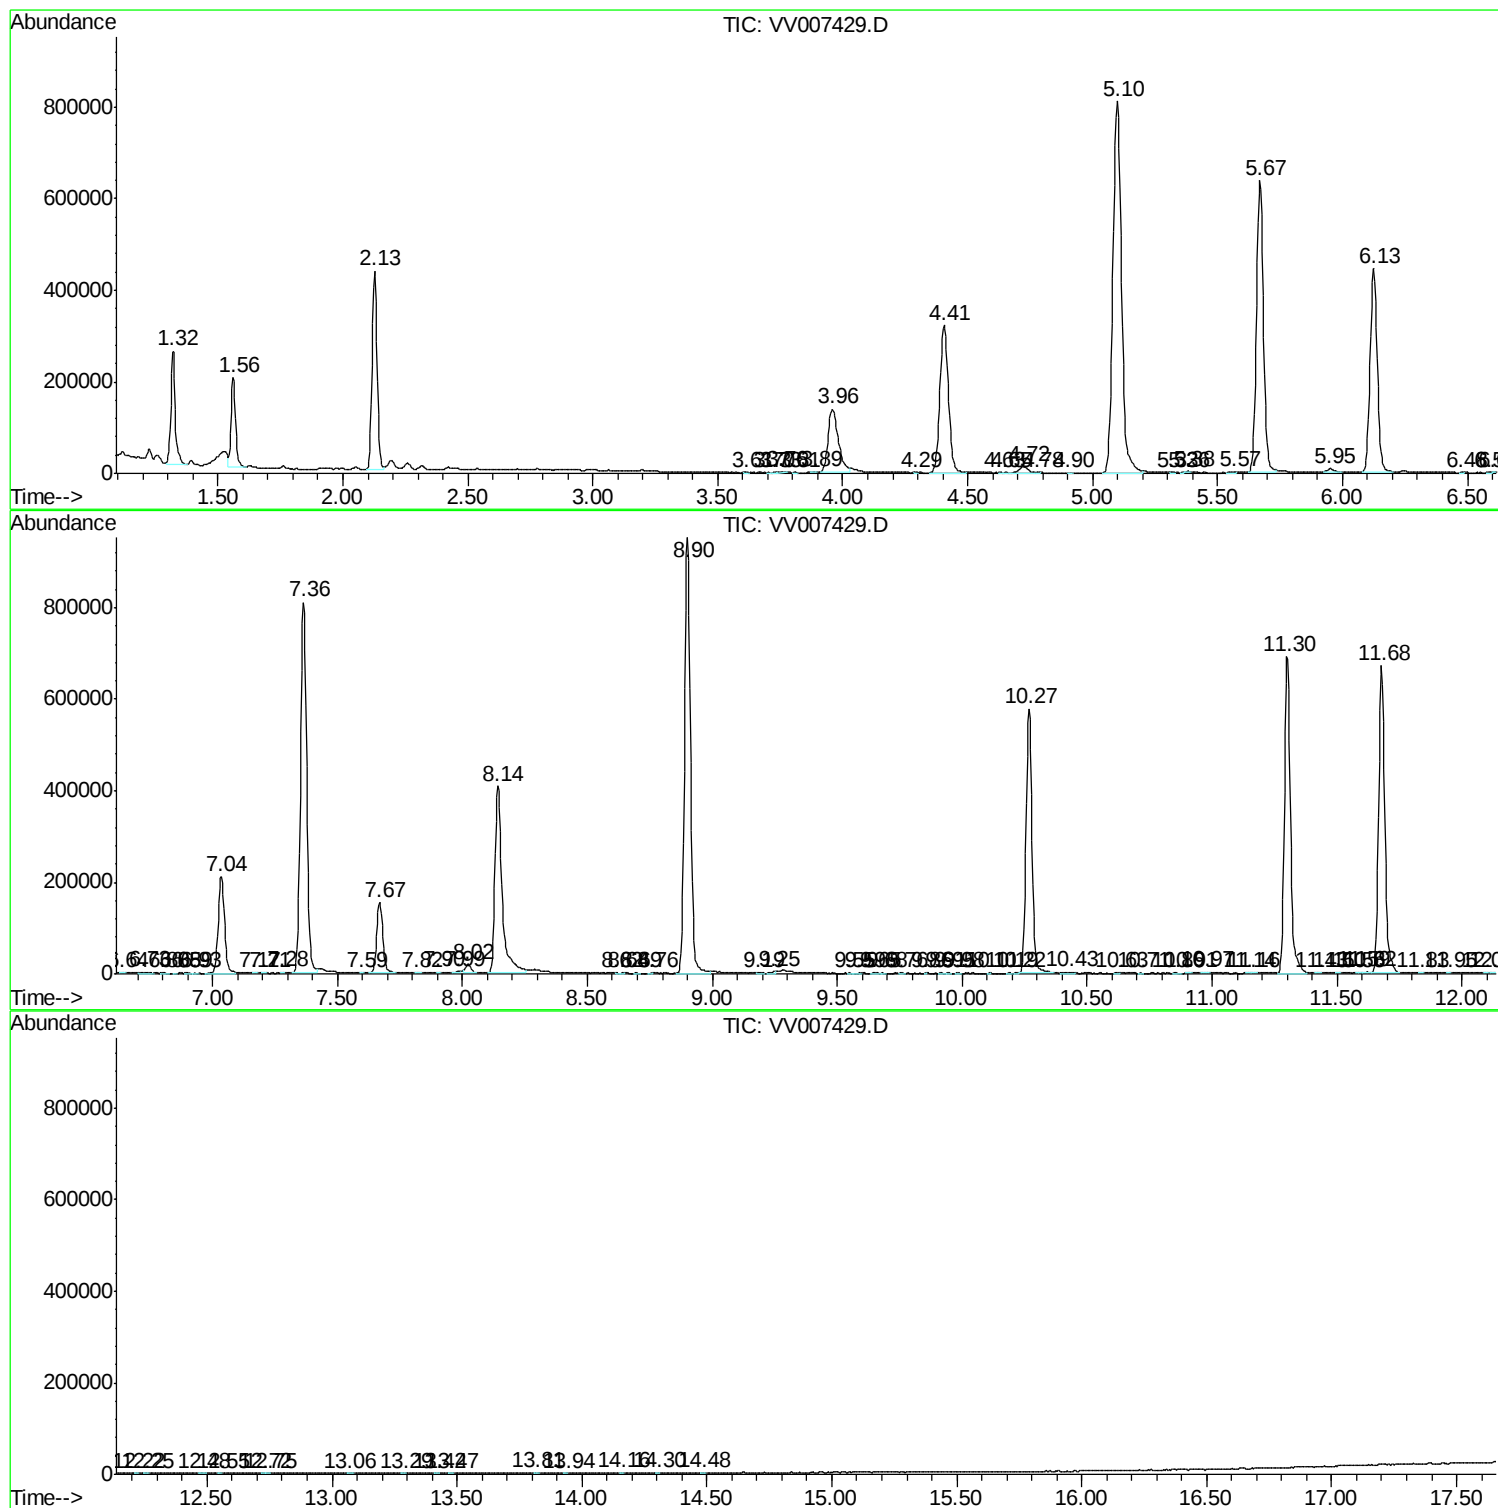

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV090618\
Data File : VV007429.D
Acq On : 06 Sep 2018 19:07
Operator : SY/MD
Sample : J4719-10
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGE6

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV090618\
Data File : VV007429.D
Acq On : 06 Sep 2018 19:07
Operator : SY/MD
Sample : J4719-10
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGE6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc