

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090618\
 Data File : VV007430.D
 Acq On : 06 Sep 2018 19:32
 Operator : SY/MD
 Sample : J4719-14
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGF0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	63	71	88	rVB	244122	285859	14.91%	1.904%
2	1.393	90	94	101	rVB	21273	20744	1.08%	0.138%
3	1.560	140	146	162	rVB	195165	243976	12.72%	1.625%
4	2.126	312	322	334	rBV	434488	609506	31.79%	4.059%
5	3.547	760	764	768	rBV5	419	362	0.02%	0.002%
6	3.685	805	807	811	rVB	602	331	0.02%	0.002%
7	3.756	827	829	832	rBV	437	305	0.02%	0.002%
8	3.962	874	893	929	rBV4	192779	556181	29.01%	3.704%
9	4.106	935	938	940	rBV2	716	373	0.02%	0.002%
10	4.280	989	992	997	rBV3	765	672	0.04%	0.004%
11	4.405	1012	1031	1055	rVV	314784	754447	39.35%	5.024%
12	4.589	1086	1088	1092	rVB2	739	481	0.03%	0.003%
13	4.614	1092	1096	1098	rBV2	516	285	0.01%	0.002%
14	4.653	1103	1108	1113	rBV6	660	823	0.04%	0.005%
15	4.721	1120	1129	1131	rBV4	1130	1463	0.08%	0.010%
16	4.775	1143	1146	1150	rVB3	430	369	0.02%	0.002%
17	4.814	1154	1158	1163	rVB2	646	573	0.03%	0.004%
18	4.852	1163	1170	1175	rBV3	445	526	0.03%	0.004%
19	4.881	1175	1179	1181	rBV2	359	295	0.02%	0.002%
20	4.958	1199	1203	1207	rBV2	439	412	0.02%	0.003%
21	5.029	1222	1225	1227	rVB	485	287	0.01%	0.002%
22	5.097	1227	1246	1288	rBV2	820095	1917408	100.00%	12.769%
23	5.306	1307	1311	1314	rVB3	498	459	0.02%	0.003%
24	5.441	1350	1353	1355	rVV2	640	402	0.02%	0.003%
25	5.460	1357	1359	1362	rVB3	838	434	0.02%	0.003%
26	5.483	1362	1366	1370	rBV3	614	321	0.02%	0.002%
27	5.505	1370	1373	1375	rBV2	385	279	0.01%	0.002%
28	5.547	1383	1386	1389	rBV3	494	333	0.02%	0.002%
29	5.595	1398	1401	1405	rBV3	525	403	0.02%	0.003%
30	5.669	1409	1424	1451	rBV	639166	1263028	65.87%	8.411%
31	5.955	1504	1513	1526	rVB6	11465	24220	1.26%	0.161%
32	6.048	1540	1542	1546	rBV2	801	482	0.03%	0.003%
33	6.122	1551	1565	1593	rBV	441478	887822	46.30%	5.913%
34	6.354	1631	1637	1640	rBV5	420	475	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090618\
 Data File : VV007430.D
 Acq On : 06 Sep 2018 19:32
 Operator : SY/MD
 Sample : J4719-14
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGF0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

35	6.389	1646	1648	1652	rBV2	405	281	0.01%	0.002%
36	6.412	1652	1655	1658	rBV2	497	386	0.02%	0.003%
37	6.534	1689	1693	1697	rBV3	432	374	0.02%	0.002%
38	6.569	1700	1704	1708	rBV2	409	437	0.02%	0.003%
39	6.637	1721	1725	1727	rBV	556	389	0.02%	0.003%
40	6.730	1744	1754	1762	rBV6	2268	4221	0.22%	0.028%
41	6.820	1775	1782	1786	rBV5	456	540	0.03%	0.004%
42	6.843	1786	1789	1792	rBV4	493	364	0.02%	0.002%
43	6.881	1799	1801	1806	rVB3	360	345	0.02%	0.002%
44	6.942	1813	1820	1823	rBV4	491	514	0.03%	0.003%
45	7.036	1835	1849	1875	rBV	205817	367155	19.15%	2.445%
46	7.364	1936	1951	1972	rBV	808616	1400443	73.04%	9.327%
47	7.669	2030	2046	2064	rBV	156135	261561	13.64%	1.742%
48	7.852	2099	2103	2106	rVB3	745	570	0.03%	0.004%
49	8.023	2138	2156	2173	rBV	383787	651378	33.97%	4.338%
50	8.142	2181	2193	2238	rBV2	425460	848253	44.24%	5.649%
51	8.486	2297	2300	2306	rVB4	607	562	0.03%	0.004%
52	8.621	2339	2342	2346	rVB4	657	428	0.02%	0.003%
53	8.720	2369	2373	2376	rBV2	517	421	0.02%	0.003%
54	8.775	2387	2390	2394	rVB2	539	333	0.02%	0.002%
55	8.820	2402	2404	2411	rVB	476	416	0.02%	0.003%
56	8.900	2415	2429	2451	rBV	965483	1571987	81.99%	10.469%
57	9.180	2510	2516	2518	rBV4	1048	1318	0.07%	0.009%
58	9.238	2526	2534	2535	rBV5	2395	2375	0.12%	0.016%
59	9.553	2628	2632	2635	rVB3	653	494	0.03%	0.003%
60	9.592	2635	2644	2653	rBV4	2767	4500	0.23%	0.030%
61	9.704	2676	2679	2683	rVB	533	491	0.03%	0.003%
62	9.826	2713	2717	2721	rBV2	667	685	0.04%	0.005%
63	9.978	2762	2764	2768	rBV2	590	381	0.02%	0.003%
64	10.084	2795	2797	2803	rVB2	454	305	0.02%	0.002%
65	10.132	2810	2812	2818	rVB3	404	376	0.02%	0.003%
66	10.158	2818	2820	2827	rBV2	460	469	0.02%	0.003%
67	10.267	2838	2854	2877	rBV	586576	950574	49.58%	6.331%
68	10.428	2897	2904	2911	rVB4	1512	1976	0.10%	0.013%
69	10.531	2932	2936	2938	rBV3	475	325	0.02%	0.002%
70	10.669	2974	2979	2983	rBV5	634	665	0.03%	0.004%
71	10.733	2995	2999	3003	rBV2	290	282	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090618\
 Data File : VV007430.D
 Acq On : 06 Sep 2018 19:32
 Operator : SY/MD
 Sample : J4719-14
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGF0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

72	10.807	3018	3022	3023	rBV	471	278	0.01%	0.002%
73	10.878	3041	3044	3046	rBV2	397	297	0.02%	0.002%
74	10.984	3073	3077	3078	rBV2	1309	959	0.05%	0.006%
75	11.019	3086	3088	3093	rVB2	847	523	0.03%	0.003%
76	11.061	3099	3101	3104	rVB2	653	323	0.02%	0.002%
77	11.084	3104	3108	3109	rBV2	622	407	0.02%	0.003%
78	11.116	3116	3118	3121	rBV2	573	290	0.02%	0.002%
79	11.141	3121	3126	3130	rVB4	701	618	0.03%	0.004%
80	11.174	3130	3136	3141	rVB3	637	714	0.04%	0.005%
81	11.299	3163	3175	3202	rBV	708885	1193027	62.22%	7.945%
82	11.418	3208	3212	3213	rBV2	540	394	0.02%	0.003%
83	11.579	3260	3262	3265	rBV3	540	356	0.02%	0.002%
84	11.678	3279	3293	3320	rBV	677496	1158726	60.43%	7.717%
85	11.910	3362	3365	3367	rVB2	548	301	0.02%	0.002%
86	11.968	3378	3383	3385	rBV2	397	395	0.02%	0.003%
87	12.051	3405	3409	3410	rBV3	441	306	0.02%	0.002%
88	12.154	3439	3441	3448	rVB3	624	393	0.02%	0.003%
89	12.260	3472	3474	3478	rBV3	497	369	0.02%	0.002%
90	12.293	3481	3484	3486	rBV2	632	498	0.03%	0.003%
91	12.341	3496	3499	3504	rBV5	789	662	0.03%	0.004%
92	12.405	3517	3519	3523	rVB2	603	365	0.02%	0.002%
93	12.672	3599	3602	3606	rBV3	675	711	0.04%	0.005%
94	12.823	3646	3649	3650	rBV4	522	331	0.02%	0.002%
95	12.865	3660	3662	3665	rBV3	520	328	0.02%	0.002%
96	12.897	3669	3672	3676	rVB3	820	591	0.03%	0.004%
97	12.997	3697	3703	3706	rBV4	618	752	0.04%	0.005%
98	13.215	3769	3771	3774	rBV3	752	461	0.02%	0.003%
99	13.936	3992	3995	3999	rBV2	856	754	0.04%	0.005%
100	13.958	4000	4002	4006	rVV4	780	537	0.03%	0.004%


Sum of corrected areas: 15015576

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV090618\
Data File : VV007430.D
Acq On : 06 Sep 2018 19:32
Operator : SY/MD
Sample : J4719-14
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGF0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

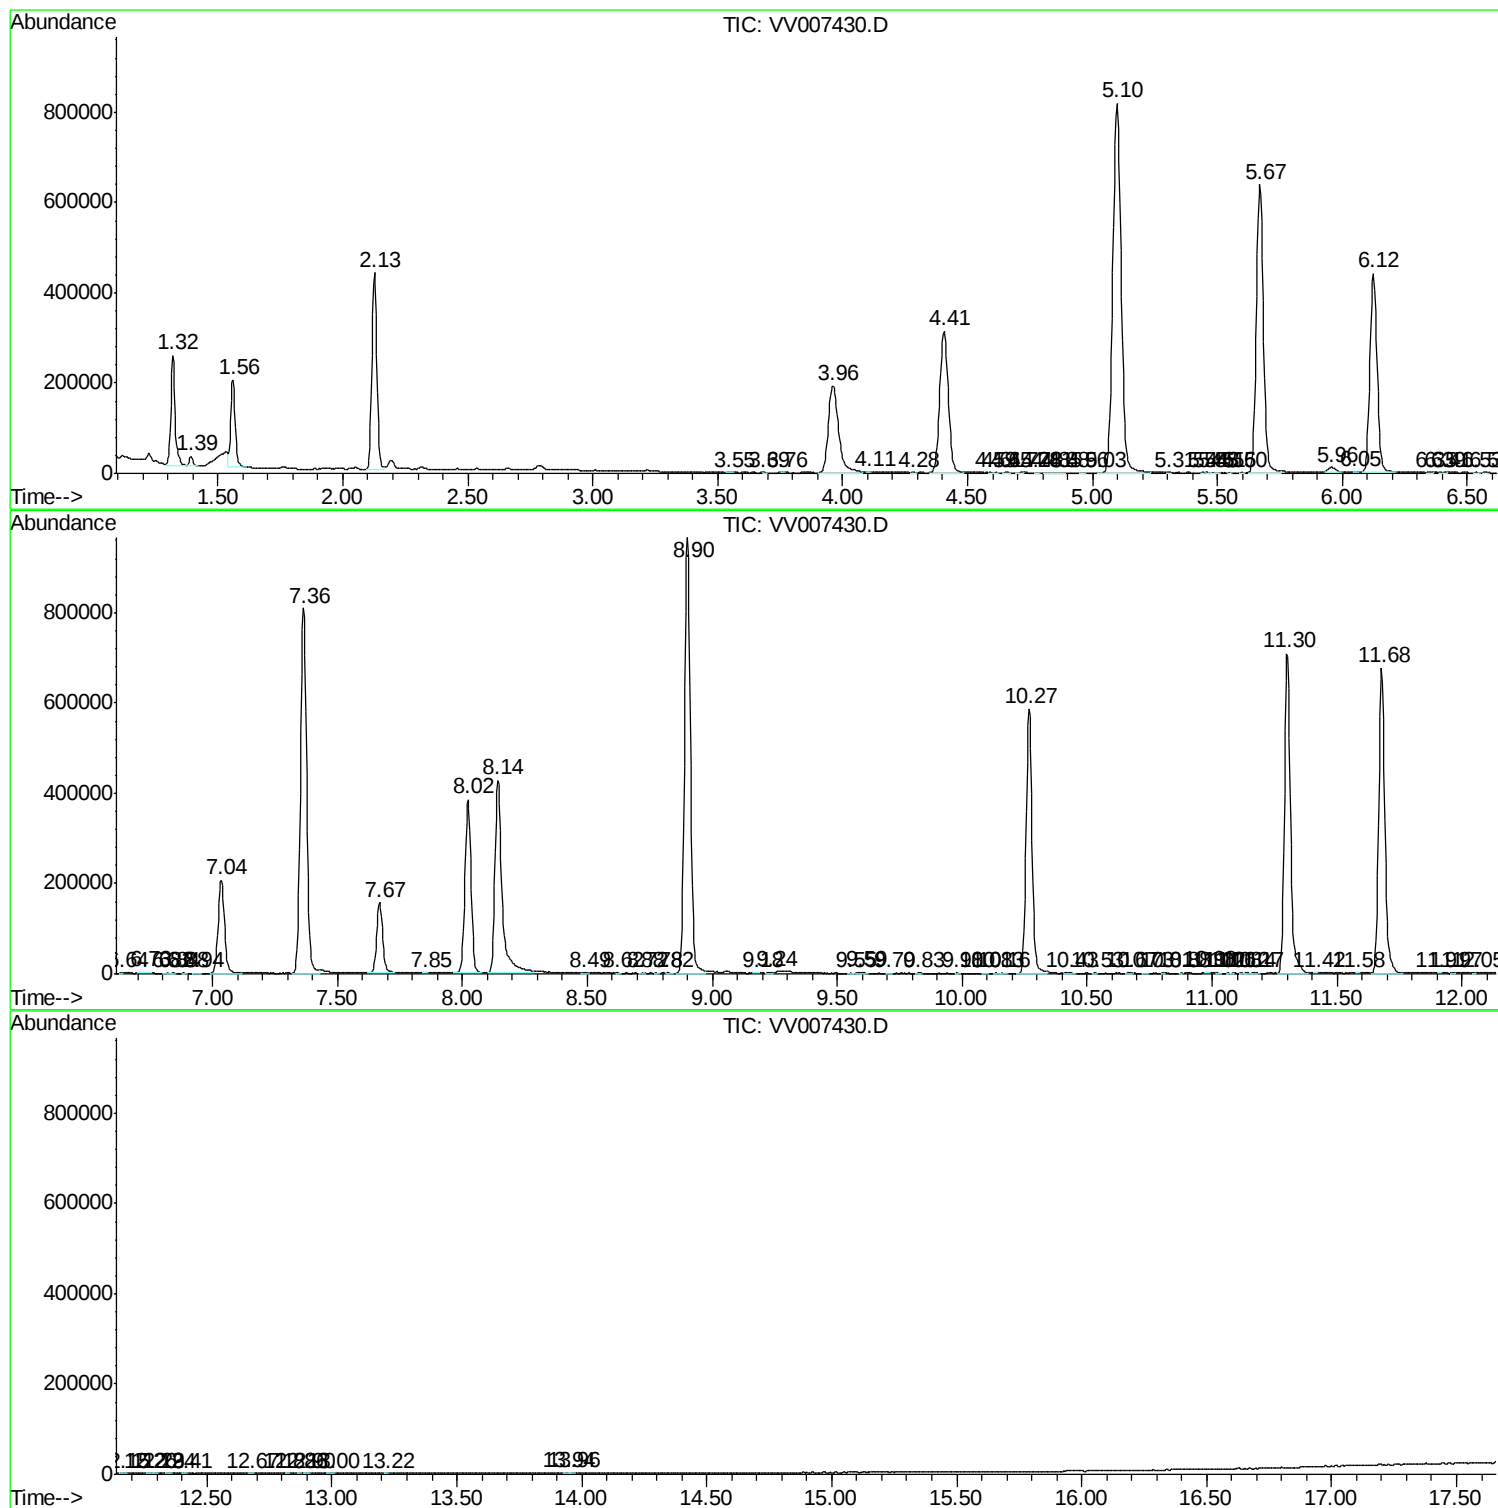

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV090618\
Data File : VV007430.D
Acq On : 06 Sep 2018 19:32
Operator : SY/MD
Sample : J4719-14
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGF0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV090618\
Data File : VV007430.D
Acq On : 06 Sep 2018 19:32
Operator : SY/MD
Sample : J4719-14
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGF0

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
