

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090618\
 Data File : VV007431.D
 Acq On : 06 Sep 2018 19:57
 Operator : SY/MD
 Sample : J4719-11DL 10X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGE7DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	63	71	89	rVB	205173	277333	15.65%	1.753%
2	1.550	139	143	165	rVB	159737	232202	13.10%	1.468%
3	2.119	310	320	334	rBV	398044	552377	31.17%	3.492%
4	2.531	441	448	458	rVB2	18366	28474	1.61%	0.180%
5	2.656	477	487	503	rVB	29183	59288	3.35%	0.375%
6	3.476	739	742	745	rVB2	610	382	0.02%	0.002%
7	3.698	809	811	815	rVB3	489	282	0.02%	0.002%
8	3.814	844	847	850	rBV2	396	242	0.01%	0.002%
9	3.849	854	858	862	rVB2	502	426	0.02%	0.003%
10	3.878	862	867	868	rBV2	406	329	0.02%	0.002%
11	3.962	875	893	941	rBV3	214641	631444	35.63%	3.992%
12	4.290	993	995	1001	rVB4	570	413	0.02%	0.003%
13	4.405	1012	1031	1055	rBV	295637	704663	39.76%	4.455%
14	4.589	1085	1088	1092	rBV3	310	245	0.01%	0.002%
15	4.627	1097	1100	1104	rBV	516	517	0.03%	0.003%
16	4.717	1125	1128	1129	rBV2	511	299	0.02%	0.002%
17	4.727	1129	1131	1135	rVB3	541	331	0.02%	0.002%
18	4.804	1151	1155	1159	rVB2	430	320	0.02%	0.002%
19	4.823	1159	1161	1164	rVB2	428	224	0.01%	0.001%
20	4.952	1198	1201	1204	rVB2	451	291	0.02%	0.002%
21	4.975	1204	1208	1213	rBV3	551	581	0.03%	0.004%
22	5.007	1213	1218	1221	rVB	315	274	0.02%	0.002%
23	5.097	1227	1246	1271	rBV2	761408	1772382	100.00%	11.206%
24	5.299	1307	1309	1314	rVB3	618	328	0.02%	0.002%
25	5.376	1329	1333	1334	rBV	372	267	0.02%	0.002%
26	5.409	1339	1343	1345	rVV3	418	302	0.02%	0.002%
27	5.421	1345	1347	1351	rVB3	409	247	0.01%	0.002%
28	5.550	1385	1387	1391	rBV3	442	303	0.02%	0.002%
29	5.573	1391	1394	1399	rBV2	375	285	0.02%	0.002%
30	5.669	1409	1424	1449	rBV	582755	1151441	64.97%	7.280%
31	5.962	1500	1515	1536	rBV	268561	519953	29.34%	3.287%
32	6.122	1550	1565	1591	rBV	418072	836194	47.18%	5.287%
33	6.431	1657	1661	1664	rBV4	560	499	0.03%	0.003%
34	6.470	1671	1673	1677	rVB2	570	317	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090618\
 Data File : VV007431.D
 Acq On : 06 Sep 2018 19:57
 Operator : SY/MD
 Sample : J4719-11DL 10X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGE7DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

35	6.489	1677	1679	1683	rVB2	402	230	0.01%	0.001%
36	6.515	1683	1687	1692	rBV5	726	859	0.05%	0.005%
37	6.560	1698	1701	1706	rBV4	424	362	0.02%	0.002%
38	6.663	1728	1733	1734	rBV4	1269	1007	0.06%	0.006%
39	6.730	1746	1754	1762	rVB	4513	6871	0.39%	0.043%
40	6.868	1794	1797	1801	rVB2	383	264	0.01%	0.002%
41	6.910	1807	1810	1812	rVV3	446	238	0.01%	0.002%
42	6.939	1815	1819	1825	rVB5	446	412	0.02%	0.003%
43	6.981	1829	1832	1835	rVB3	427	272	0.02%	0.002%
44	7.036	1835	1849	1871	rBV	193649	349225	19.70%	2.208%
45	7.280	1923	1925	1929	rBV3	675	458	0.03%	0.003%
46	7.364	1935	1951	1972	rBV	745559	1283881	72.44%	8.118%
47	7.563	2010	2013	2015	rBV4	643	321	0.02%	0.002%
48	7.669	2032	2046	2066	rBV	139849	236450	13.34%	1.495%
49	7.852	2100	2103	2106	rBV3	517	410	0.02%	0.003%
50	8.023	2139	2156	2180	rBV	992081	1653936	93.32%	10.457%
51	8.145	2182	2194	2229	rBV2	423610	849806	47.95%	5.373%
52	8.495	2301	2303	2307	rBV4	416	255	0.01%	0.002%
53	8.605	2334	2337	2339	rBV2	602	314	0.02%	0.002%
54	8.662	2352	2355	2357	rVB2	594	307	0.02%	0.002%
55	8.852	2410	2414	2416	rBV2	352	313	0.02%	0.002%
56	8.900	2416	2429	2452	rBV	876256	1441366	81.32%	9.113%
57	9.251	2533	2538	2539	rBV2	421	368	0.02%	0.002%
58	9.338	2561	2565	2568	rBV5	611	516	0.03%	0.003%
59	9.460	2599	2603	2605	rBV2	507	301	0.02%	0.002%
60	9.592	2640	2644	2648	rBV5	563	480	0.03%	0.003%
61	9.672	2666	2669	2671	rBV	466	367	0.02%	0.002%
62	9.752	2691	2694	2697	rBV2	531	431	0.02%	0.003%
63	9.833	2716	2719	2723	rVB3	481	326	0.02%	0.002%
64	9.871	2723	2731	2737	rBV4	666	796	0.04%	0.005%
65	9.900	2737	2740	2742	rBV2	522	346	0.02%	0.002%
66	9.942	2750	2753	2754	rBV2	401	241	0.01%	0.002%
67	9.971	2759	2762	2764	rBV	554	341	0.02%	0.002%
68	10.016	2773	2776	2780	rVB3	411	338	0.02%	0.002%
69	10.039	2780	2783	2786	rBV2	328	244	0.01%	0.002%
70	10.071	2789	2793	2796	rBV	333	346	0.02%	0.002%
71	10.267	2842	2854	2887	rBV	586845	961166	54.23%	6.077%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090618\
 Data File : VV007431.D
 Acq On : 06 Sep 2018 19:57
 Operator : SY/MD
 Sample : J4719-11DL 10X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGE7DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

72	10.434	2902	2906	2912	rVB3	1009	982	0.06%	0.006%
73	10.502	2924	2927	2932	rVB3	446	373	0.02%	0.002%
74	10.547	2939	2941	2945	rBV4	343	225	0.01%	0.001%
75	10.598	2954	2957	2960	rVB	399	241	0.01%	0.002%
76	10.679	2978	2982	2986	rVB2	382	372	0.02%	0.002%
77	10.894	3046	3049	3051	rBV2	554	295	0.02%	0.002%
78	10.913	3051	3055	3061	rVB4	790	672	0.04%	0.004%
79	11.013	3083	3086	3089	rBV4	477	303	0.02%	0.002%
80	11.061	3097	3101	3106	rBV3	539	509	0.03%	0.003%
81	11.084	3106	3108	3111	rBV3	326	246	0.01%	0.002%
82	11.142	3123	3126	3129	rBV2	523	327	0.02%	0.002%
83	11.302	3163	3176	3201	rBV	673055	1126964	63.58%	7.125%
84	11.479	3224	3231	3237	rBV4	770	1215	0.07%	0.008%
85	11.505	3237	3239	3243	rVB3	661	366	0.02%	0.002%
86	11.524	3243	3245	3247	rBV2	455	248	0.01%	0.002%
87	11.678	3280	3293	3318	rBV	655611	1109924	62.62%	7.018%
88	11.801	3329	3331	3334	rBV2	454	305	0.02%	0.002%
89	11.871	3351	3353	3357	rVB2	599	336	0.02%	0.002%
90	12.045	3404	3407	3411	rBV3	530	444	0.03%	0.003%
91	12.322	3491	3493	3498	rVB2	491	315	0.02%	0.002%
92	12.344	3498	3500	3504	rBV2	408	401	0.02%	0.003%
93	12.556	3563	3566	3568	rBV2	655	502	0.03%	0.003%
94	12.598	3576	3579	3582	rBV2	683	486	0.03%	0.003%
95	12.817	3645	3647	3650	rVB2	594	315	0.02%	0.002%
96	13.032	3712	3714	3717	rBV2	532	230	0.01%	0.001%
97	13.235	3774	3777	3781	rVB3	632	422	0.02%	0.003%
98	13.762	3938	3941	3944	rBV2	482	428	0.02%	0.003%
99	13.958	4001	4002	4005	rBV3	501	350	0.02%	0.002%
100	14.309	4109	4111	4116	rBV3	852	698	0.04%	0.004%


Sum of corrected areas: 15816113

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV090618\
Data File : VV007431.D
Acq On : 06 Sep 2018 19:57
Operator : SY/MD
Sample : J4719-11DL 10X
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGE7DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

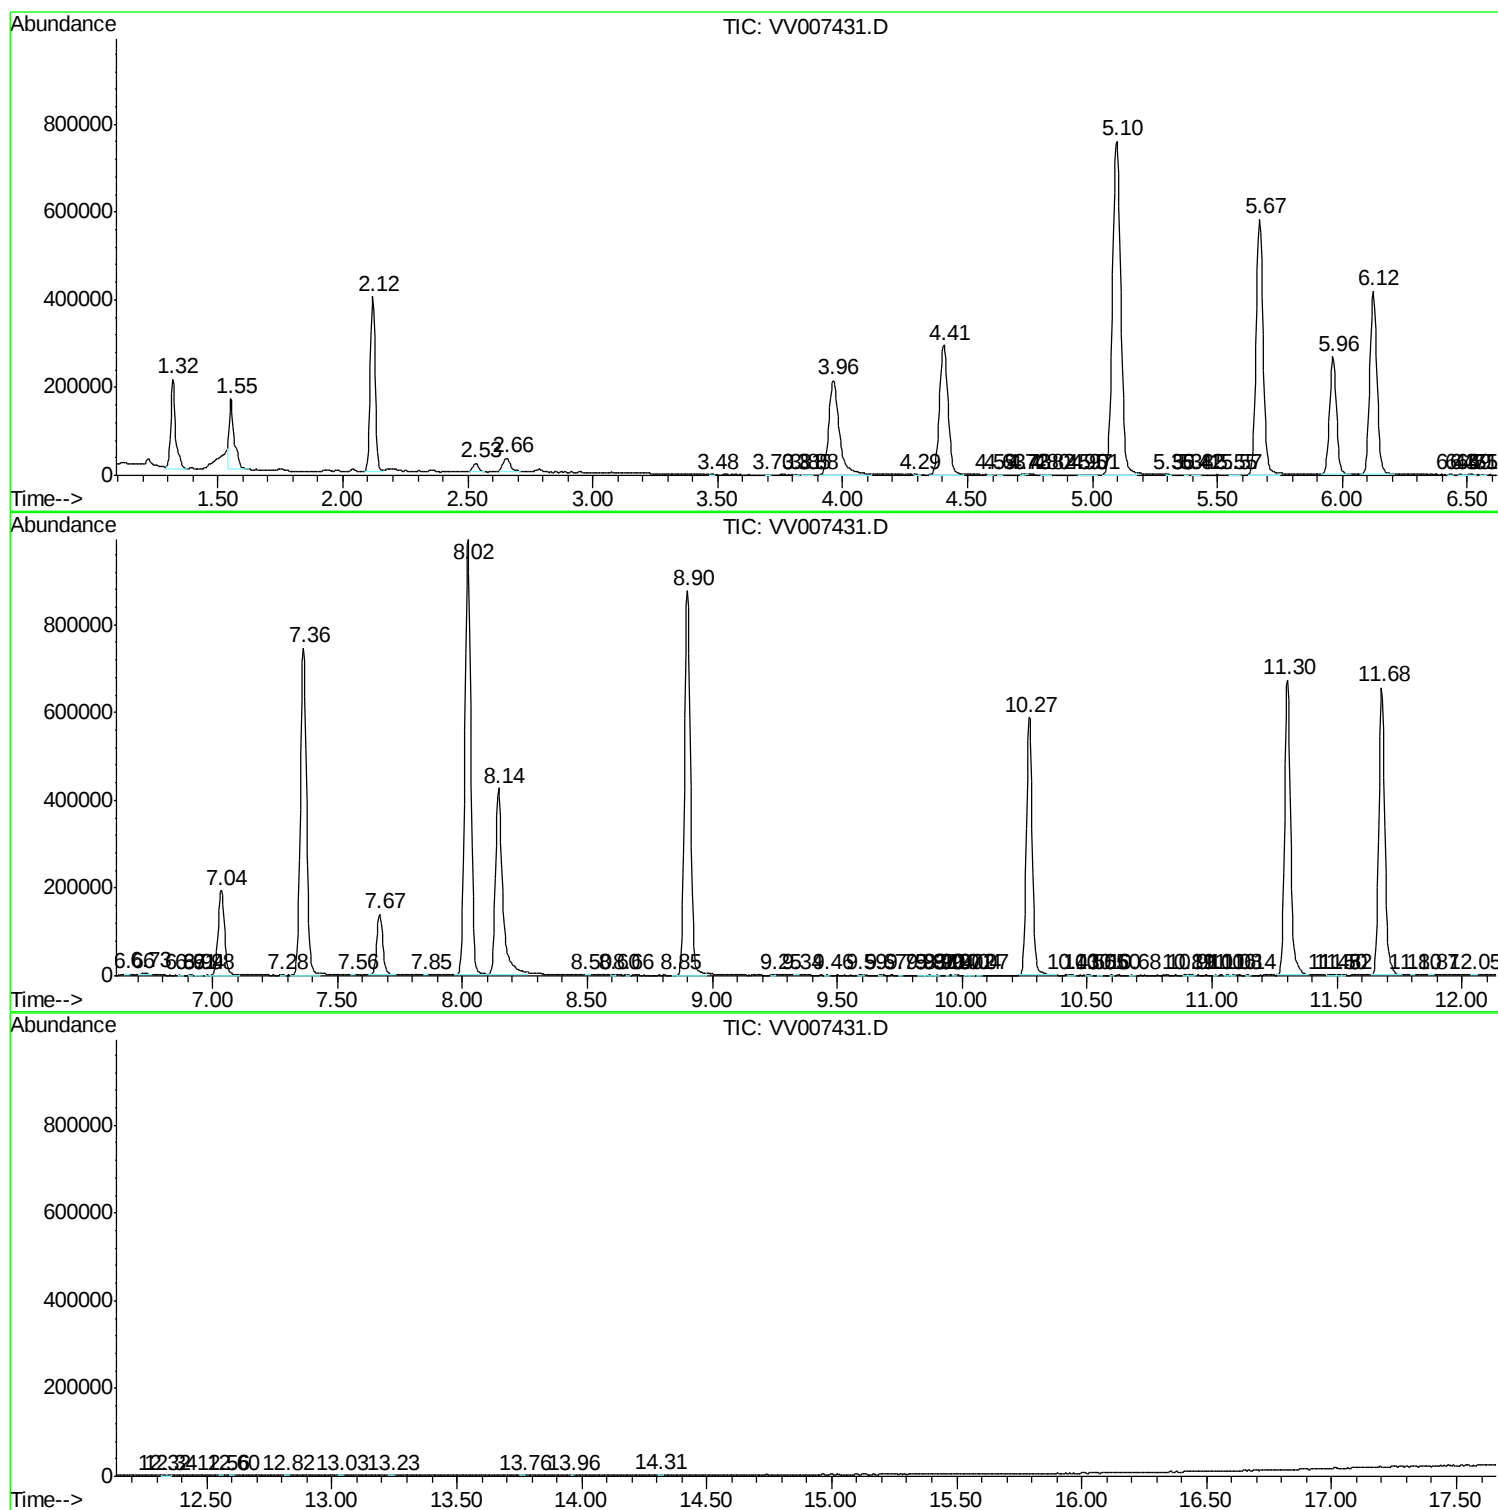

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV090618\
Data File : VV007431.D
Acq On : 06 Sep 2018 19:57
Operator : SY/MD
Sample : J4719-11DL 10X
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGE7DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV090618\
Data File : VV007431.D
Acq On : 06 Sep 2018 19:57
Operator : SY/MD
Sample : J4719-11DL 10X
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGE7DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc