

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090618\
 Data File : VV007432.D
 Acq On : 06 Sep 2018 20:22
 Operator : SY/MD
 Sample : J4719-12DL 10X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGE8DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	63	71	88	rVB	238692	287643	15.00%	1.856%
2	1.560	140	146	160	rVB	195914	240142	12.53%	1.550%
3	2.126	312	322	336	rBV	439699	619050	32.29%	3.995%
4	2.656	480	487	504	rVB2	20470	41180	2.15%	0.266%
5	3.377	709	711	717	rVB4	725	570	0.03%	0.004%
6	3.563	764	769	772	rBV3	451	461	0.02%	0.003%
7	3.647	792	795	799	rVB	582	392	0.02%	0.003%
8	3.695	807	810	816	rBV3	421	290	0.02%	0.002%
9	3.762	827	831	834	rVB3	458	356	0.02%	0.002%
10	3.881	863	868	874	rBV5	440	449	0.02%	0.003%
11	3.965	874	894	932	rBV2	143763	465931	24.30%	3.007%
12	4.315	997	1003	1007	rBV3	540	619	0.03%	0.004%
13	4.405	1013	1031	1057	rVV	320460	761327	39.71%	4.914%
14	4.650	1103	1107	1111	rBV3	495	341	0.02%	0.002%
15	4.711	1120	1126	1127	rBV2	553	556	0.03%	0.004%
16	4.836	1159	1165	1166	rBV	323	290	0.02%	0.002%
17	4.849	1166	1169	1174	rVB3	314	276	0.01%	0.002%
18	4.952	1192	1201	1206	rBV2	340	289	0.02%	0.002%
19	5.100	1222	1247	1274	rBV2	817738	1917250	100.00%	12.374%
20	5.338	1318	1321	1322	rBV3	563	327	0.02%	0.002%
21	5.354	1324	1326	1331	rVV3	479	271	0.01%	0.002%
22	5.380	1331	1334	1337	rVV3	653	478	0.02%	0.003%
23	5.396	1337	1339	1344	rVB3	417	301	0.02%	0.002%
24	5.669	1405	1424	1445	rBV	628597	1239806	64.67%	8.002%
25	5.962	1501	1515	1532	rVB3	48363	100265	5.23%	0.647%
26	6.036	1536	1538	1540	rBV2	496	324	0.02%	0.002%
27	6.122	1550	1565	1593	rBV	443774	895640	46.71%	5.781%
28	6.486	1675	1678	1681	rBV3	402	268	0.01%	0.002%
29	6.508	1681	1685	1688	rVV4	364	279	0.01%	0.002%
30	6.534	1690	1693	1695	rVB3	528	301	0.02%	0.002%
31	6.601	1710	1714	1716	rBV	565	397	0.02%	0.003%
32	6.646	1721	1728	1731	rBV6	1094	1341	0.07%	0.009%
33	6.727	1745	1753	1765	rVB2	2174	4162	0.22%	0.027%
34	6.926	1813	1815	1821	rVB4	713	538	0.03%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090618\
 Data File : VV007432.D
 Acq On : 06 Sep 2018 20:22
 Operator : SY/MD
 Sample : J4719-12DL 10X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGE8DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

35	6.962	1821	1826	1829	rBV4	539	573	0.03%	0.004%
36	7.036	1834	1849	1871	rBV	204194	367772	19.18%	2.374%
37	7.196	1896	1899	1902	rVB3	507	279	0.01%	0.002%
38	7.222	1904	1907	1910	rVB3	783	493	0.03%	0.003%
39	7.363	1936	1951	1968	rBV	815443	1403481	73.20%	9.058%
40	7.566	2012	2014	2019	rBV3	484	344	0.02%	0.002%
41	7.669	2034	2046	2063	rBV	143637	236325	12.33%	1.525%
42	7.843	2096	2100	2101	rBV2	566	422	0.02%	0.003%
43	7.875	2106	2110	2112	rBV2	672	631	0.03%	0.004%
44	8.023	2142	2156	2176	rBV	711076	1210130	63.12%	7.810%
45	8.142	2181	2193	2238	rBV2	437153	876867	45.74%	5.659%
46	8.495	2300	2303	2305	rBV4	653	466	0.02%	0.003%
47	8.598	2329	2335	2336	rBV2	446	411	0.02%	0.003%
48	8.653	2348	2352	2354	rBV4	495	492	0.03%	0.003%
49	8.711	2367	2370	2373	rVB4	780	505	0.03%	0.003%
50	8.781	2389	2392	2393	rVV2	486	304	0.02%	0.002%
51	8.807	2397	2400	2403	rBV3	439	330	0.02%	0.002%
52	8.900	2415	2429	2458	rBV	948220	1548771	80.78%	9.996%
53	9.170	2512	2513	2518	rVV4	472	438	0.02%	0.003%
54	9.193	2518	2520	2524	rVV	523	394	0.02%	0.003%
55	9.222	2528	2529	2535	rVB2	587	398	0.02%	0.003%
56	9.296	2549	2552	2555	rBV2	531	340	0.02%	0.002%
57	9.457	2599	2602	2607	rVV2	420	268	0.01%	0.002%
58	9.736	2686	2689	2696	rVB3	402	369	0.02%	0.002%
59	9.868	2727	2730	2734	rBV2	451	339	0.02%	0.002%
60	9.907	2740	2742	2746	rVB2	482	307	0.02%	0.002%
61	9.939	2746	2752	2754	rBV2	377	391	0.02%	0.003%
62	9.981	2760	2765	2769	rBV3	441	464	0.02%	0.003%
63	10.000	2769	2771	2775	rVV2	407	330	0.02%	0.002%
64	10.135	2808	2813	2815	rBV3	410	290	0.02%	0.002%
65	10.187	2825	2829	2831	rBV2	455	286	0.01%	0.002%
66	10.267	2842	2854	2889	rVV	585022	961255	50.14%	6.204%
67	10.402	2892	2896	2900	rBV3	371	380	0.02%	0.002%
68	10.424	2900	2903	2910	rVV6	750	773	0.04%	0.005%
69	10.502	2925	2927	2931	rBV2	463	287	0.01%	0.002%
70	10.547	2936	2941	2945	rBV3	362	460	0.02%	0.003%
71	10.621	2962	2964	2969	rVV3	505	463	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090618\
 Data File : VV007432.D
 Acq On : 06 Sep 2018 20:22
 Operator : SY/MD
 Sample : J4719-12DL 10X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGE8DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

72	10.656	2973	2975	2980	rVB4	605	347	0.02%	0.002%
73	10.727	2994	2997	3001	rVV2	404	345	0.02%	0.002%
74	10.775	3005	3012	3014	rVB3	354	348	0.02%	0.002%
75	10.839	3029	3032	3036	rBV2	413	405	0.02%	0.003%
76	11.000	3077	3082	3086	rBV4	683	728	0.04%	0.005%
77	11.045	3092	3096	3099	rBV2	618	454	0.02%	0.003%
78	11.225	3145	3152	3153	rBV4	503	506	0.03%	0.003%
79	11.299	3162	3175	3203	rBV	672134	1146404	59.79%	7.399%
80	11.495	3230	3236	3240	rBV5	555	709	0.04%	0.005%
81	11.518	3240	3243	3247	rVB3	565	452	0.02%	0.003%
82	11.678	3278	3293	3319	rBV	660936	1136493	59.28%	7.335%
83	11.968	3380	3383	3386	rBV2	361	280	0.01%	0.002%
84	12.135	3432	3435	3439	rBV2	383	302	0.02%	0.002%
85	12.186	3444	3451	3455	rBV3	445	695	0.04%	0.004%
86	12.238	3464	3467	3469	rBV2	371	267	0.01%	0.002%
87	12.383	3509	3512	3515	rBV2	359	334	0.02%	0.002%
88	12.450	3530	3533	3537	rBV2	420	353	0.02%	0.002%
89	12.479	3538	3542	3545	rBV3	511	457	0.02%	0.003%
90	12.788	3635	3638	3642	rBV2	628	383	0.02%	0.002%
91	12.903	3672	3674	3678	rVB2	596	344	0.02%	0.002%
92	12.974	3693	3696	3698	rBV	589	360	0.02%	0.002%
93	12.997	3698	3703	3709	rVV5	555	651	0.03%	0.004%
94	13.302	3795	3798	3799	rBV3	559	298	0.02%	0.002%
95	13.347	3809	3812	3814	rBV3	787	495	0.03%	0.003%
96	13.563	3876	3879	3883	rVB3	702	515	0.03%	0.003%
97	13.630	3896	3900	3901	rBV3	622	410	0.02%	0.003%
98	13.891	3979	3981	3984	rBV3	553	318	0.02%	0.002%
99	14.411	4141	4143	4147	rBV2	680	544	0.03%	0.004%
100	14.518	4173	4176	4180	rBV3	1092	846	0.04%	0.005%


Sum of corrected areas: 15493981

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV090618\
Data File : VV007432.D
Acq On : 06 Sep 2018 20:22
Operator : SY/MD
Sample : J4719-12DL 10X
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGE8DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

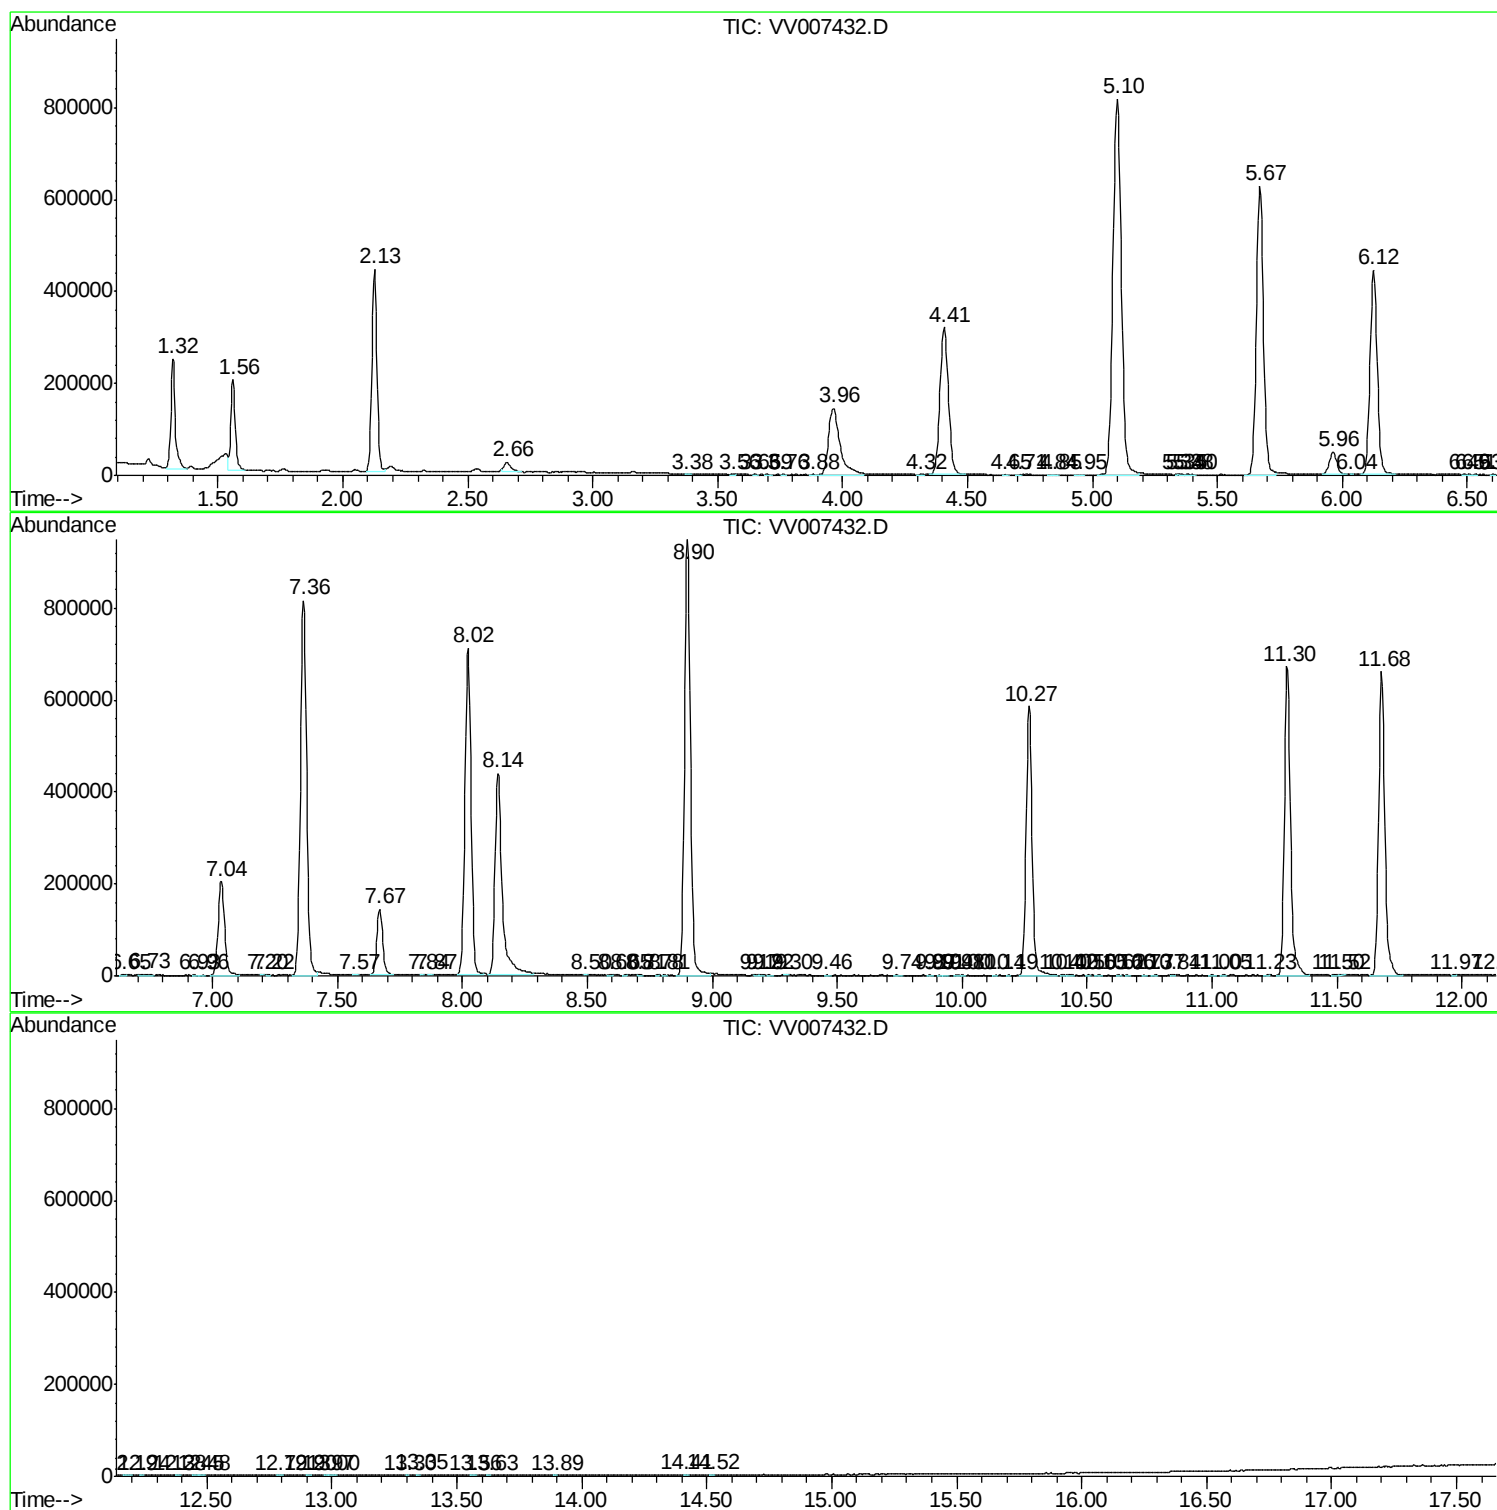

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV090618\
Data File : VV007432.D
Acq On : 06 Sep 2018 20:22
Operator : SY/MD
Sample : J4719-12DL 10X
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGE8DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV090618\
Data File : VV007432.D
Acq On : 06 Sep 2018 20:22
Operator : SY/MD
Sample : J4719-12DL 10X
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGE8DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc