

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090618\
 Data File : VV007435.D
 Acq On : 06 Sep 2018 21:37
 Operator : SY/MD
 Sample : J4719-16 10X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGF2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.322	64	72	88	rVB	220705	274048	7.50%	1.524%
2	1.560	140	146	163	rVB	188134	240207	6.58%	1.336%
3	2.126	313	322	335	rBV	423792	591602	16.20%	3.291%
4	3.492	744	747	751	rVB2	799	469	0.01%	0.003%
5	3.527	755	758	763	rVV3	531	423	0.01%	0.002%
6	3.695	804	810	813	rBV3	502	646	0.02%	0.004%
7	3.820	846	849	854	rVV4	285	277	0.01%	0.002%
8	3.881	865	868	873	rBV3	405	356	0.01%	0.002%
9	3.962	873	893	937	rBV3	213285	635603	17.40%	3.535%
10	4.290	992	995	996	rBV2	498	279	0.01%	0.002%
11	4.338	1008	1010	1013	rVB2	554	305	0.01%	0.002%
12	4.405	1013	1031	1056	rBV	310642	741497	20.30%	4.124%
13	4.601	1088	1092	1098	rVB3	482	392	0.01%	0.002%
14	4.704	1121	1124	1126	rBV3	478	304	0.01%	0.002%
15	4.717	1126	1128	1130	rBV2	738	417	0.01%	0.002%
16	4.865	1171	1174	1177	rBV	488	406	0.01%	0.002%
17	5.097	1227	1246	1283	rBV2	794452	1875646	51.35%	10.432%
18	5.489	1362	1368	1370	rBV3	435	460	0.01%	0.003%
19	5.531	1377	1381	1386	rVB4	496	443	0.01%	0.002%
20	5.553	1386	1388	1391	rVB2	486	265	0.01%	0.001%
21	5.669	1408	1424	1450	rBV	613563	1213857	33.23%	6.752%
22	5.961	1501	1515	1533	rBV	149245	291793	7.99%	1.623%
23	6.122	1550	1565	1592	rBV	434722	878511	24.05%	4.886%
24	6.351	1633	1636	1638	rBV2	459	367	0.01%	0.002%
25	6.392	1646	1649	1655	rVB2	712	440	0.01%	0.002%
26	6.466	1670	1672	1674	rBV2	499	267	0.01%	0.001%
27	6.566	1700	1703	1707	rBV2	567	352	0.01%	0.002%
28	6.595	1707	1712	1715	rVB2	428	392	0.01%	0.002%
29	6.614	1715	1718	1720	rBV2	467	304	0.01%	0.002%
30	6.659	1725	1732	1738	rBV6	884	1349	0.04%	0.008%
31	6.720	1741	1751	1762	rBV6	2114	4725	0.13%	0.026%
32	6.836	1783	1787	1793	rVB3	661	613	0.02%	0.003%
33	6.887	1797	1803	1811	rBV5	494	717	0.02%	0.004%
34	6.961	1821	1826	1831	rBV4	604	568	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090618\
 Data File : VV007435.D
 Acq On : 06 Sep 2018 21:37
 Operator : SY/MD
 Sample : J4719-16 10X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGF2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

35	7.035	1835	1849	1868	rBV	198425	355892	9.74%	1.979%
36	7.238	1909	1912	1917	rVB2	729	708	0.02%	0.004%
37	7.277	1919	1924	1925	rBV3	374	294	0.01%	0.002%
38	7.363	1937	1951	1980	rBV	793693	1372807	37.58%	7.636%
39	7.669	2033	2046	2074	rVV	134602	229674	6.29%	1.277%
40	7.810	2087	2090	2091	rBV3	622	329	0.01%	0.002%
41	7.858	2103	2105	2108	rBV2	558	417	0.01%	0.002%
42	7.904	2115	2119	2122	rBV2	401	378	0.01%	0.002%
43	8.022	2141	2156	2179	rBV	2218408	3652780	100.00%	20.317%
44	8.141	2182	2193	2233	rVB2	424253	853217	23.36%	4.746%
45	8.485	2297	2300	2302	rBV2	788	432	0.01%	0.002%
46	8.566	2321	2325	2327	rBV3	628	513	0.01%	0.003%
47	8.621	2339	2342	2347	rVB4	502	457	0.01%	0.003%
48	8.653	2347	2352	2354	rBV2	691	620	0.02%	0.003%
49	8.736	2375	2378	2382	rVB3	466	323	0.01%	0.002%
50	8.784	2389	2393	2394	rBV2	467	284	0.01%	0.002%
51	8.900	2416	2429	2456	rBV	939400	1532857	41.96%	8.526%
52	9.170	2509	2513	2514	rBV	431	271	0.01%	0.002%
53	9.183	2514	2517	2525	rVV5	836	1152	0.03%	0.006%
54	9.225	2527	2530	2532	rVV4	394	267	0.01%	0.001%
55	9.238	2532	2534	2538	rVV	626	378	0.01%	0.002%
56	9.260	2538	2541	2544	rVV2	607	511	0.01%	0.003%
57	9.293	2547	2551	2554	rBV3	803	699	0.02%	0.004%
58	9.309	2554	2556	2561	rVV5	659	502	0.01%	0.003%
59	9.450	2596	2600	2601	rBV2	498	324	0.01%	0.002%
60	9.592	2640	2644	2645	rBV2	441	318	0.01%	0.002%
61	9.678	2666	2671	2673	rVB2	534	467	0.01%	0.003%
62	9.820	2712	2715	2721	rVB3	264	278	0.01%	0.002%
63	9.862	2725	2728	2731	rVB	459	263	0.01%	0.001%
64	10.022	2776	2778	2783	rVB3	465	325	0.01%	0.002%
65	10.087	2794	2798	2799	rBV3	546	347	0.01%	0.002%
66	10.125	2807	2810	2814	rVB2	578	446	0.01%	0.002%
67	10.267	2840	2854	2888	rBV	564760	939984	25.73%	5.228%
68	10.428	2902	2904	2909	rVB3	603	374	0.01%	0.002%
69	10.479	2917	2920	2923	rVB3	379	285	0.01%	0.002%
70	10.601	2956	2958	2963	rBV2	640	560	0.02%	0.003%
71	10.797	3015	3019	3029	rVB3	657	888	0.02%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090618\
 Data File : VV007435.D
 Acq On : 06 Sep 2018 21:37
 Operator : SY/MD
 Sample : J4719-16 10X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGF2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

72	10.845	3030	3034	3036	rBV3	383	262	0.01%	0.001%
73	11.154	3127	3130	3133	rVB2	452	271	0.01%	0.002%
74	11.199	3140	3144	3146	rBV2	477	378	0.01%	0.002%
75	11.231	3150	3154	3156	rVV2	524	320	0.01%	0.002%
76	11.299	3161	3175	3206	rBV	664774	1138988	31.18%	6.335%
77	11.418	3210	3212	3219	rVB4	691	597	0.02%	0.003%
78	11.492	3233	3235	3238	rBV3	414	273	0.01%	0.002%
79	11.678	3279	3293	3320	rBV	655959	1119715	30.65%	6.228%
80	11.858	3346	3349	3352	rVB2	780	394	0.01%	0.002%
81	11.955	3377	3379	3384	rVB4	836	603	0.02%	0.003%
82	11.984	3384	3388	3390	rBV2	526	443	0.01%	0.002%
83	12.099	3421	3424	3428	rBV3	437	331	0.01%	0.002%
84	12.218	3458	3461	3464	rVB2	576	341	0.01%	0.002%
85	12.238	3464	3467	3472	rVV2	516	430	0.01%	0.002%
86	12.263	3472	3475	3479	rVB	488	417	0.01%	0.002%
87	12.373	3503	3509	3510	rBV3	440	413	0.01%	0.002%
88	12.466	3535	3538	3539	rBV	414	271	0.01%	0.002%
89	12.932	3680	3683	3684	rBV2	830	382	0.01%	0.002%
90	13.263	3783	3786	3789	rVB4	588	332	0.01%	0.002%
91	13.315	3798	3802	3803	rBV2	547	412	0.01%	0.002%
92	13.347	3810	3812	3816	rBV2	620	450	0.01%	0.003%
93	13.392	3824	3826	3828	rBV3	512	278	0.01%	0.002%
94	13.598	3888	3890	3895	rBV5	533	529	0.01%	0.003%
95	13.681	3913	3916	3919	rBV3	806	478	0.01%	0.003%
96	13.935	3993	3995	4000	rBV3	606	663	0.02%	0.004%
97	14.045	4026	4029	4030	rBV2	893	490	0.01%	0.003%
98	14.074	4036	4038	4040	rBV3	542	294	0.01%	0.002%
99	14.379	4131	4133	4138	rVB4	1086	690	0.02%	0.004%
100	14.559	4186	4189	4191	rBV3	861	541	0.01%	0.003%


Sum of corrected areas: 17978907

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV090618\
Data File : VV007435.D
Acq On : 06 Sep 2018 21:37
Operator : SY/MD
Sample : J4719-16 10X
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGF2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

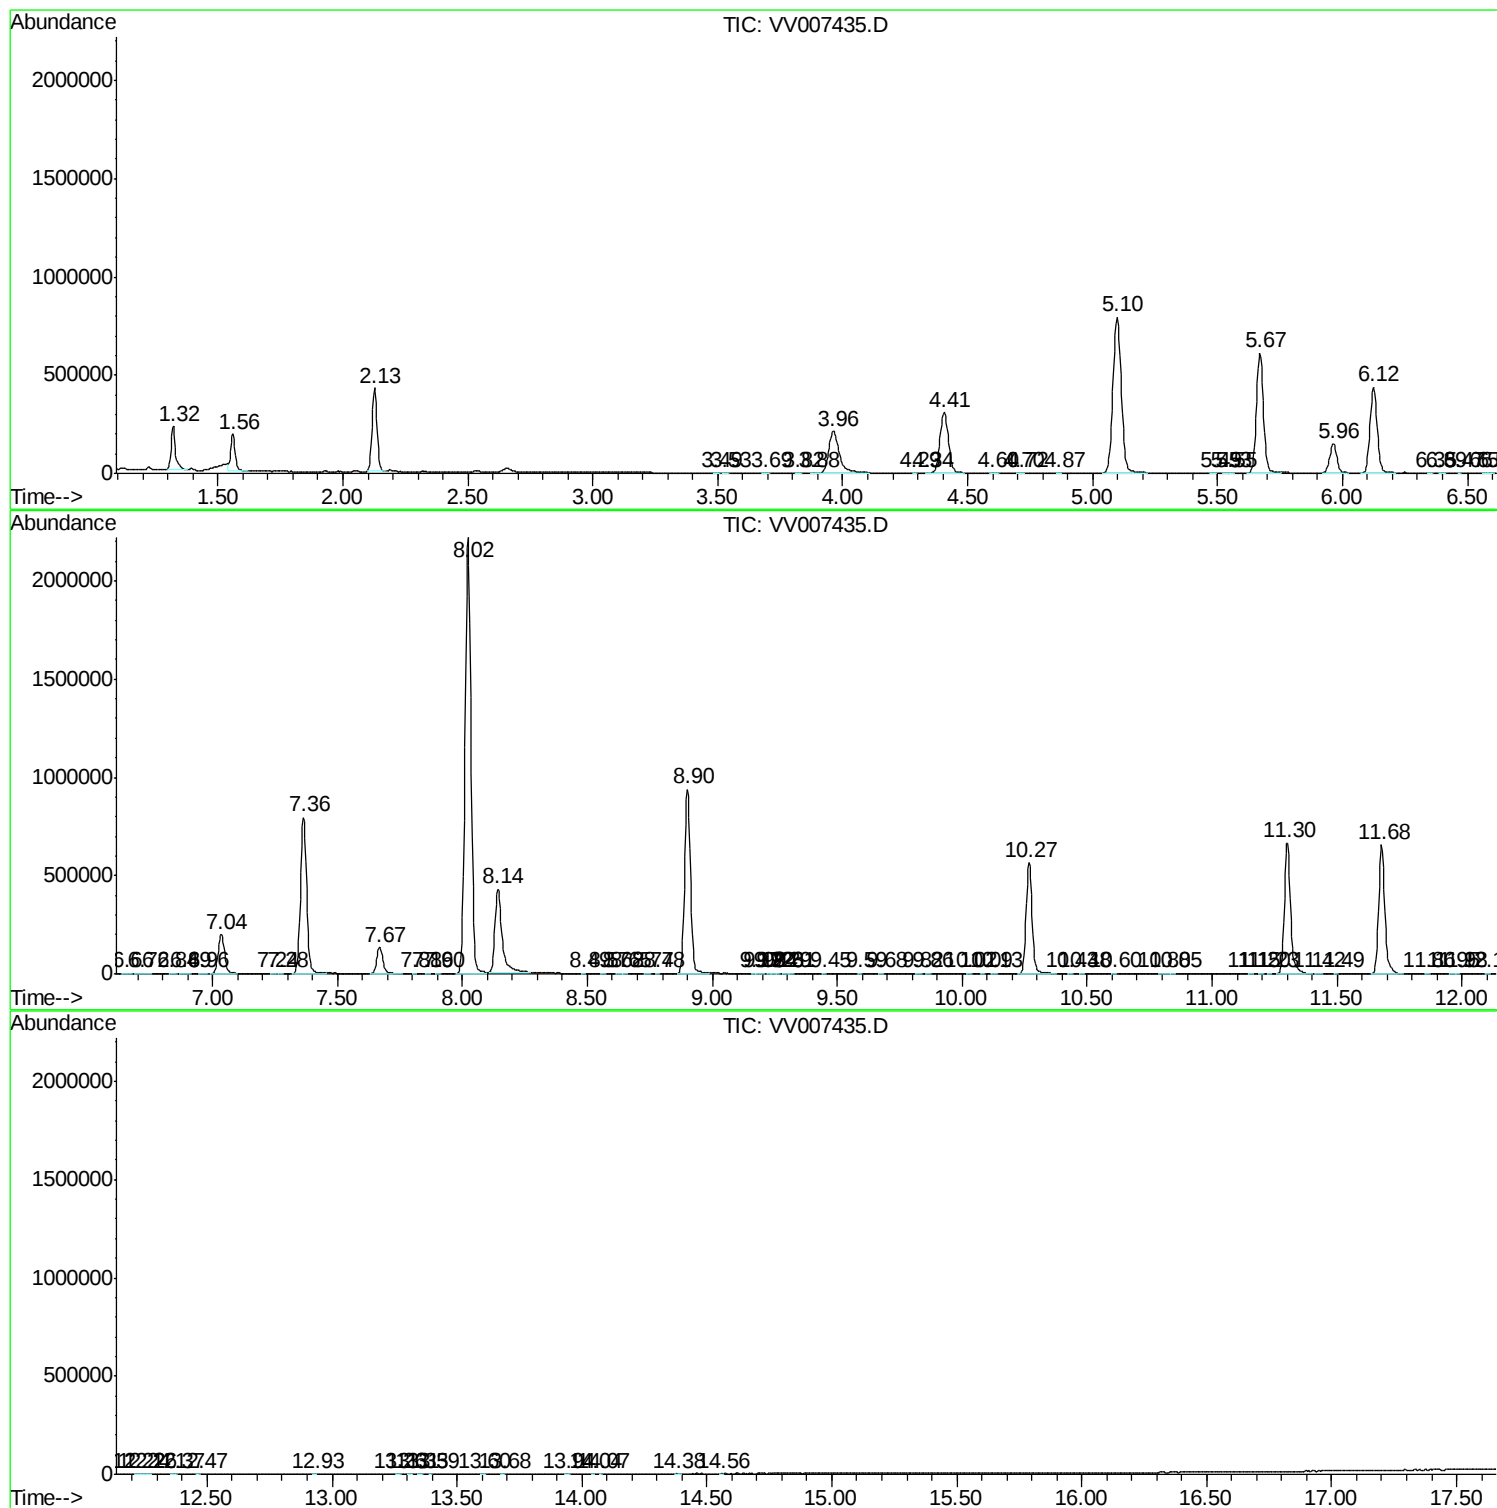

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV090618\
Data File : VV007435.D
Acq On : 06 Sep 2018 21:37
Operator : SY/MD
Sample : J4719-16 10X
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGF2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV090618\
Data File : VV007435.D
Acq On : 06 Sep 2018 21:37
Operator : SY/MD
Sample : J4719-16 10X
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGF2

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc