

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090618\
 Data File : VV007438.D
 Acq On : 06 Sep 2018 22:52
 Operator : SY/MD
 Sample : J4719-11
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGE7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	63	71	88	rVB	251378	301116	1.34%	0.654%
2	1.560	140	146	158	rVB	194648	237004	1.06%	0.515%
3	2.126	312	322	335	rBV	419855	596870	2.66%	1.297%
4	2.788	519	528	542	rVB	61941	104729	0.47%	0.228%
5	3.409	719	721	725	rVB2	599	398	0.00%	0.001%
6	3.560	764	768	772	rVB4	626	427	0.00%	0.001%
7	3.688	806	808	811	rVB2	607	329	0.00%	0.001%
8	3.746	821	826	827	rBV	289	239	0.00%	0.001%
9	3.814	844	847	854	rVB5	861	862	0.00%	0.002%
10	3.862	859	862	864	rBV	349	239	0.00%	0.001%
11	3.888	868	870	873	rBV2	342	245	0.00%	0.001%
12	3.965	873	894	923	rBV2	1270878	3109902	13.86%	6.756%
13	4.405	1013	1031	1055	rBV	310072	746018	3.33%	1.621%
14	4.508	1061	1063	1065	rBV3	449	260	0.00%	0.001%
15	4.640	1101	1104	1106	rBV4	729	507	0.00%	0.001%
16	4.720	1120	1129	1132	rBV6	3086	4407	0.02%	0.010%
17	4.826	1159	1162	1165	rBV	399	311	0.00%	0.001%
18	4.878	1175	1178	1181	rVB3	437	301	0.00%	0.001%
19	4.907	1185	1187	1191	rVB2	362	238	0.00%	0.001%
20	4.945	1191	1199	1202	rBV4	633	816	0.00%	0.002%
21	5.097	1228	1246	1278	rBV2	805084	1896387	8.45%	4.120%
22	5.277	1298	1302	1303	rBV3	973	663	0.00%	0.001%
23	5.347	1320	1324	1326	rBV2	325	256	0.00%	0.001%
24	5.373	1330	1332	1336	rVB3	347	250	0.00%	0.001%
25	5.428	1345	1349	1353	rVB3	401	369	0.00%	0.001%
26	5.537	1382	1383	1387	rVB2	594	284	0.00%	0.001%
27	5.588	1391	1399	1406	rBV7	1124	1799	0.01%	0.004%
28	5.669	1406	1424	1447	rBV	623776	1236513	5.51%	2.686%
29	5.961	1499	1515	1543	rBV	3428750	6517428	29.05%	14.159%
30	6.122	1552	1565	1598	rVB	442017	905085	4.03%	1.966%
31	6.376	1642	1644	1645	rBV2	700	330	0.00%	0.001%
32	6.524	1687	1690	1695	rBV4	654	586	0.00%	0.001%
33	6.550	1695	1698	1702	rVB4	594	451	0.00%	0.001%
34	6.621	1717	1720	1725	rVB5	573	581	0.00%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090618\
 Data File : VV007438.D
 Acq On : 06 Sep 2018 22:52
 Operator : SY/MD
 Sample : J4719-11
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGE7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

35	6.659	1725	1732	1737	rBV6	1240	1647	0.01%	0.004%
36	6.688	1739	1741	1744	rVB2	562	357	0.00%	0.001%
37	6.717	1744	1750	1752	rBV3	2135	2161	0.01%	0.005%
38	6.839	1786	1788	1792	rBV3	491	278	0.00%	0.001%
39	6.894	1802	1805	1808	rBV3	361	288	0.00%	0.001%
40	6.939	1815	1819	1824	rBV2	596	624	0.00%	0.001%
41	7.035	1835	1849	1875	rVV	203010	363906	1.62%	0.791%
42	7.125	1875	1877	1879	rBV2	655	360	0.00%	0.001%
43	7.363	1935	1951	1968	rBV	802735	1381973	6.16%	3.002%
44	7.624	2030	2032	2033	rBV	594	235	0.00%	0.001%
45	7.669	2034	2046	2064	rVV	151534	255799	1.14%	0.556%
46	7.801	2084	2087	2093	rVB4	944	990	0.00%	0.002%
47	7.859	2103	2105	2108	rBV5	562	333	0.00%	0.001%
48	7.926	2124	2126	2129	rVB3	630	250	0.00%	0.001%
49	7.958	2134	2136	2140	rBV2	583	552	0.00%	0.001%
50	8.022	2140	2156	2183	rBV	13487611	22432571	100.00%	48.734%
51	8.141	2183	2193	2236	rVB	494183	995176	4.44%	2.162%
52	8.498	2302	2304	2307	rVB2	650	327	0.00%	0.001%
53	8.788	2389	2394	2397	rBV3	558	550	0.00%	0.001%
54	8.826	2404	2406	2410	rBV2	361	251	0.00%	0.001%
55	8.900	2416	2429	2463	rBV	971802	1578240	7.04%	3.429%
56	9.154	2505	2508	2511	rBV3	584	457	0.00%	0.001%
57	9.183	2511	2517	2526	rVB6	1974	2962	0.01%	0.006%
58	9.238	2532	2534	2536	rBV2	561	307	0.00%	0.001%
59	9.479	2605	2609	2610	rBV2	543	384	0.00%	0.001%
60	9.592	2638	2644	2651	rBV5	1248	1676	0.01%	0.004%
61	9.640	2655	2659	2662	rBV3	575	480	0.00%	0.001%
62	9.672	2667	2669	2673	rVB3	485	268	0.00%	0.001%
63	9.711	2679	2681	2684	rVB2	665	344	0.00%	0.001%
64	9.733	2684	2688	2689	rBV2	446	279	0.00%	0.001%
65	9.868	2727	2730	2732	rBV3	489	388	0.00%	0.001%
66	9.907	2738	2742	2746	rVB2	454	379	0.00%	0.001%
67	9.932	2746	2750	2752	rBV2	378	265	0.00%	0.001%
68	9.974	2758	2763	2765	rBV3	530	572	0.00%	0.001%
69	9.990	2765	2768	2769	rVV2	420	258	0.00%	0.001%
70	10.000	2769	2771	2774	rVV2	463	324	0.00%	0.001%
71	10.141	2810	2815	2818	rBV3	595	408	0.00%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090618\
 Data File : VV007438.D
 Acq On : 06 Sep 2018 22:52
 Operator : SY/MD
 Sample : J4719-11
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGE7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

72	10.267	2842	2854	2885	rBV	580650	952569	4.25%	2.069%
73	10.656	2972	2975	2978	rVB2	485	353	0.00%	0.001%
74	10.694	2984	2987	2990	rVV2	438	306	0.00%	0.001%
75	10.791	3013	3017	3022	rBV3	503	521	0.00%	0.001%
76	10.813	3022	3024	3027	rVB2	458	244	0.00%	0.001%
77	10.846	3031	3034	3037	rBV3	352	266	0.00%	0.001%
78	10.884	3042	3046	3047	rBV2	609	365	0.00%	0.001%
79	10.939	3060	3063	3064	rBV2	417	241	0.00%	0.001%
80	10.952	3064	3067	3068	rBV2	454	257	0.00%	0.001%
81	11.103	3110	3114	3116	rBV4	479	448	0.00%	0.001%
82	11.157	3126	3131	3133	rVB2	399	292	0.00%	0.001%
83	11.215	3146	3149	3153	rBV2	480	467	0.00%	0.001%
84	11.238	3153	3156	3160	rVB	731	560	0.00%	0.001%
85	11.299	3162	3175	3205	rBV	715290	1209280	5.39%	2.627%
86	11.489	3232	3234	3236	rBV2	423	259	0.00%	0.001%
87	11.678	3279	3293	3317	rBV	681657	1162741	5.18%	2.526%
88	12.273	3475	3478	3480	rBV3	580	399	0.00%	0.001%
89	12.517	3551	3554	3556	rBV3	858	479	0.00%	0.001%
90	12.553	3562	3565	3569	rBV2	548	569	0.00%	0.001%
91	12.656	3593	3597	3600	rBV4	521	481	0.00%	0.001%
92	12.743	3621	3624	3628	rBV2	699	682	0.00%	0.001%
93	12.781	3634	3636	3637	rBV	663	284	0.00%	0.001%
94	12.984	3696	3699	3703	rVB2	950	634	0.00%	0.001%
95	13.009	3703	3707	3711	rBV3	615	581	0.00%	0.001%
96	13.630	3898	3900	3903	rBV3	411	238	0.00%	0.001%
97	13.665	3909	3911	3913	rBV3	491	280	0.00%	0.001%
98	13.781	3939	3947	3951	rBV7	1076	1550	0.01%	0.003%
99	14.427	4144	4148	4152	rVB5	1362	1161	0.01%	0.003%
100	14.450	4152	4155	4157	rBV2	1146	905	0.00%	0.002%


Sum of corrected areas: 46030231

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV090618\
Data File : VV007438.D
Acq On : 06 Sep 2018 22:52
Operator : SY/MD
Sample : J4719-11
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGE7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

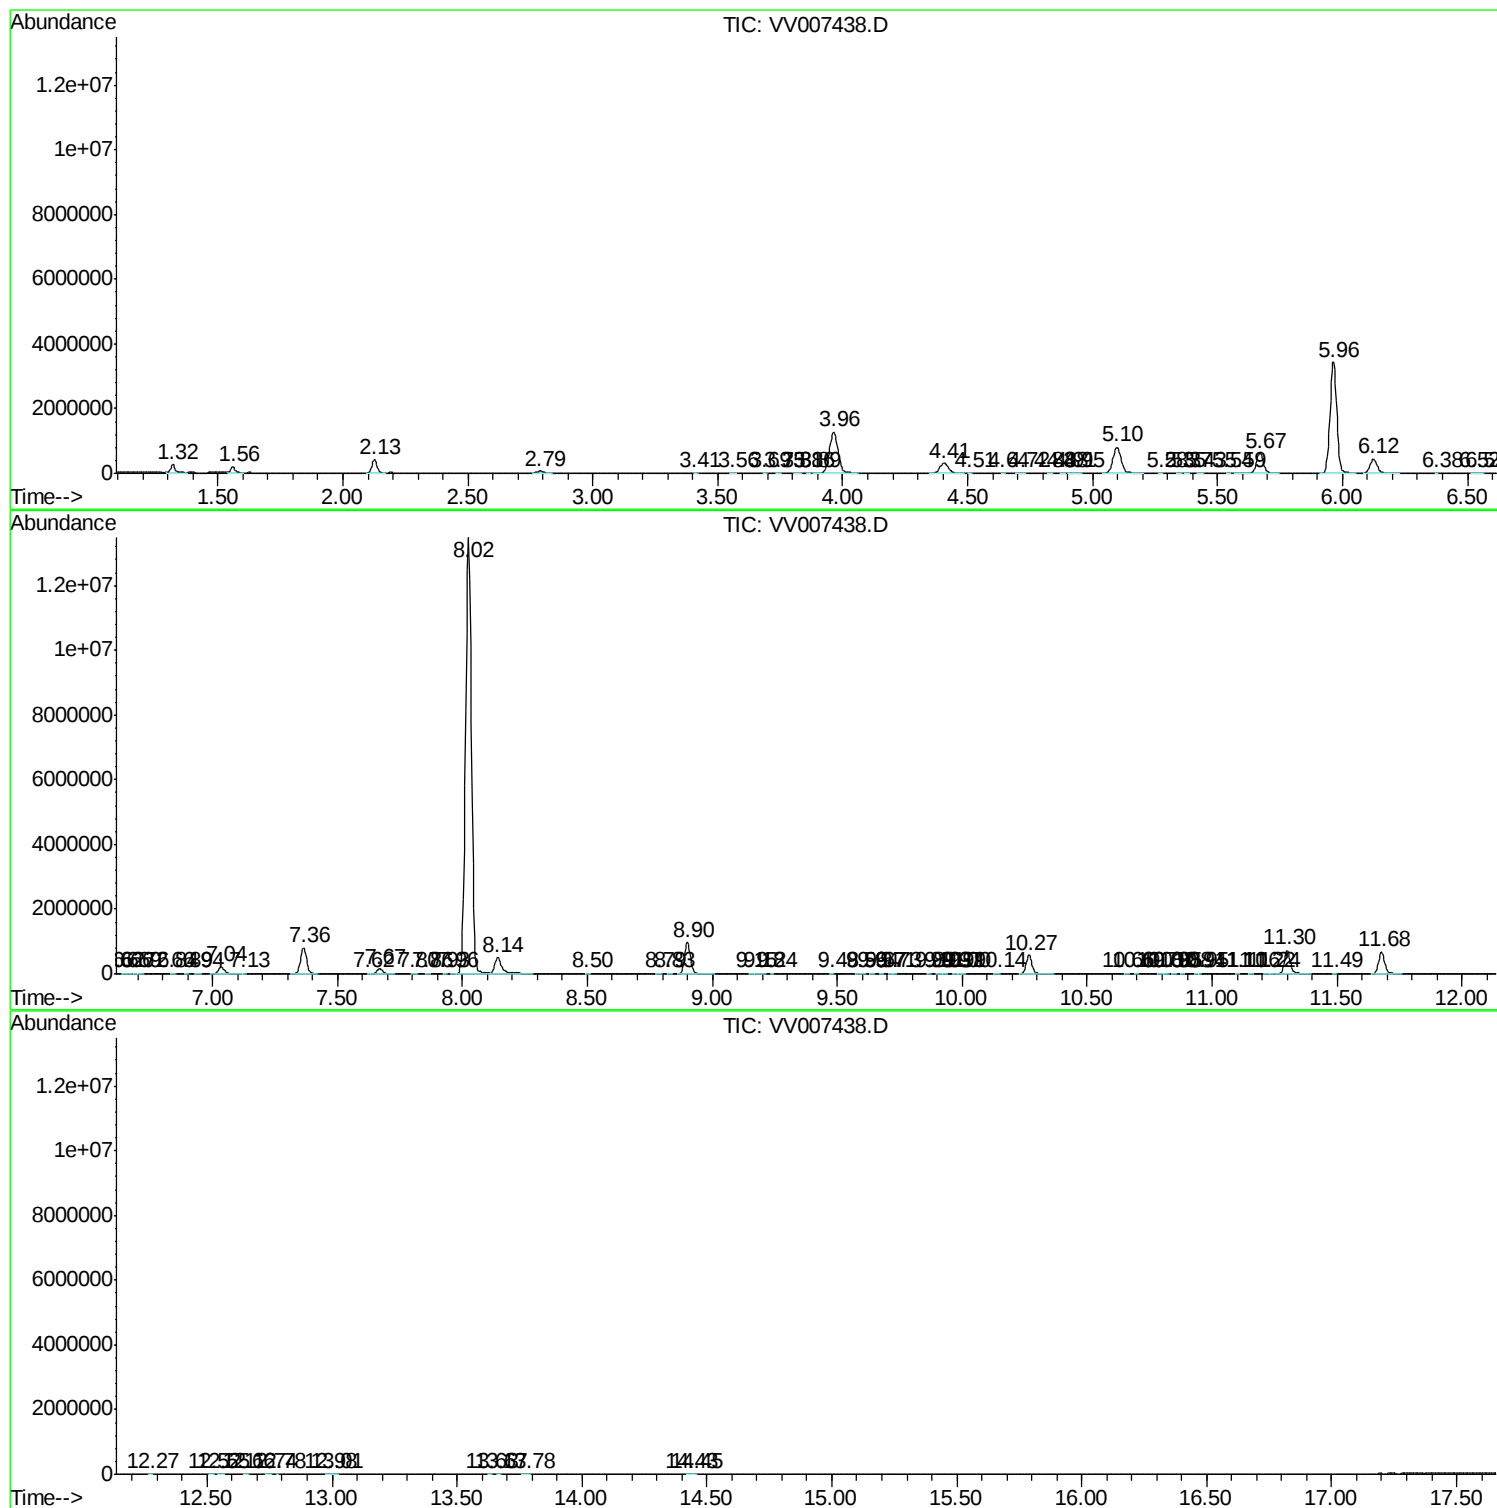

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV090618\
Data File : VV007438.D
Acq On : 06 Sep 2018 22:52
Operator : SY/MD
Sample : J4719-11
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGE7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV090618\
Data File : VV007438.D
Acq On : 06 Sep 2018 22:52
Operator : SY/MD
Sample : J4719-11
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGE7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc