

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090618\
 Data File : VV007439.D
 Acq On : 06 Sep 2018 23:17
 Operator : SY/MD
 Sample : J4719-12
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGE8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.322	64	72	88	rVV	232238	285148	2.22%	1.012%
2	1.392	89	94	105	rVB	34011	39097	0.30%	0.139%
3	1.560	141	146	161	rVB	188670	225364	1.75%	0.800%
4	2.126	312	322	334	rBV	424588	597783	4.65%	2.122%
5	3.344	698	701	705	rBV3	811	631	0.00%	0.002%
6	3.363	705	707	713	rVB3	1123	699	0.01%	0.002%
7	3.392	713	716	721	rVB6	859	746	0.01%	0.003%
8	3.463	735	738	741	rVB3	923	567	0.00%	0.002%
9	3.479	741	743	746	rBV2	454	336	0.00%	0.001%
10	3.495	746	748	752	rVB3	640	468	0.00%	0.002%
11	3.560	765	768	771	rVB2	635	384	0.00%	0.001%
12	3.595	775	779	782	rBV3	452	411	0.00%	0.001%
13	3.637	789	792	797	rBV2	570	472	0.00%	0.002%
14	3.720	816	818	823	rVB2	517	320	0.00%	0.001%
15	3.749	823	827	829	rBV3	689	615	0.00%	0.002%
16	3.765	829	832	836	rVB2	672	457	0.00%	0.002%
17	3.897	867	873	874	rVV2	574	482	0.00%	0.002%
18	3.961	875	893	935	rVV3	206140	595581	4.63%	2.114%
19	4.260	982	986	988	rBV3	483	397	0.00%	0.001%
20	4.289	993	995	998	rVB2	676	339	0.00%	0.001%
21	4.309	998	1001	1005	rBV2	657	573	0.00%	0.002%
22	4.405	1014	1031	1061	rVV	309595	754704	5.86%	2.679%
23	4.540	1070	1073	1076	rVB2	496	285	0.00%	0.001%
24	4.588	1086	1088	1092	rVB3	567	356	0.00%	0.001%
25	4.656	1105	1109	1119	rVB4	1660	2439	0.02%	0.009%
26	4.720	1125	1129	1130	rBV3	868	643	0.00%	0.002%
27	4.785	1145	1149	1151	rBV2	488	390	0.00%	0.001%
28	4.817	1156	1159	1163	rBV3	296	245	0.00%	0.001%
29	4.907	1184	1187	1190	rBV2	319	252	0.00%	0.001%
30	4.949	1195	1200	1203	rVB4	378	297	0.00%	0.001%
31	5.096	1227	1246	1276	rBV2	799818	1924825	14.96%	6.834%
32	5.347	1320	1324	1328	rVB2	529	438	0.00%	0.002%
33	5.389	1330	1337	1340	rBV3	760	742	0.01%	0.003%
34	5.566	1385	1392	1394	rBV4	550	551	0.00%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090618\
 Data File : VV007439.D
 Acq On : 06 Sep 2018 23:17
 Operator : SY/MD
 Sample : J4719-12
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGE8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

35	5.588	1394	1399	1400	rBV2	429	344	0.00%	0.001%
36	5.669	1408	1424	1447	rBV	619881	1238566	9.62%	4.397%
37	5.965	1501	1516	1533	rBV	385631	749757	5.83%	2.662%
38	6.125	1551	1566	1593	rVB	437459	880889	6.85%	3.127%
39	6.299	1617	1620	1621	rBV2	594	372	0.00%	0.001%
40	6.312	1621	1624	1627	rVB4	957	651	0.01%	0.002%
41	6.614	1716	1718	1722	rVB2	396	258	0.00%	0.001%
42	6.643	1722	1727	1730	rBV5	903	773	0.01%	0.003%
43	6.720	1742	1751	1759	rBV5	2187	3946	0.03%	0.014%
44	6.852	1786	1792	1795	rBV3	503	497	0.00%	0.002%
45	6.875	1795	1799	1800	rBV2	392	302	0.00%	0.001%
46	6.923	1811	1814	1819	rVB4	531	475	0.00%	0.002%
47	6.952	1819	1823	1826	rBV4	528	297	0.00%	0.001%
48	7.035	1836	1849	1871	rVV	202466	361423	2.81%	1.283%
49	7.244	1909	1914	1915	rBV2	506	359	0.00%	0.001%
50	7.363	1936	1951	1973	rBV	796634	1391578	10.81%	4.940%
51	7.617	2028	2030	2034	rBV4	477	389	0.00%	0.001%
52	7.669	2034	2046	2064	rBV	153683	257466	2.00%	0.914%
53	8.022	2139	2156	2182	rBV	7777903	12869084	100.00%	45.689%
54	8.141	2183	2193	2238	rVB	482882	975385	7.58%	3.463%
55	8.649	2349	2351	2355	rVB4	494	263	0.00%	0.001%
56	8.723	2372	2374	2380	rVB4	612	536	0.00%	0.002%
57	8.804	2396	2399	2402	rBV3	446	383	0.00%	0.001%
58	8.823	2403	2405	2408	rVB2	610	326	0.00%	0.001%
59	8.900	2416	2429	2448	rBV	972302	1577120	12.26%	5.599%
60	9.148	2502	2506	2509	rVB3	391	289	0.00%	0.001%
61	9.170	2509	2513	2514	rBV2	841	562	0.00%	0.002%
62	9.267	2526	2543	2567	rBV4	10835	48461	0.38%	0.172%
63	9.450	2597	2600	2602	rBV3	480	293	0.00%	0.001%
64	9.591	2641	2644	2648	rVV4	523	436	0.00%	0.002%
65	9.649	2656	2662	2665	rBV3	704	735	0.01%	0.003%
66	9.665	2665	2667	2673	rBV5	471	372	0.00%	0.001%
67	9.810	2709	2712	2716	rVB3	444	315	0.00%	0.001%
68	9.836	2716	2720	2724	rVB2	460	384	0.00%	0.001%
69	9.897	2736	2739	2742	rBV2	657	442	0.00%	0.002%
70	10.000	2767	2771	2775	rVB3	562	383	0.00%	0.001%
71	10.026	2775	2779	2782	rVB3	487	394	0.00%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090618\
 Data File : VV007439.D
 Acq On : 06 Sep 2018 23:17
 Operator : SY/MD
 Sample : J4719-12
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGE8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

72	10.048	2782	2786	2787	rBV3	333	244	0.00%	0.001%
73	10.090	2796	2799	2802	rVB3	438	322	0.00%	0.001%
74	10.132	2806	2812	2813	rBV3	303	348	0.00%	0.001%
75	10.267	2839	2854	2886	rVV	594451	966836	7.51%	3.433%
76	10.427	2901	2904	2912	rVB2	1109	1253	0.01%	0.004%
77	10.482	2915	2921	2923	rBV3	369	291	0.00%	0.001%
78	10.662	2974	2977	2982	rVB3	398	327	0.00%	0.001%
79	10.704	2988	2990	2993	rBV	393	255	0.00%	0.001%
80	10.807	3020	3022	3027	rVB3	472	286	0.00%	0.001%
81	10.903	3048	3052	3055	rBV4	749	645	0.01%	0.002%
82	10.984	3072	3077	3079	rBV4	600	599	0.00%	0.002%
83	11.087	3104	3109	3114	rBV5	370	497	0.00%	0.002%
84	11.122	3116	3120	3127	rBV3	662	605	0.00%	0.002%
85	11.199	3141	3144	3146	rBV3	535	293	0.00%	0.001%
86	11.299	3163	3175	3205	rBV	715524	1209448	9.40%	4.294%
87	11.514	3240	3242	3245	rBV2	375	260	0.00%	0.001%
88	11.585	3258	3264	3266	rBV3	757	881	0.01%	0.003%
89	11.678	3280	3293	3321	rBV	695866	1177112	9.15%	4.179%
90	11.833	3339	3341	3345	rBV	665	384	0.00%	0.001%
91	11.906	3361	3364	3365	rBV	550	304	0.00%	0.001%
92	12.138	3434	3436	3440	rVB2	490	292	0.00%	0.001%
93	12.431	3524	3527	3531	rBV3	499	417	0.00%	0.001%
94	12.456	3531	3535	3537	rBV3	573	517	0.00%	0.002%
95	12.517	3551	3554	3555	rBV	540	322	0.00%	0.001%
96	12.765	3629	3631	3634	rBV4	410	276	0.00%	0.001%
97	12.923	3677	3680	3682	rBV2	576	473	0.00%	0.002%
98	13.070	3723	3726	3728	rVB3	686	338	0.00%	0.001%
99	13.296	3792	3796	3798	rBV2	698	535	0.00%	0.002%
100	14.733	4240	4243	4246	rBV4	1219	907	0.01%	0.003%


Sum of corrected areas: 28166809

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV090618\
Data File : VV007439.D
Acq On : 06 Sep 2018 23:17
Operator : SY/MD
Sample : J4719-12
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGE8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

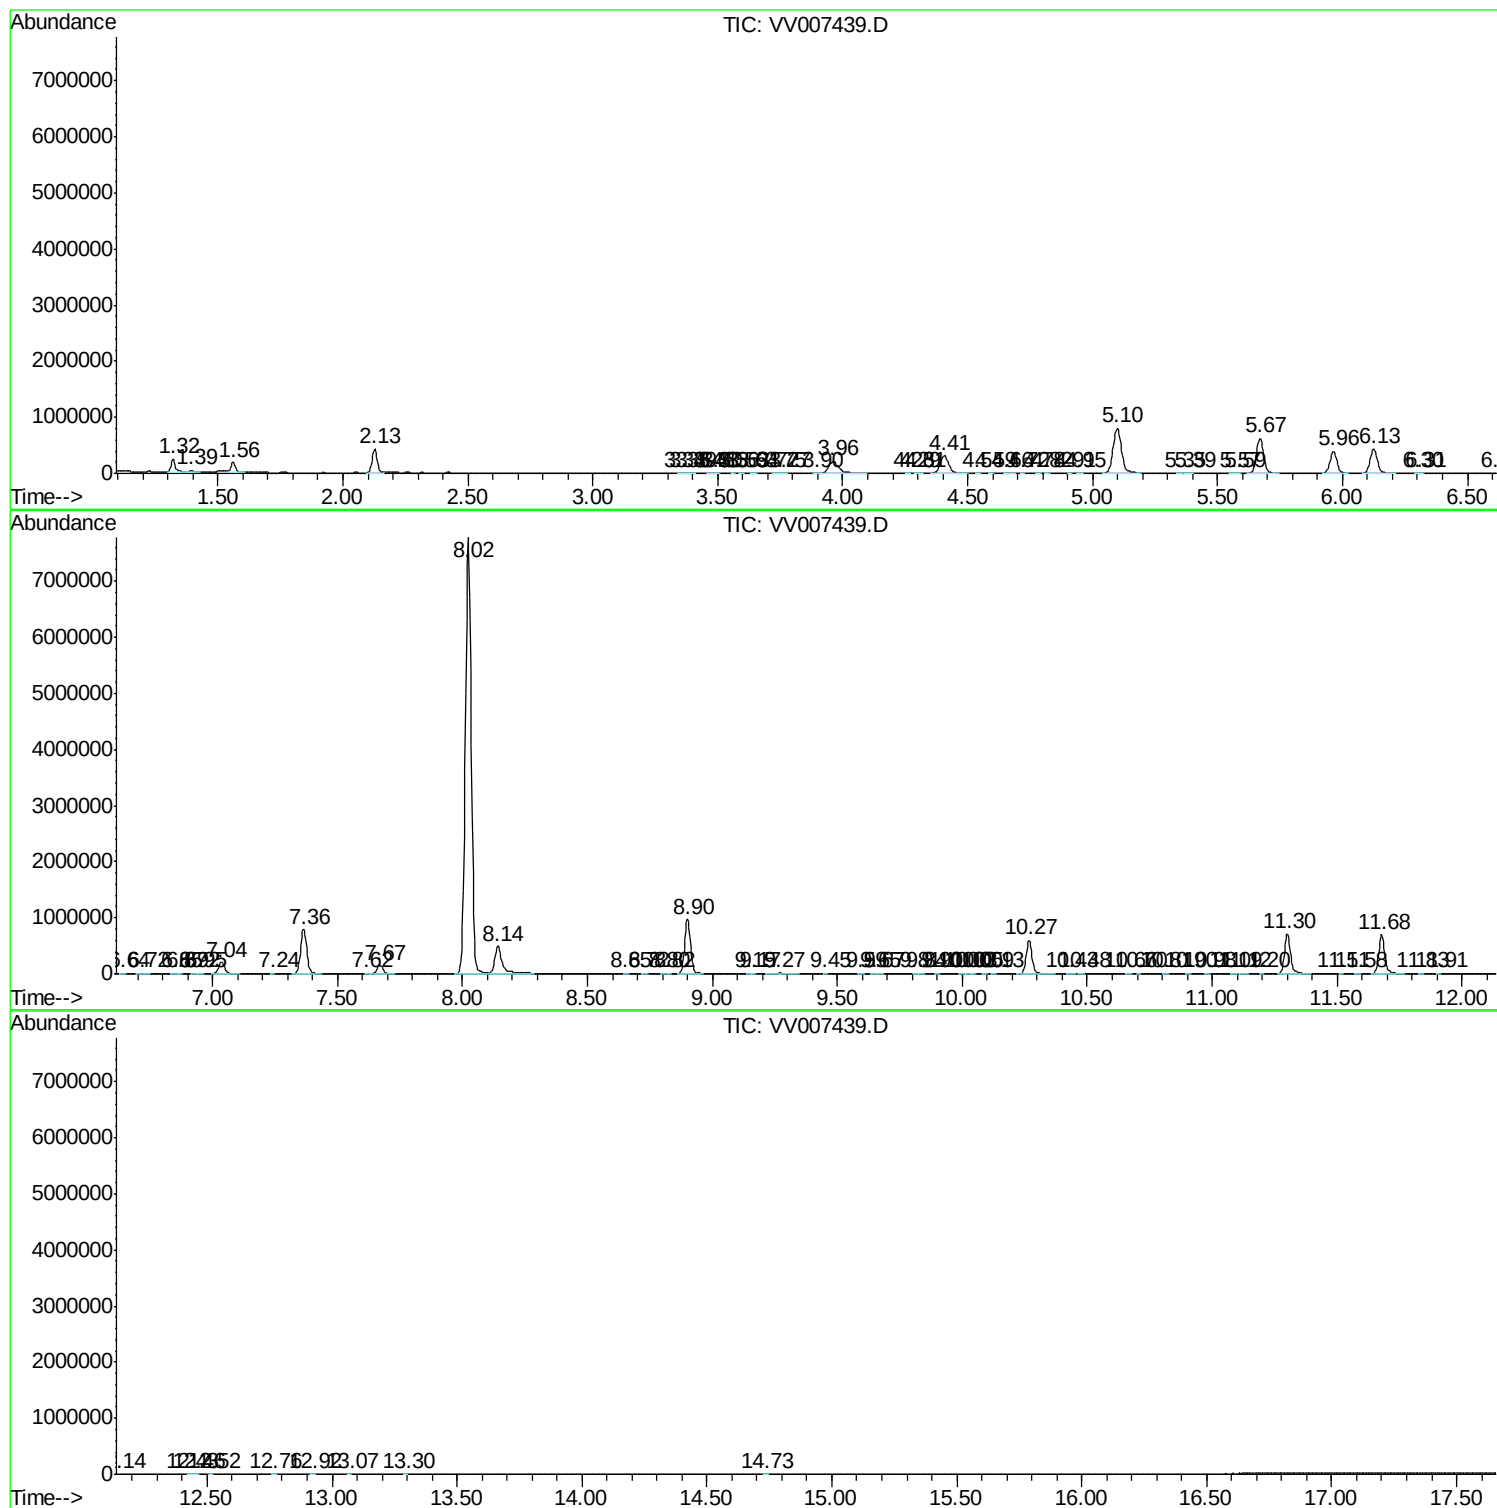

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV090618\
Data File : VV007439.D
Acq On : 06 Sep 2018 23:17
Operator : SY/MD
Sample : J4719-12
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGE8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV090618\
Data File : VV007439.D
Acq On : 06 Sep 2018 23:17
Operator : SY/MD
Sample : J4719-12
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGE8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
