

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090618\
 Data File : VV007442.D
 Acq On : 07 Sep 2018 01:22
 Operator : SY/MD
 Sample : VV0906WBL02
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK77

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	63	71	86	rVB	248748	288829	14.66%	2.012%
2	1.557	140	145	165	rVB	207906	260456	13.22%	1.815%
3	2.126	312	322	335	rBV	447991	630006	31.97%	4.390%
4	3.698	810	811	817	rVB2	736	526	0.03%	0.004%
5	3.746	817	826	830	rBV4	553	857	0.04%	0.006%
6	3.962	875	893	938	rBV3	126775	449517	22.81%	3.132%
7	4.405	1013	1031	1058	rBV	325005	775026	39.33%	5.400%
8	4.540	1071	1073	1076	rVB2	640	296	0.02%	0.002%
9	4.611	1091	1095	1100	rBV3	438	431	0.02%	0.003%
10	4.634	1100	1102	1107	rBV3	518	404	0.02%	0.003%
11	4.691	1117	1120	1123	rBV2	370	294	0.01%	0.002%
12	4.711	1123	1126	1127	rBV	679	351	0.02%	0.002%
13	4.833	1161	1164	1167	rBV2	379	318	0.02%	0.002%
14	4.875	1175	1177	1184	rVB2	483	491	0.02%	0.003%
15	4.910	1184	1188	1189	rBV2	455	317	0.02%	0.002%
16	4.949	1195	1200	1203	rBV2	436	344	0.02%	0.002%
17	5.097	1228	1246	1295	rBV2	843460	1970540	100.00%	13.730%
18	5.325	1311	1317	1319	rBV4	564	586	0.03%	0.004%
19	5.389	1334	1337	1341	rVB4	506	368	0.02%	0.003%
20	5.441	1349	1353	1359	rVB4	598	540	0.03%	0.004%
21	5.505	1368	1373	1376	rBV3	934	691	0.04%	0.005%
22	5.553	1384	1388	1391	rBV2	398	330	0.02%	0.002%
23	5.669	1406	1424	1444	rBV	617267	1212097	61.51%	8.445%
24	5.949	1500	1511	1527	rVB5	12415	26077	1.32%	0.182%
25	6.122	1550	1565	1589	rBV	454945	915718	46.47%	6.380%
26	6.466	1670	1672	1675	rVB3	587	339	0.02%	0.002%
27	6.492	1675	1680	1682	rBV2	401	390	0.02%	0.003%
28	6.531	1690	1692	1698	rVB4	788	791	0.04%	0.006%
29	6.563	1698	1702	1703	rBV2	425	277	0.01%	0.002%
30	6.579	1703	1707	1712	rVB4	616	475	0.02%	0.003%
31	6.608	1712	1716	1721	rVB3	660	652	0.03%	0.005%
32	6.633	1721	1724	1726	rBV2	516	348	0.02%	0.002%
33	6.727	1743	1753	1763	rBV4	2792	4570	0.23%	0.032%
34	6.836	1785	1787	1792	rVB2	415	297	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090618\
 Data File : VV007442.D
 Acq On : 07 Sep 2018 01:22
 Operator : SY/MD
 Sample : VV0906WBL02
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK77

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

35	6.868	1794	1797	1800	rVB2	533	287	0.01%	0.002%
36	6.920	1809	1813	1815	rBV3	582	421	0.02%	0.003%
37	6.945	1815	1821	1822	rBV2	443	318	0.02%	0.002%
38	6.968	1825	1828	1830	rBV2	466	307	0.02%	0.002%
39	7.035	1835	1849	1871	rBV	206385	371453	18.85%	2.588%
40	7.170	1889	1891	1896	rVB2	865	489	0.02%	0.003%
41	7.228	1907	1909	1914	rVB2	760	594	0.03%	0.004%
42	7.254	1914	1917	1921	rBV4	603	565	0.03%	0.004%
43	7.289	1923	1928	1931	rVV4	629	645	0.03%	0.004%
44	7.363	1936	1951	1968	rBV	835326	1438405	73.00%	10.022%
45	7.521	1998	2000	2005	rVB4	1087	750	0.04%	0.005%
46	7.669	2033	2046	2069	rBV	154429	261352	13.26%	1.821%
47	7.836	2095	2098	2104	rBV5	786	1097	0.06%	0.008%
48	7.894	2113	2116	2119	rBV2	725	530	0.03%	0.004%
49	7.984	2140	2144	2147	rBV3	1474	1368	0.07%	0.010%
50	8.019	2147	2155	2169	rVB3	10711	18161	0.92%	0.127%
51	8.096	2176	2179	2181	rBV2	532	364	0.02%	0.003%
52	8.141	2181	2193	2239	rVV2	442898	904056	45.88%	6.299%
53	8.466	2292	2294	2299	rVB5	599	397	0.02%	0.003%
54	8.601	2333	2336	2343	rBV6	541	540	0.03%	0.004%
55	8.666	2353	2356	2360	rVB4	517	337	0.02%	0.002%
56	8.707	2363	2369	2370	rBV2	704	559	0.03%	0.004%
57	8.801	2394	2398	2400	rBV3	534	375	0.02%	0.003%
58	8.900	2413	2429	2454	rBV	932334	1502494	76.25%	10.469%
59	9.190	2515	2519	2524	rVB4	955	933	0.05%	0.007%
60	9.248	2533	2537	2544	rVB2	497	482	0.02%	0.003%
61	9.309	2554	2556	2558	rBV2	587	294	0.01%	0.002%
62	9.373	2573	2576	2580	rBV2	529	360	0.02%	0.003%
63	9.453	2598	2601	2606	rVV2	390	345	0.02%	0.002%
64	9.527	2620	2624	2627	rVB2	452	367	0.02%	0.003%
65	9.559	2630	2634	2638	rVB3	304	301	0.02%	0.002%
66	9.598	2642	2646	2648	rBV5	934	724	0.04%	0.005%
67	9.701	2675	2678	2683	rVB3	422	395	0.02%	0.003%
68	9.836	2716	2720	2726	rVB2	432	461	0.02%	0.003%
69	9.874	2726	2732	2734	rBV3	488	421	0.02%	0.003%
70	9.952	2754	2756	2759	rBV	471	328	0.02%	0.002%
71	10.141	2808	2815	2816	rBV3	293	316	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090618\
 Data File : VV007442.D
 Acq On : 07 Sep 2018 01:22
 Operator : SY/MD
 Sample : VV0906WBL02
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK77

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

72	10.267	2841	2854	2888	rVV	603665	984616	49.97%	6.860%
73	10.434	2897	2906	2910	rBV5	571	978	0.05%	0.007%
74	10.498	2924	2926	2935	rVB2	627	738	0.04%	0.005%
75	10.537	2935	2938	2941	rBV	501	349	0.02%	0.002%
76	10.579	2948	2951	2954	rBV2	379	299	0.02%	0.002%
77	10.736	2996	3000	3002	rBV2	468	446	0.02%	0.003%
78	10.791	3012	3017	3020	rBV3	456	523	0.03%	0.004%
79	10.820	3024	3026	3029	rVB2	573	275	0.01%	0.002%
80	10.897	3046	3050	3052	rVV2	380	282	0.01%	0.002%
81	10.910	3052	3054	3061	rVB4	437	299	0.02%	0.002%
82	10.993	3078	3080	3083	rVB2	573	296	0.02%	0.002%
83	11.013	3083	3086	3088	rBV3	777	511	0.03%	0.004%
84	11.038	3092	3094	3098	rVB3	423	277	0.01%	0.002%
85	11.228	3147	3153	3162	rVV4	1709	2634	0.13%	0.018%
86	11.299	3162	3175	3202	rBV	653738	1114384	56.55%	7.765%
87	11.479	3228	3231	3236	rVB4	679	425	0.02%	0.003%
88	11.678	3280	3293	3319	rBV	686496	1174213	59.59%	8.181%
89	11.907	3362	3364	3371	rVV3	669	478	0.02%	0.003%
90	11.942	3371	3375	3378	rVB4	409	317	0.02%	0.002%
91	12.080	3411	3418	3422	rBV3	513	709	0.04%	0.005%
92	12.132	3430	3434	3439	rVB4	752	841	0.04%	0.006%
93	12.421	3521	3524	3528	rBV2	560	329	0.02%	0.002%
94	12.440	3528	3530	3533	rBV3	542	307	0.02%	0.002%
95	12.698	3604	3610	3614	rBV4	2007	2242	0.11%	0.016%
96	12.865	3657	3662	3664	rBV3	743	670	0.03%	0.005%
97	13.308	3796	3800	3801	rBV4	1266	865	0.04%	0.006%
98	13.562	3872	3879	3888	rBV2	3822	5542	0.28%	0.039%
99	13.804	3948	3954	3959	rBV6	2164	2634	0.13%	0.018%
100	14.424	4145	4147	4150	rBV2	692	470	0.02%	0.003%


Sum of corrected areas: 14352089

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV090618\
Data File : VV007442.D
Acq On : 07 Sep 2018 01:22
Operator : SY/MD
Sample : VV0906WBL02
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK77

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

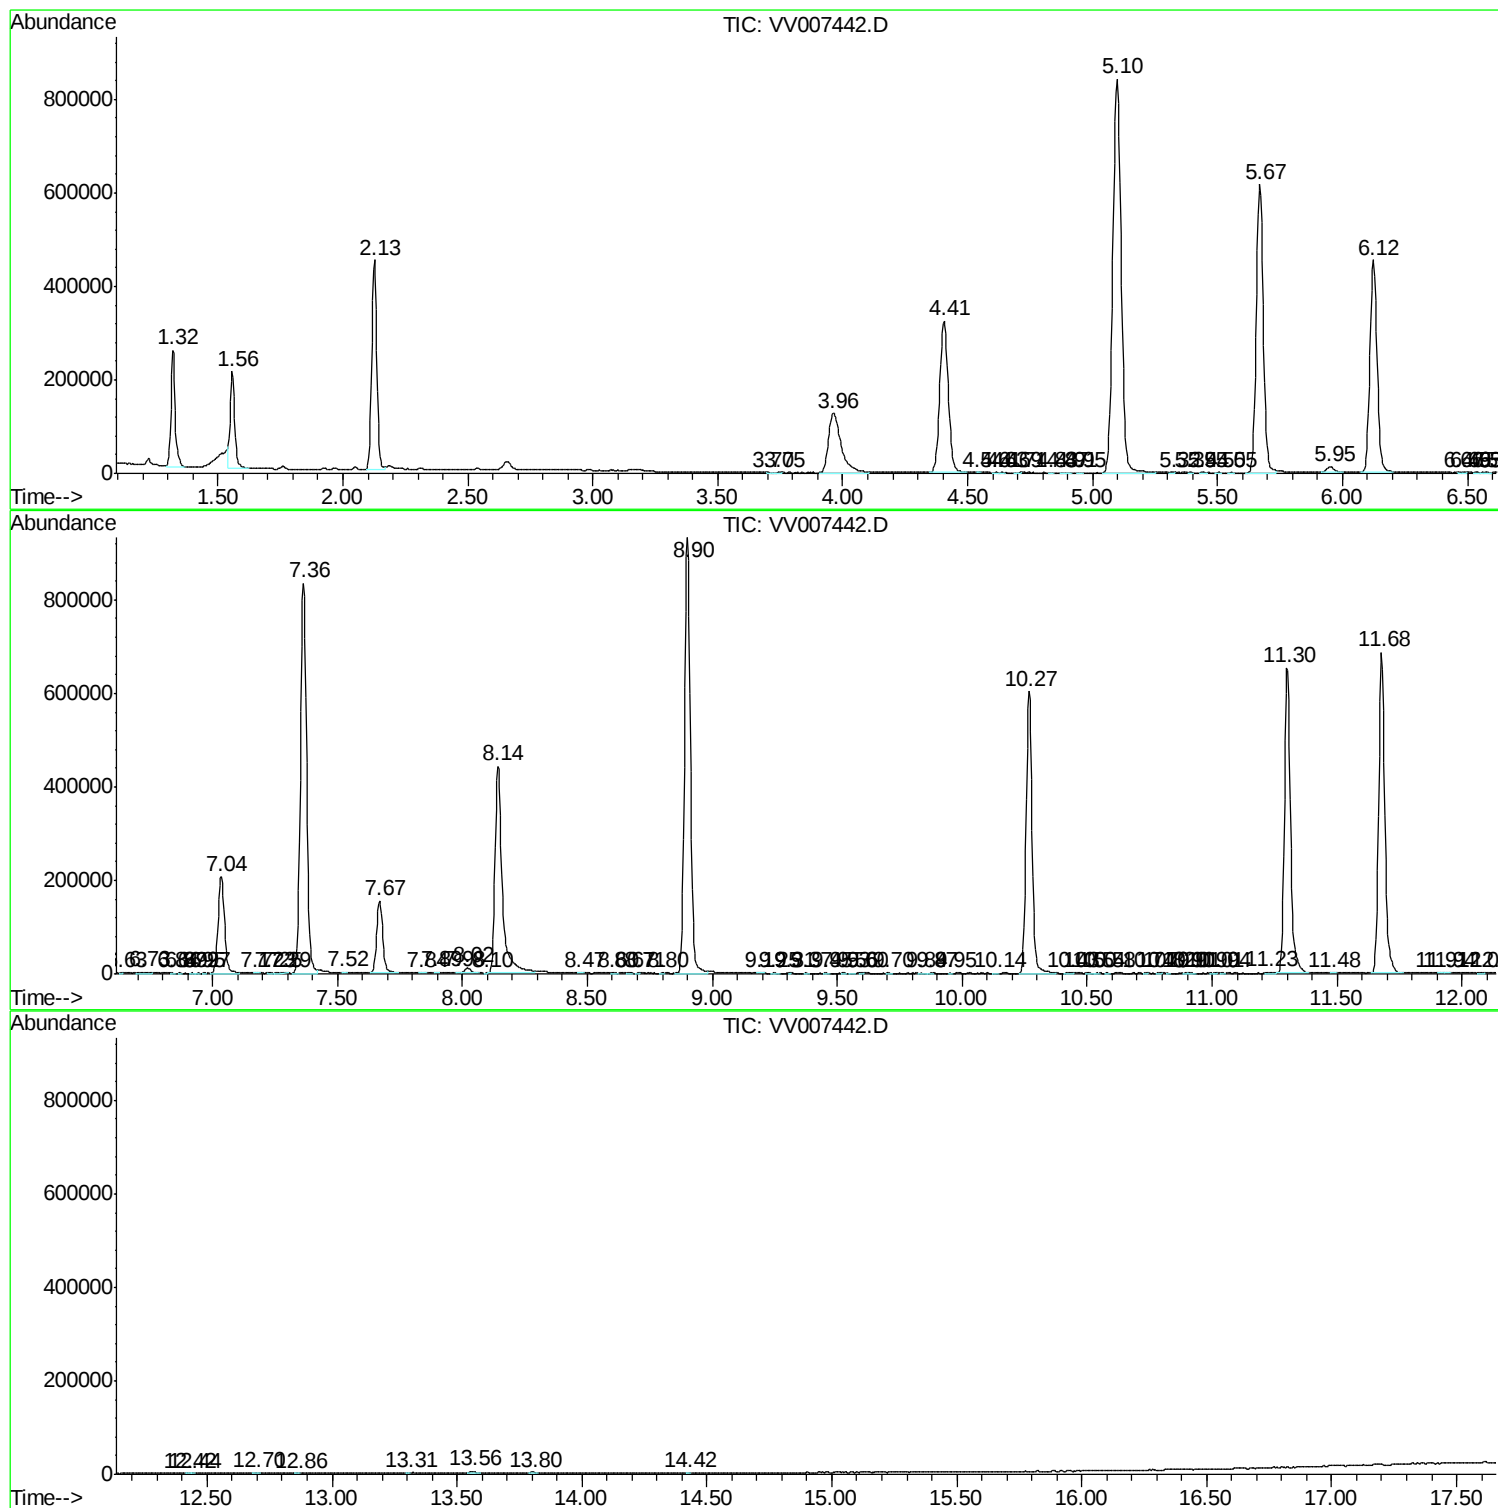

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV090618\
Data File : VV007442.D
Acq On : 07 Sep 2018 01:22
Operator : SY/MD
Sample : VV0906WBL02
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK77

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV090618\
Data File : VV007442.D
Acq On : 07 Sep 2018 01:22
Operator : SY/MD
Sample : VV0906WBL02
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK77

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc