

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090618\
 Data File : VV007443.D
 Acq On : 07 Sep 2018 01:47
 Operator : SY/MD
 Sample : J4751-01DL 500X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGH2DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	63	71	87	rVB	219934	259621	13.77%	1.899%
2	1.557	140	145	160	rVB	191285	236143	12.52%	1.727%
3	2.126	312	322	334	rBV	411401	576676	30.59%	4.218%
4	2.656	478	487	500	rVB	27820	54408	2.89%	0.398%
5	3.569	768	771	774	rBV2	431	274	0.01%	0.002%
6	3.749	824	827	835	rBV2	712	698	0.04%	0.005%
7	3.843	852	856	861	rVB4	355	300	0.02%	0.002%
8	3.884	866	869	872	rBV3	385	301	0.02%	0.002%
9	3.962	873	893	932	rBV2	125448	443999	23.55%	3.247%
10	4.290	992	995	998	rBV3	502	366	0.02%	0.003%
11	4.331	1005	1008	1011	rBV3	480	283	0.02%	0.002%
12	4.405	1011	1031	1056	rBV	309990	746152	39.57%	5.457%
13	4.569	1080	1082	1086	rVB3	454	318	0.02%	0.002%
14	4.659	1107	1110	1112	rBV2	405	262	0.01%	0.002%
15	4.724	1127	1130	1132	rVB5	835	505	0.03%	0.004%
16	4.807	1153	1156	1161	rBV2	349	337	0.02%	0.002%
17	4.900	1182	1185	1187	rBV	384	259	0.01%	0.002%
18	4.923	1190	1192	1195	rVB2	530	270	0.01%	0.002%
19	4.942	1195	1198	1201	rBV2	760	514	0.03%	0.004%
20	4.978	1207	1209	1215	rVB3	494	462	0.02%	0.003%
21	5.010	1215	1219	1221	rBV2	502	335	0.02%	0.002%
22	5.029	1221	1225	1228	rBV	386	270	0.01%	0.002%
23	5.097	1228	1246	1282	rBV2	800660	1885468	100.00%	13.790%
24	5.296	1306	1308	1312	rVB4	551	345	0.02%	0.003%
25	5.347	1321	1324	1326	rBV2	516	407	0.02%	0.003%
26	5.418	1343	1346	1349	rVB2	467	310	0.02%	0.002%
27	5.450	1349	1356	1360	rBV3	982	1212	0.06%	0.009%
28	5.476	1360	1364	1369	rVB3	920	829	0.04%	0.006%
29	5.518	1374	1377	1380	rVV4	392	263	0.01%	0.002%
30	5.566	1389	1392	1397	rBV3	481	366	0.02%	0.003%
31	5.598	1397	1402	1404	rBV2	404	348	0.02%	0.003%
32	5.669	1407	1424	1456	rBV	607815	1203568	63.83%	8.803%
33	5.949	1501	1511	1526	rVB8	11161	23955	1.27%	0.175%
34	6.122	1550	1565	1595	rBV	440391	883286	46.85%	6.460%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090618\
 Data File : VV007443.D
 Acq On : 07 Sep 2018 01:47
 Operator : SY/MD
 Sample : J4751-01DL 500X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGH2DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

35	6.379	1643	1645	1653	rVB5	607	600	0.03%	0.004%
36	6.466	1670	1672	1676	rVB2	616	324	0.02%	0.002%
37	6.515	1684	1687	1691	rBV3	571	446	0.02%	0.003%
38	6.550	1696	1698	1701	rVV3	681	395	0.02%	0.003%
39	6.582	1705	1708	1709	rVV2	411	257	0.01%	0.002%
40	6.656	1729	1731	1733	rVB3	800	358	0.02%	0.003%
41	6.727	1744	1753	1758	rBV3	2796	3730	0.20%	0.027%
42	6.826	1781	1784	1786	rBV	470	266	0.01%	0.002%
43	6.842	1786	1789	1796	rVB4	443	439	0.02%	0.003%
44	7.035	1835	1849	1865	rBV	195660	348752	18.50%	2.551%
45	7.241	1909	1913	1914	rBV2	498	325	0.02%	0.002%
46	7.273	1919	1923	1924	rBV3	624	439	0.02%	0.003%
47	7.363	1937	1951	1968	rBV	746829	1290286	68.43%	9.437%
48	7.669	2032	2046	2064	rBV	146366	247634	13.13%	1.811%
49	7.839	2096	2099	2103	rBV2	526	467	0.02%	0.003%
50	7.984	2139	2144	2147	rBV4	1213	1605	0.09%	0.012%
51	8.022	2147	2156	2168	rVB2	16720	27924	1.48%	0.204%
52	8.090	2173	2177	2181	rBV3	542	613	0.03%	0.004%
53	8.141	2181	2193	2235	rBV2	424915	878525	46.59%	6.426%
54	8.531	2311	2314	2319	rVB5	819	705	0.04%	0.005%
55	8.553	2319	2321	2324	rBV2	384	278	0.01%	0.002%
56	8.730	2374	2376	2380	rVV	522	379	0.02%	0.003%
57	8.826	2403	2406	2409	rVB2	375	254	0.01%	0.002%
58	8.900	2412	2429	2460	rBV	887618	1441353	76.45%	10.542%
59	9.183	2514	2517	2522	rVV3	941	767	0.04%	0.006%
60	9.241	2531	2535	2539	rBV3	775	542	0.03%	0.004%
61	9.321	2558	2560	2568	rVB2	578	653	0.03%	0.005%
62	9.373	2572	2576	2579	rBV3	417	357	0.02%	0.003%
63	9.392	2579	2582	2588	rVB3	627	587	0.03%	0.004%
64	9.521	2617	2622	2623	rBV2	509	366	0.02%	0.003%
65	9.566	2632	2636	2638	rVB4	387	291	0.02%	0.002%
66	9.611	2643	2650	2654	rVB3	1162	1341	0.07%	0.010%
67	9.646	2654	2661	2663	rBV	250	286	0.02%	0.002%
68	9.669	2663	2668	2671	rBV3	268	276	0.01%	0.002%
69	9.707	2675	2680	2682	rVV2	318	324	0.02%	0.002%
70	9.791	2703	2706	2709	rBV3	368	305	0.02%	0.002%
71	9.817	2711	2714	2718	rBV2	405	292	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090618\
 Data File : VV007443.D
 Acq On : 07 Sep 2018 01:47
 Operator : SY/MD
 Sample : J4751-01DL 500X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGH2DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

72	9.910	2739	2743	2750	rBV2	521	570	0.03%	0.004%
73	9.942	2750	2753	2756	rVB3	464	325	0.02%	0.002%
74	9.965	2756	2760	2762	rBV	627	429	0.02%	0.003%
75	10.109	2801	2805	2807	rVB2	497	255	0.01%	0.002%
76	10.145	2807	2816	2818	rBV2	333	445	0.02%	0.003%
77	10.267	2839	2854	2887	rBV	583095	955247	50.66%	6.987%
78	10.389	2890	2892	2896	rVV2	589	337	0.02%	0.002%
79	10.418	2896	2901	2903	rVV3	475	463	0.02%	0.003%
80	10.608	2954	2960	2962	rBV3	411	396	0.02%	0.003%
81	10.665	2975	2978	2982	rBV3	450	373	0.02%	0.003%
82	10.691	2982	2986	2987	rBV2	480	339	0.02%	0.002%
83	10.775	3008	3012	3015	rBV2	540	468	0.02%	0.003%
84	10.865	3036	3040	3043	rBV3	360	374	0.02%	0.003%
85	10.907	3049	3053	3056	rBV	407	340	0.02%	0.002%
86	11.064	3099	3102	3108	rBV3	392	455	0.02%	0.003%
87	11.157	3127	3131	3133	rBV2	368	290	0.02%	0.002%
88	11.193	3139	3142	3144	rBV3	403	307	0.02%	0.002%
89	11.231	3151	3154	3160	rVB4	886	1007	0.05%	0.007%
90	11.302	3163	3176	3205	rBV	623194	1059871	56.21%	7.752%
91	11.508	3237	3240	3244	rVV2	481	315	0.02%	0.002%
92	11.678	3279	3293	3318	rBV	619234	1070237	56.76%	7.828%
93	12.276	3475	3479	3482	rBV3	501	415	0.02%	0.003%
94	12.418	3519	3523	3526	rBV2	434	419	0.02%	0.003%
95	12.646	3590	3594	3595	rBV	636	482	0.03%	0.004%
96	12.762	3627	3630	3632	rBV3	480	346	0.02%	0.003%
97	12.807	3641	3644	3647	rBV3	733	454	0.02%	0.003%
98	13.029	3711	3713	3716	rBV	579	333	0.02%	0.002%
99	13.132	3742	3745	3748	rBV5	530	485	0.03%	0.004%
100	14.595	4197	4200	4203	rBV2	976	730	0.04%	0.005%


Sum of corrected areas: 13672358

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV090618\
Data File : VV007443.D
Acq On : 07 Sep 2018 01:47
Operator : SY/MD
Sample : J4751-01DL 500X
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGH2DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

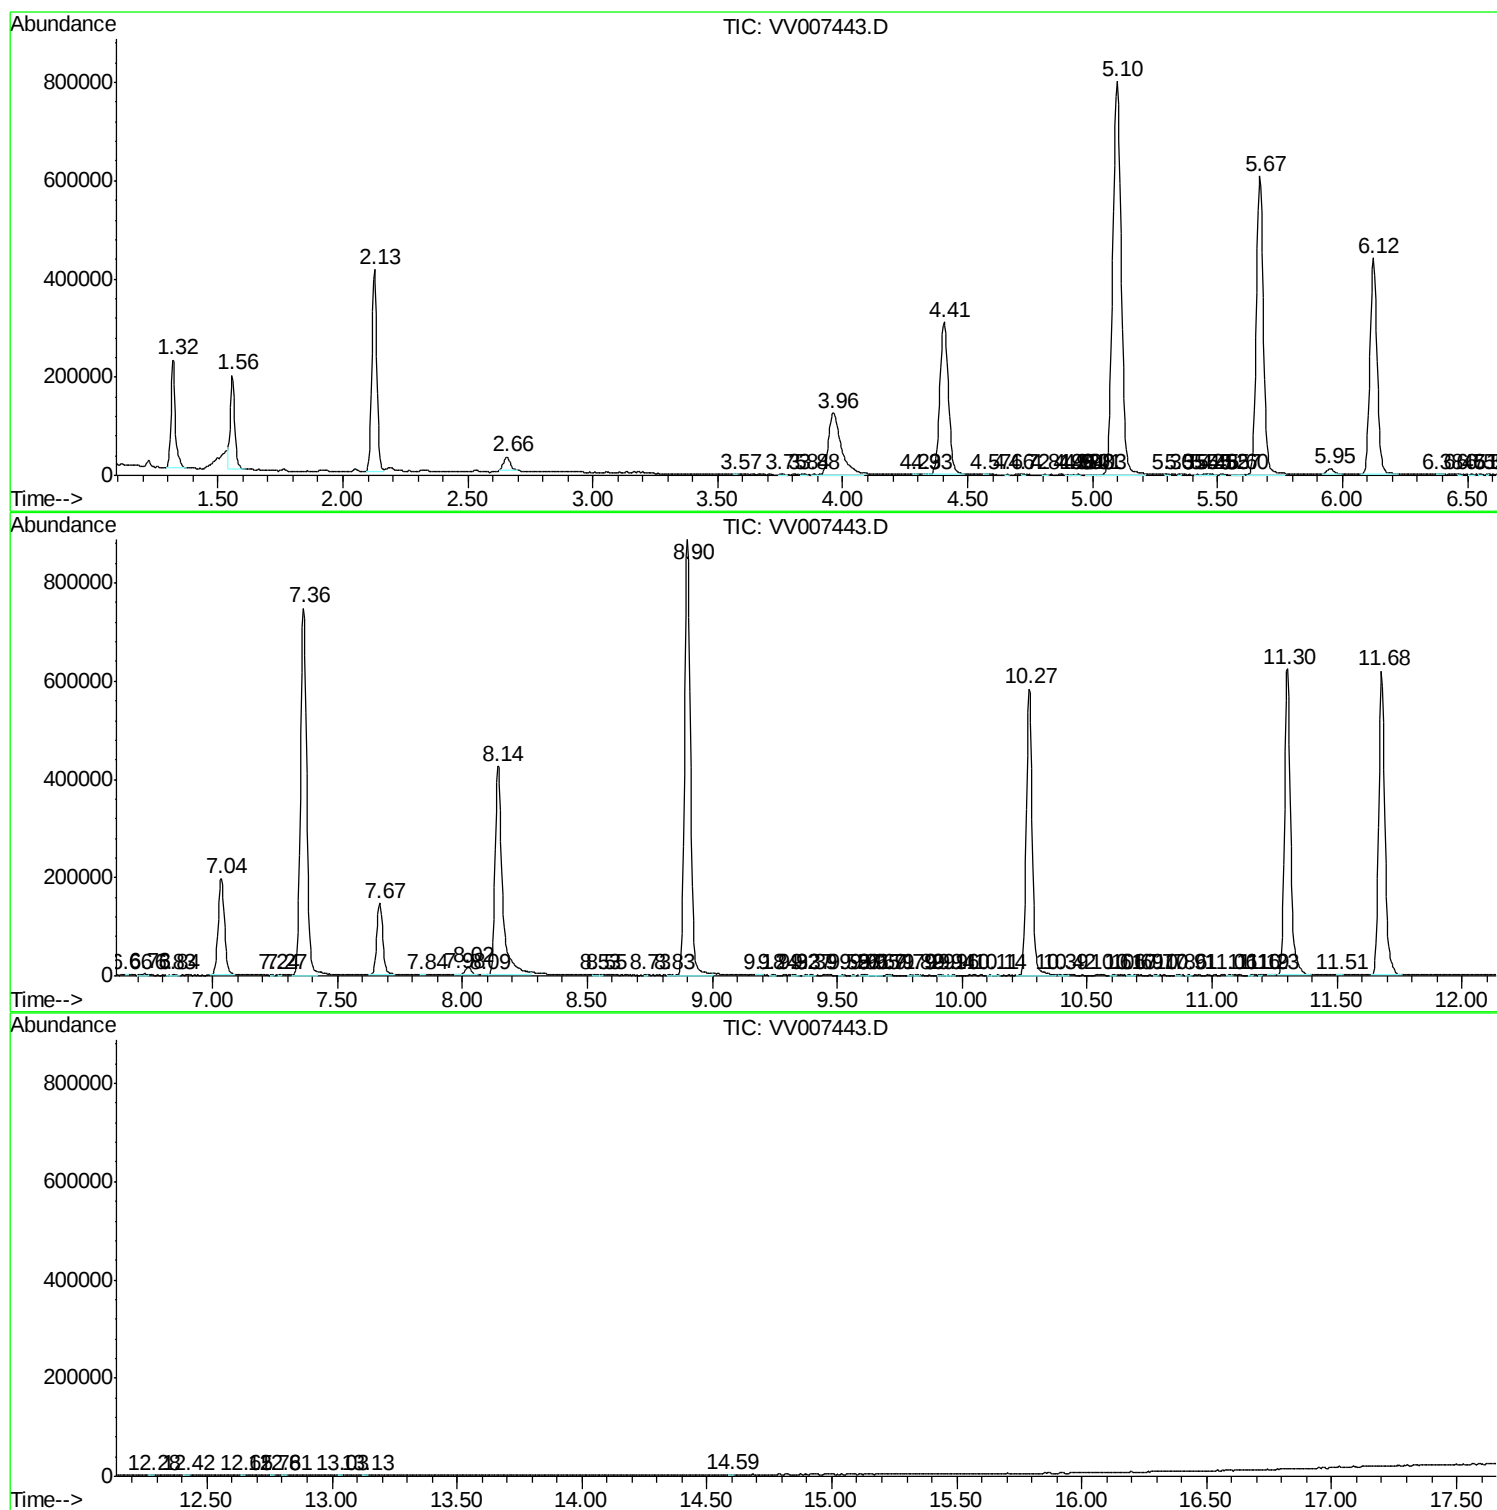

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV090618\
Data File : VV007443.D
Acq On : 07 Sep 2018 01:47
Operator : SY/MD
Sample : J4751-01DL 500X
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGH2DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV090618\
Data File : VV007443.D
Acq On : 07 Sep 2018 01:47
Operator : SY/MD
Sample : J4751-01DL 500X
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGH2DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc