

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090618\
 Data File : VV007446.D
 Acq On : 07 Sep 2018 03:02
 Operator : SY/MD
 Sample : J4751-04DL 500X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGH5DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	64	71	89	rVB	229784	274914	14.50%	1.988%
2	1.557	139	145	160	rVB	192940	246026	12.98%	1.779%
3	2.126	311	322	334	rBV	404952	571422	30.14%	4.132%
4	2.653	479	486	506	rVB	38118	78617	4.15%	0.569%
5	3.402	716	719	724	rVB2	613	606	0.03%	0.004%
6	3.502	746	750	751	rBV3	412	278	0.01%	0.002%
7	3.544	759	763	765	rVB2	443	282	0.01%	0.002%
8	3.602	778	781	785	rVB2	458	371	0.02%	0.003%
9	3.692	807	809	812	rVB2	559	287	0.02%	0.002%
10	3.714	812	816	823	rBV2	501	547	0.03%	0.004%
11	3.775	832	835	838	rBV4	364	276	0.01%	0.002%
12	3.962	876	893	935	rVV3	126067	449629	23.72%	3.252%
13	4.280	989	992	995	rBV3	647	468	0.02%	0.003%
14	4.405	1013	1031	1059	rBV	312811	755402	39.85%	5.463%
15	4.708	1122	1125	1127	rBV2	618	509	0.03%	0.004%
16	4.772	1144	1145	1151	rVB2	534	417	0.02%	0.003%
17	4.811	1151	1157	1162	rBV	591	565	0.03%	0.004%
18	4.849	1162	1169	1172	rBV4	432	507	0.03%	0.004%
19	4.904	1180	1186	1189	rBV3	370	435	0.02%	0.003%
20	4.962	1198	1204	1210	rBV3	272	362	0.02%	0.003%
21	5.097	1225	1246	1283	rBV2	808040	1895817	100.00%	13.710%
22	5.274	1299	1301	1304	rVB3	940	409	0.02%	0.003%
23	5.364	1325	1329	1332	rBV3	648	528	0.03%	0.004%
24	5.502	1366	1372	1377	rBV4	640	958	0.05%	0.007%
25	5.573	1392	1394	1398	rBV2	345	285	0.02%	0.002%
26	5.669	1407	1424	1444	rBV	613726	1206017	63.61%	8.722%
27	5.946	1501	1510	1522	rBV5	10375	22248	1.17%	0.161%
28	6.122	1550	1565	1591	rBV	446650	890465	46.97%	6.440%
29	6.370	1639	1642	1646	rBV3	540	478	0.03%	0.003%
30	6.441	1661	1664	1666	rBV	450	299	0.02%	0.002%
31	6.537	1692	1694	1698	rBV2	539	387	0.02%	0.003%
32	6.650	1726	1729	1731	rBV3	423	348	0.02%	0.003%
33	6.720	1741	1751	1759	rBV5	3029	5611	0.30%	0.041%
34	6.833	1783	1786	1790	rVB3	569	355	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090618\
 Data File : VV007446.D
 Acq On : 07 Sep 2018 03:02
 Operator : SY/MD
 Sample : J4751-04DL 500X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGH5DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

35	6.862	1790	1795	1798	rBV3	690	623	0.03%	0.005%
36	6.904	1807	1808	1812	rVB2	673	379	0.02%	0.003%
37	6.929	1812	1816	1818	rBV2	477	320	0.02%	0.002%
38	6.965	1822	1827	1829	rBV2	408	297	0.02%	0.002%
39	7.036	1836	1849	1869	rBV	195359	347934	18.35%	2.516%
40	7.232	1907	1910	1915	rBV6	354	355	0.02%	0.003%
41	7.283	1921	1926	1928	rBV5	1082	855	0.05%	0.006%
42	7.364	1937	1951	1974	rBV	755829	1305354	68.85%	9.440%
43	7.576	2014	2017	2019	rVV3	434	277	0.01%	0.002%
44	7.624	2026	2032	2033	rBV4	623	640	0.03%	0.005%
45	7.669	2034	2046	2065	rVV	145920	245568	12.95%	1.776%
46	7.817	2090	2092	2097	rVB2	733	530	0.03%	0.004%
47	7.843	2097	2100	2104	rBV3	1079	988	0.05%	0.007%
48	7.984	2139	2144	2145	rBV3	1510	1309	0.07%	0.009%
49	8.023	2147	2156	2167	rVB4	20888	35850	1.89%	0.259%
50	8.142	2181	2193	2234	rBV2	424790	882790	46.57%	6.384%
51	8.511	2306	2308	2314	rVB4	473	354	0.02%	0.003%
52	8.579	2326	2329	2332	rBV2	728	583	0.03%	0.004%
53	8.685	2356	2362	2366	rBV4	658	783	0.04%	0.006%
54	8.743	2377	2380	2383	rVB4	580	439	0.02%	0.003%
55	8.772	2383	2389	2390	rBV2	642	589	0.03%	0.004%
56	8.807	2396	2400	2404	rVB3	581	464	0.02%	0.003%
57	8.900	2416	2429	2463	rBV	898667	1475359	77.82%	10.669%
58	9.154	2503	2508	2512	rBV3	389	409	0.02%	0.003%
59	9.180	2512	2516	2518	rBV3	663	464	0.02%	0.003%
60	9.251	2535	2538	2542	rBV2	532	475	0.03%	0.003%
61	9.299	2550	2553	2555	rBV3	341	278	0.01%	0.002%
62	9.389	2577	2581	2585	rVV2	575	486	0.03%	0.004%
63	9.425	2589	2592	2597	rVB4	339	305	0.02%	0.002%
64	9.457	2597	2602	2604	rBV3	394	346	0.02%	0.003%
65	9.515	2614	2620	2623	rBV3	783	873	0.05%	0.006%
66	9.556	2627	2633	2636	rBV2	508	508	0.03%	0.004%
67	9.608	2646	2649	2652	rBV3	623	423	0.02%	0.003%
68	9.650	2660	2662	2665	rVB2	506	292	0.02%	0.002%
69	9.675	2665	2670	2673	rBV2	433	365	0.02%	0.003%
70	9.794	2704	2707	2712	rVB4	501	361	0.02%	0.003%
71	10.045	2778	2785	2788	rBV3	527	600	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090618\
 Data File : VV007446.D
 Acq On : 07 Sep 2018 03:02
 Operator : SY/MD
 Sample : J4751-04DL 500X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGH5DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

72	10.103	2801	2803	2809	rVB3	360	273	0.01%	0.002%
73	10.158	2816	2820	2824	rVB2	320	298	0.02%	0.002%
74	10.267	2841	2854	2894	rVB	588309	970178	51.17%	7.016%
75	10.421	2898	2902	2905	rBV4	506	494	0.03%	0.004%
76	10.492	2920	2924	2926	rBV2	573	385	0.02%	0.003%
77	10.508	2926	2929	2935	rVV2	426	397	0.02%	0.003%
78	10.679	2977	2982	2988	rBV3	639	828	0.04%	0.006%
79	10.904	3050	3052	3057	rVB3	683	463	0.02%	0.003%
80	10.987	3076	3078	3082	rVB3	636	316	0.02%	0.002%
81	11.026	3085	3090	3094	rBV2	800	713	0.04%	0.005%
82	11.222	3146	3151	3153	rBV2	584	466	0.02%	0.003%
83	11.299	3163	3175	3208	rVB	614854	1057640	55.79%	7.649%
84	11.415	3208	3211	3213	rBV2	407	347	0.02%	0.003%
85	11.527	3242	3246	3257	rVB3	627	841	0.04%	0.006%
86	11.678	3280	3293	3317	rBV	622448	1071440	56.52%	7.748%
87	11.781	3322	3325	3333	rVV4	966	1123	0.06%	0.008%
88	11.826	3337	3339	3342	rVB2	664	324	0.02%	0.002%
89	11.923	3364	3369	3370	rBV2	389	307	0.02%	0.002%
90	12.019	3395	3399	3405	rBV4	642	582	0.03%	0.004%
91	12.080	3412	3418	3422	rBV4	716	816	0.04%	0.006%
92	12.219	3456	3461	3465	rVB2	461	529	0.03%	0.004%
93	12.643	3590	3593	3598	rBV4	432	454	0.02%	0.003%
94	12.711	3610	3614	3615	rBV2	463	305	0.02%	0.002%
95	12.965	3690	3693	3696	rVB2	634	377	0.02%	0.003%
96	12.984	3696	3699	3703	rBV3	663	601	0.03%	0.004%
97	13.305	3796	3799	3800	rBV2	592	342	0.02%	0.002%
98	14.032	4019	4025	4027	rBV4	845	917	0.05%	0.007%
99	14.096	4043	4045	4047	rBV3	900	599	0.03%	0.004%
100	14.534	4179	4181	4187	rVB5	1135	694	0.04%	0.005%


Sum of corrected areas: 13827999

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV090618\
Data File : VV007446.D
Acq On : 07 Sep 2018 03:02
Operator : SY/MD
Sample : J4751-04DL 500X
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGH5DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

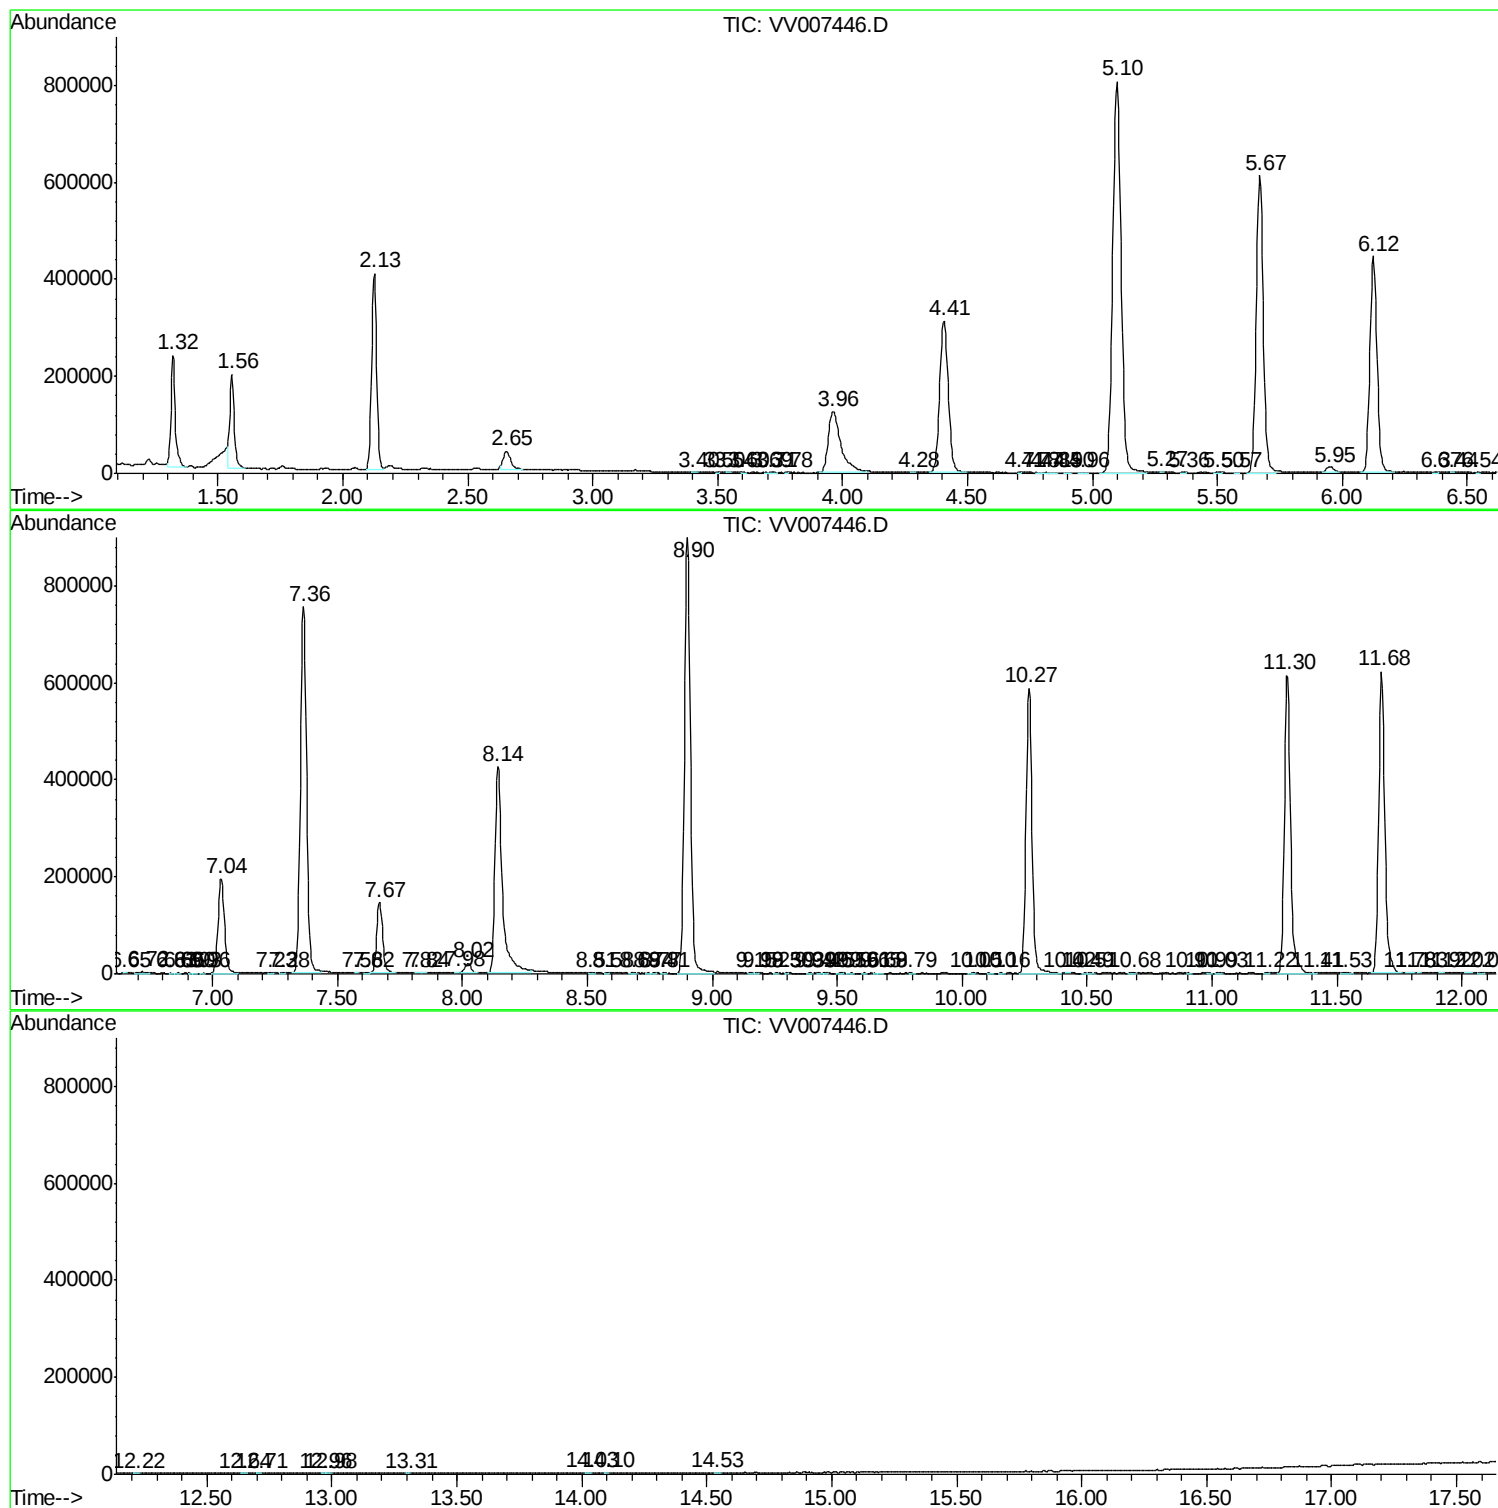

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV090618\
Data File : VV007446.D
Acq On : 07 Sep 2018 03:02
Operator : SY/MD
Sample : J4751-04DL 500X
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGH5DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV090618\
Data File : VV007446.D
Acq On : 07 Sep 2018 03:02
Operator : SY/MD
Sample : J4751-04DL 500X
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGH5DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc