

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090618\
 Data File : VV007447.D
 Acq On : 07 Sep 2018 03:27
 Operator : SY/MD
 Sample : J4751-05DL 500X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGH6DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	64	71	90	rVB	221217	270240	14.71%	2.004%
2	1.560	140	146	162	rVB	191396	236318	12.86%	1.752%
3	2.126	312	322	334	rBV	404169	568026	30.91%	4.212%
4	2.653	477	486	507	rVB	33376	74204	4.04%	0.550%
5	3.325	693	695	700	rVB4	663	437	0.02%	0.003%
6	3.376	709	711	715	rVB4	756	451	0.02%	0.003%
7	3.515	751	754	757	rBV2	388	276	0.02%	0.002%
8	3.640	790	793	796	rVB2	459	341	0.02%	0.003%
9	3.685	803	807	809	rBV2	454	331	0.02%	0.002%
10	3.878	860	867	871	rBV3	553	531	0.03%	0.004%
11	3.965	871	894	934	rBV3	122022	445249	24.23%	3.302%
12	4.232	975	977	981	rBV2	523	440	0.02%	0.003%
13	4.405	1013	1031	1054	rBV	308658	740967	40.32%	5.495%
14	4.511	1062	1064	1065	rBV2	537	276	0.02%	0.002%
15	4.592	1086	1089	1093	rVV3	413	279	0.02%	0.002%
16	4.627	1098	1100	1104	rVB3	736	497	0.03%	0.004%
17	4.682	1115	1117	1120	rBV2	437	296	0.02%	0.002%
18	4.788	1146	1150	1155	rBB4	322	327	0.02%	0.002%
19	4.826	1159	1162	1165	rVB	603	406	0.02%	0.003%
20	4.987	1207	1212	1214	rBV2	332	290	0.02%	0.002%
21	5.097	1227	1246	1269	rBV2	777360	1837515	100.00%	13.626%
22	5.444	1348	1354	1358	rBV5	474	560	0.03%	0.004%
23	5.489	1365	1368	1369	rBV2	496	288	0.02%	0.002%
24	5.515	1374	1376	1382	rVB2	461	271	0.01%	0.002%
25	5.556	1385	1389	1395	rVB4	632	488	0.03%	0.004%
26	5.588	1395	1399	1406	rVB2	687	667	0.04%	0.005%
27	5.669	1406	1424	1445	rBV	593172	1171020	63.73%	8.683%
28	5.949	1501	1511	1533	rVB3	12295	26219	1.43%	0.194%
29	6.122	1549	1565	1590	rBV	429009	868515	47.27%	6.440%
30	6.306	1619	1622	1624	rBV3	498	384	0.02%	0.003%
31	6.624	1717	1721	1722	rBV3	479	323	0.02%	0.002%
32	6.650	1725	1729	1730	rBV4	635	417	0.02%	0.003%
33	6.797	1773	1775	1782	rVB4	595	508	0.03%	0.004%
34	6.852	1788	1792	1795	rBV2	419	402	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090618\
 Data File : VV007447.D
 Acq On : 07 Sep 2018 03:27
 Operator : SY/MD
 Sample : J4751-05DL 500X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGH6DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

35	6.868	1795	1797	1799	rBV2	517	271	0.01%	0.002%
36	7.035	1834	1849	1869	rBV	187811	335990	18.29%	2.491%
37	7.193	1894	1898	1903	rVB4	785	870	0.05%	0.006%
38	7.215	1903	1905	1909	rVB3	473	323	0.02%	0.002%
39	7.363	1937	1951	1971	rBV	735643	1280223	69.67%	9.493%
40	7.582	2016	2019	2021	rBV3	561	284	0.02%	0.002%
41	7.621	2029	2031	2033	rBV2	528	328	0.02%	0.002%
42	7.669	2034	2046	2065	rVV	142152	239252	13.02%	1.774%
43	7.797	2084	2086	2092	rVB5	415	365	0.02%	0.003%
44	7.836	2095	2098	2100	rBV2	417	292	0.02%	0.002%
45	7.984	2139	2144	2146	rBV3	1597	1555	0.08%	0.012%
46	8.022	2148	2156	2167	rVB2	15671	26437	1.44%	0.196%
47	8.077	2167	2173	2176	rBV4	697	719	0.04%	0.005%
48	8.141	2180	2193	2236	rBV2	405578	853831	46.47%	6.331%
49	8.547	2313	2319	2321	rBV6	527	474	0.03%	0.004%
50	8.582	2327	2330	2334	rBV2	438	355	0.02%	0.003%
51	8.649	2349	2351	2356	rVB3	669	550	0.03%	0.004%
52	8.672	2356	2358	2361	rBV3	427	346	0.02%	0.003%
53	8.688	2361	2363	2369	rVB4	730	621	0.03%	0.005%
54	8.736	2372	2378	2380	rBV2	554	585	0.03%	0.004%
55	8.788	2390	2394	2400	rBV2	696	638	0.03%	0.005%
56	8.830	2403	2407	2411	rBV4	447	363	0.02%	0.003%
57	8.900	2415	2429	2454	rBV	859862	1418930	77.22%	10.522%
58	9.157	2505	2509	2514	rVB3	681	531	0.03%	0.004%
59	9.180	2514	2516	2519	rBV4	505	344	0.02%	0.003%
60	9.199	2519	2522	2529	rVV3	597	593	0.03%	0.004%
61	9.235	2531	2533	2537	rVB2	446	300	0.02%	0.002%
62	9.270	2537	2544	2549	rBV3	455	582	0.03%	0.004%
63	9.402	2582	2585	2590	rVB2	435	374	0.02%	0.003%
64	9.460	2599	2603	2606	rVB2	447	384	0.02%	0.003%
65	9.518	2616	2621	2625	rVB3	560	551	0.03%	0.004%
66	9.540	2625	2628	2631	rBV3	515	391	0.02%	0.003%
67	9.611	2645	2650	2651	rBV2	368	269	0.01%	0.002%
68	9.698	2674	2677	2681	rVV2	353	305	0.02%	0.002%
69	9.759	2693	2696	2701	rBV3	498	520	0.03%	0.004%
70	9.894	2734	2738	2740	rBV2	338	294	0.02%	0.002%
71	10.051	2784	2787	2789	rBV2	404	270	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090618\
 Data File : VV007447.D
 Acq On : 07 Sep 2018 03:27
 Operator : SY/MD
 Sample : J4751-05DL 500X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGH6DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

72	10.167	2817	2823	2826	rBV2	379	365	0.02%	0.003%
73	10.206	2833	2835	2841	rVB	339	290	0.02%	0.002%
74	10.267	2841	2854	2885	rBV	573870	940917	51.21%	6.977%
75	10.456	2911	2913	2919	rVB2	683	629	0.03%	0.005%
76	10.569	2946	2948	2953	rVB2	459	277	0.02%	0.002%
77	10.630	2964	2967	2970	rVB3	470	335	0.02%	0.002%
78	10.649	2970	2973	2977	rBV2	352	265	0.01%	0.002%
79	10.694	2983	2987	2992	rVB2	354	346	0.02%	0.003%
80	10.720	2992	2995	2999	rBV4	475	381	0.02%	0.003%
81	10.903	3050	3052	3058	rVB4	699	686	0.04%	0.005%
82	10.932	3058	3061	3065	rBV2	455	316	0.02%	0.002%
83	11.051	3094	3098	3103	rBV3	376	478	0.03%	0.004%
84	11.103	3112	3114	3119	rBV3	403	305	0.02%	0.002%
85	11.132	3119	3123	3129	rVB4	445	523	0.03%	0.004%
86	11.199	3141	3144	3147	rVB2	642	298	0.02%	0.002%
87	11.231	3149	3154	3156	rBV3	647	593	0.03%	0.004%
88	11.299	3162	3175	3205	rBV	608283	1051907	57.25%	7.800%
89	11.678	3280	3293	3316	rBV	611217	1065056	57.96%	7.898%
90	11.945	3373	3376	3388	rVB4	577	776	0.04%	0.006%
91	11.993	3388	3391	3395	rVB2	584	409	0.02%	0.003%
92	12.273	3474	3478	3481	rBV3	448	322	0.02%	0.002%
93	12.289	3481	3483	3485	rBV2	459	260	0.01%	0.002%
94	12.399	3514	3517	3520	rBV2	453	393	0.02%	0.003%
95	12.653	3593	3596	3597	rBV2	378	284	0.02%	0.002%
96	12.897	3669	3672	3677	rVB4	773	656	0.04%	0.005%
97	13.559	3876	3878	3880	rBV	564	330	0.02%	0.002%
98	13.942	3995	3997	4000	rBV3	524	338	0.02%	0.003%
99	14.051	4029	4031	4033	rBV4	600	308	0.02%	0.002%
100	14.164	4064	4066	4069	rBV3	688	474	0.03%	0.004%


Sum of corrected areas: 13485586

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV090618\
Data File : VV007447.D
Acq On : 07 Sep 2018 03:27
Operator : SY/MD
Sample : J4751-05DL 500X
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGH6DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

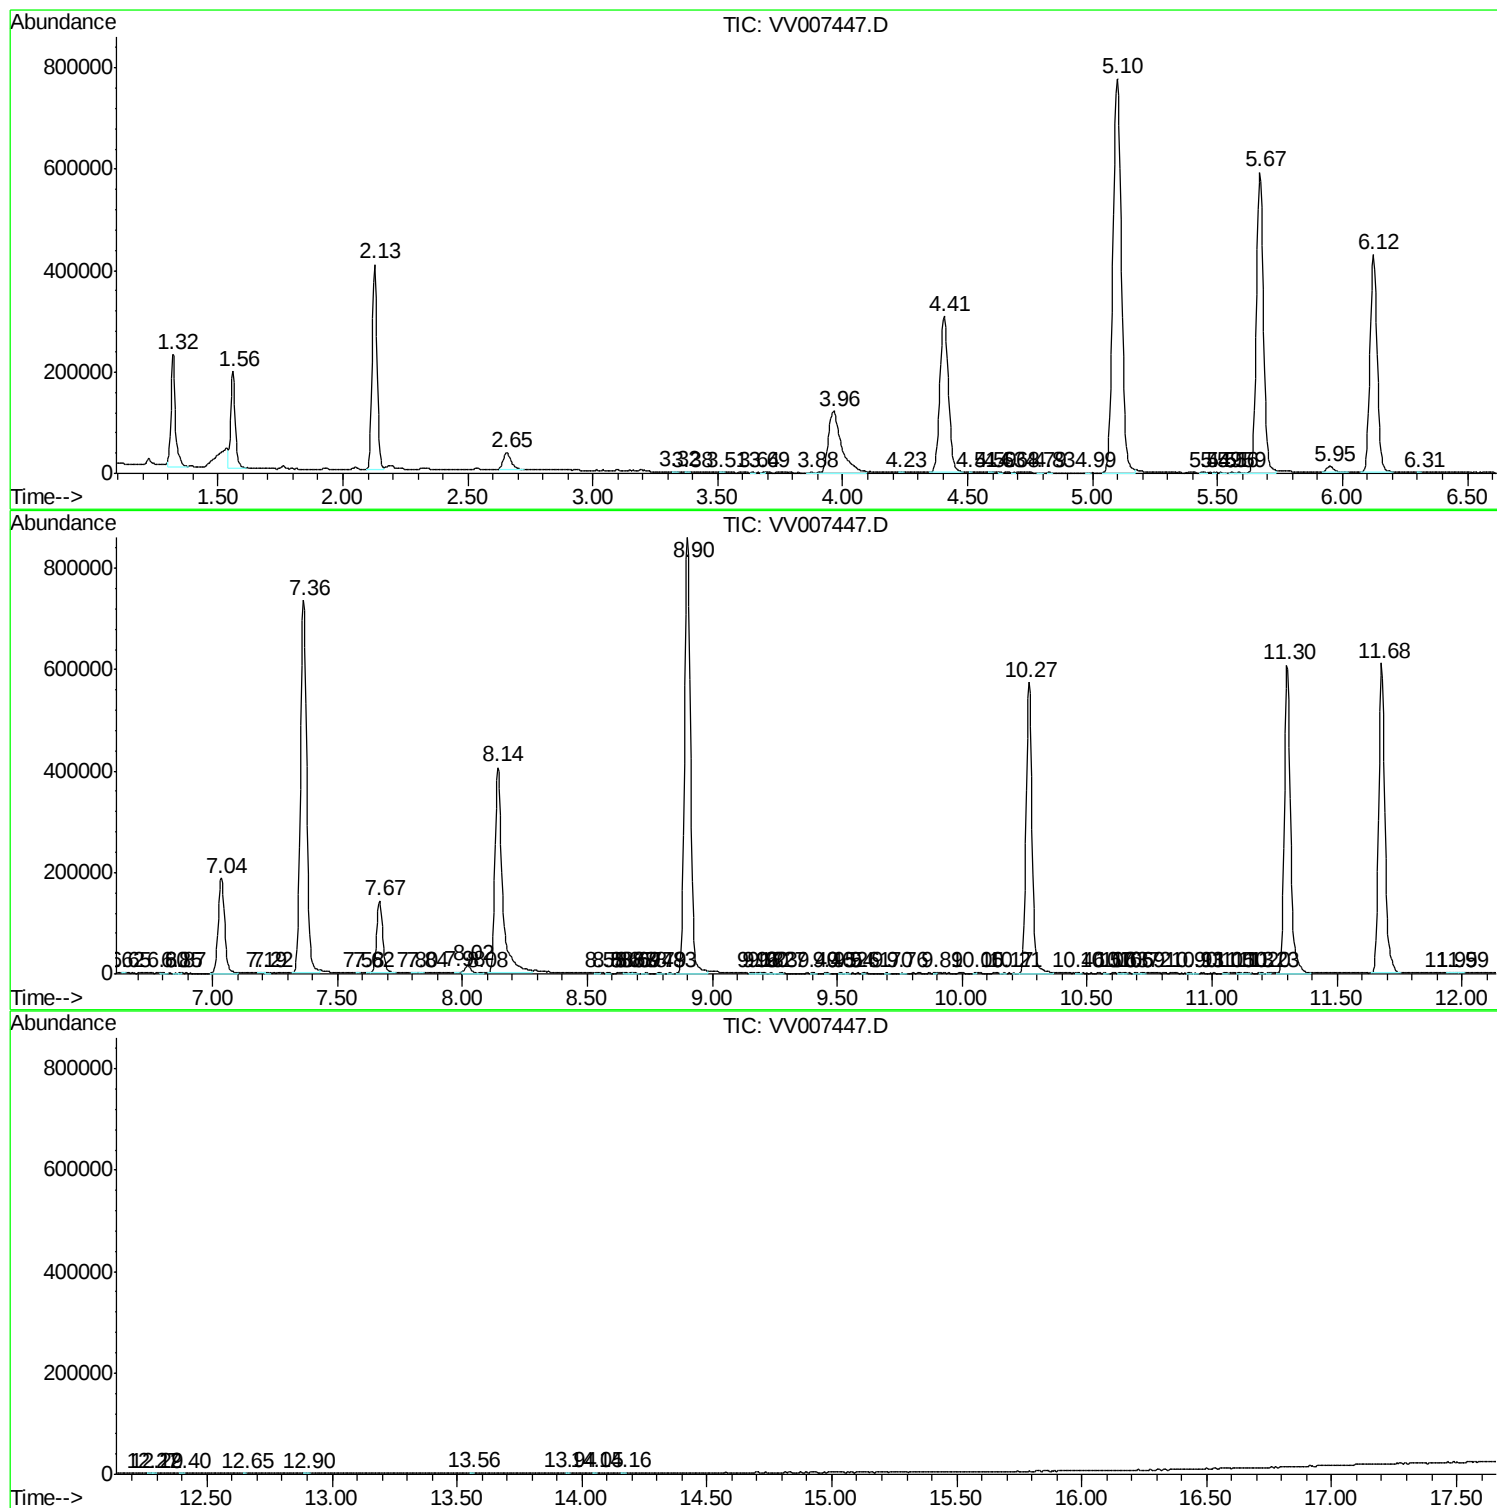

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV090618\
Data File : VV007447.D
Acq On : 07 Sep 2018 03:27
Operator : SY/MD
Sample : J4751-05DL 500X
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGH6DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV090618\
Data File : VV007447.D
Acq On : 07 Sep 2018 03:27
Operator : SY/MD
Sample : J4751-05DL 500X
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGH6DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc