

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090618\
 Data File : VV007449.D
 Acq On : 07 Sep 2018 04:17
 Operator : SY/MD
 Sample : J4751-07DL 1000X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGH8DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	63	71	89	rVB	243374	280165	14.07%	1.918%
2	1.560	140	146	160	rVB	200462	248416	12.47%	1.701%
3	2.126	312	322	334	rBV	448047	628911	31.58%	4.306%
4	2.656	479	487	512	rVB	29219	65934	3.31%	0.451%
5	3.447	731	733	738	rBV2	515	447	0.02%	0.003%
6	3.556	764	767	773	rVB	607	522	0.03%	0.004%
7	3.601	778	781	784	rBV2	503	401	0.02%	0.003%
8	3.692	806	809	812	rBV2	357	247	0.01%	0.002%
9	3.759	826	830	831	rBV2	344	270	0.01%	0.002%
10	3.884	866	869	872	rBV2	529	362	0.02%	0.002%
11	3.962	875	893	929	rBV3	125784	445644	22.38%	3.051%
12	4.335	1007	1009	1012	rVB3	751	350	0.02%	0.002%
13	4.405	1012	1031	1056	rBV	327763	790167	39.68%	5.410%
14	4.714	1122	1127	1128	rBV2	551	462	0.02%	0.003%
15	4.753	1137	1139	1142	rVB	466	254	0.01%	0.002%
16	4.859	1165	1172	1175	rBV3	350	392	0.02%	0.003%
17	5.026	1219	1224	1227	rBV3	341	309	0.02%	0.002%
18	5.097	1227	1246	1286	rBV2	840179	1991527	100.00%	13.636%
19	5.376	1330	1333	1336	rBV3	511	411	0.02%	0.003%
20	5.447	1348	1355	1358	rBV5	566	794	0.04%	0.005%
21	5.460	1358	1359	1366	rVB3	476	378	0.02%	0.003%
22	5.505	1370	1373	1376	rBV3	341	248	0.01%	0.002%
23	5.540	1380	1384	1387	rVB3	686	585	0.03%	0.004%
24	5.579	1391	1396	1397	rBV2	428	352	0.02%	0.002%
25	5.592	1397	1400	1404	rVB3	618	537	0.03%	0.004%
26	5.669	1409	1424	1447	rBV	636548	1257995	63.17%	8.613%
27	5.949	1501	1511	1524	rVB5	12973	25746	1.29%	0.176%
28	6.122	1550	1565	1591	rBV	457465	926669	46.53%	6.345%
29	6.273	1609	1612	1616	rVV4	579	449	0.02%	0.003%
30	6.315	1620	1625	1628	rBV5	435	479	0.02%	0.003%
31	6.370	1640	1642	1645	rVB2	586	297	0.01%	0.002%
32	6.386	1645	1647	1652	rVB3	309	241	0.01%	0.002%
33	6.418	1654	1657	1662	rVB4	492	459	0.02%	0.003%
34	6.524	1687	1690	1695	rVB4	853	652	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090618\
 Data File : VV007449.D
 Acq On : 07 Sep 2018 04:17
 Operator : SY/MD
 Sample : J4751-07DL 1000X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGH8DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

35	6.556	1695	1700	1703	rBV3	507	420	0.02%	0.003%
36	6.643	1725	1727	1731	rBV4	492	457	0.02%	0.003%
37	6.685	1736	1740	1742	rBV3	577	415	0.02%	0.003%
38	6.720	1742	1751	1753	rBV2	2255	2556	0.13%	0.018%
39	6.756	1760	1762	1764	rVB2	661	271	0.01%	0.002%
40	6.772	1764	1767	1770	rVB3	599	487	0.02%	0.003%
41	6.871	1794	1798	1802	rBV4	443	406	0.02%	0.003%
42	6.923	1812	1814	1819	rVB2	789	536	0.03%	0.004%
43	6.961	1821	1826	1828	rBV2	355	285	0.01%	0.002%
44	7.035	1836	1849	1871	rBV	201426	363584	18.26%	2.489%
45	7.363	1937	1951	1984	rBV	833900	1464963	73.56%	10.030%
46	7.534	2002	2004	2008	rBV3	705	473	0.02%	0.003%
47	7.669	2033	2046	2063	rBV	152393	256299	12.87%	1.755%
48	7.759	2072	2074	2077	rVB3	645	265	0.01%	0.002%
49	7.839	2097	2099	2102	rBV4	684	445	0.02%	0.003%
50	8.023	2146	2156	2167	rVB2	24211	39921	2.00%	0.273%
51	8.093	2174	2178	2181	rBV	551	496	0.02%	0.003%
52	8.141	2181	2193	2234	rBV2	430881	891339	44.76%	6.103%
53	8.518	2308	2310	2314	rVB3	788	450	0.02%	0.003%
54	8.537	2314	2316	2320	rBV3	350	246	0.01%	0.002%
55	8.579	2327	2329	2334	rVB5	544	372	0.02%	0.003%
56	8.604	2334	2337	2339	rBV3	424	255	0.01%	0.002%
57	8.646	2348	2350	2355	rVB2	586	422	0.02%	0.003%
58	8.704	2366	2368	2371	rVV2	479	249	0.01%	0.002%
59	8.730	2374	2376	2379	rVB3	524	290	0.01%	0.002%
60	8.756	2379	2384	2387	rBV3	706	707	0.04%	0.005%
61	8.775	2387	2390	2393	rBV3	347	243	0.01%	0.002%
62	8.836	2406	2409	2411	rBV2	535	359	0.02%	0.002%
63	8.900	2416	2429	2455	rBV	978262	1569012	78.78%	10.743%
64	9.135	2501	2502	2505	rVB2	1080	521	0.03%	0.004%
65	9.177	2512	2515	2517	rBV2	638	435	0.02%	0.003%
66	9.447	2596	2599	2603	rBV2	648	418	0.02%	0.003%
67	9.511	2615	2619	2623	rVB3	373	289	0.01%	0.002%
68	9.765	2694	2698	2703	rBV3	605	653	0.03%	0.004%
69	9.878	2730	2733	2735	rBV3	394	250	0.01%	0.002%
70	9.932	2744	2750	2753	rBV3	365	357	0.02%	0.002%
71	9.990	2764	2768	2773	rVB3	310	334	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090618\
 Data File : VV007449.D
 Acq On : 07 Sep 2018 04:17
 Operator : SY/MD
 Sample : J4751-07DL 1000X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGH8DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

72	10.161	2816	2821	2828	rBV4	471	597	0.03%	0.004%
73	10.190	2828	2830	2833	rVB	414	240	0.01%	0.002%
74	10.267	2840	2854	2887	rVV	609979	995387	49.98%	6.815%
75	10.379	2887	2889	2894	rVB2	532	301	0.02%	0.002%
76	10.521	2930	2933	2935	rBV2	455	345	0.02%	0.002%
77	10.601	2955	2958	2961	rBV3	498	386	0.02%	0.003%
78	10.620	2961	2964	2968	rVV2	368	292	0.01%	0.002%
79	10.714	2989	2993	2995	rBV3	350	294	0.01%	0.002%
80	10.874	3039	3043	3046	rBV2	249	260	0.01%	0.002%
81	10.894	3046	3049	3052	rBV3	466	412	0.02%	0.003%
82	10.968	3067	3072	3076	rBV3	483	536	0.03%	0.004%
83	11.151	3122	3129	3130	rBV3	630	573	0.03%	0.004%
84	11.299	3162	3175	3200	rBV	674421	1152444	57.87%	7.891%
85	11.678	3279	3293	3318	rBV	688985	1175405	59.02%	8.048%
86	11.823	3336	3338	3340	rBV2	441	268	0.01%	0.002%
87	12.350	3499	3502	3503	rBV	434	237	0.01%	0.002%
88	12.395	3514	3516	3519	rVB2	491	265	0.01%	0.002%
89	12.698	3608	3610	3615	rBV3	501	418	0.02%	0.003%
90	12.781	3634	3636	3639	rVB	505	271	0.01%	0.002%
91	12.836	3651	3653	3655	rBV	437	237	0.01%	0.002%
92	12.903	3669	3674	3676	rBV3	488	490	0.02%	0.003%
93	13.173	3756	3758	3760	rBV	638	416	0.02%	0.003%
94	13.244	3773	3780	3783	rBV4	736	919	0.05%	0.006%
95	13.627	3894	3899	3903	rBV4	869	951	0.05%	0.007%
96	13.698	3919	3921	3925	rVB2	859	524	0.03%	0.004%
97	13.858	3968	3971	3975	rVB2	842	534	0.03%	0.004%
98	13.881	3976	3978	3981	rBV3	527	413	0.02%	0.003%
99	14.032	4022	4025	4028	rBV5	602	488	0.02%	0.003%
100	14.312	4109	4112	4114	rBV2	842	645	0.03%	0.004%


Sum of corrected areas: 14605100

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV090618\
Data File : VV007449.D
Acq On : 07 Sep 2018 04:17
Operator : SY/MD
Sample : J4751-07DL 1000X
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGH8DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

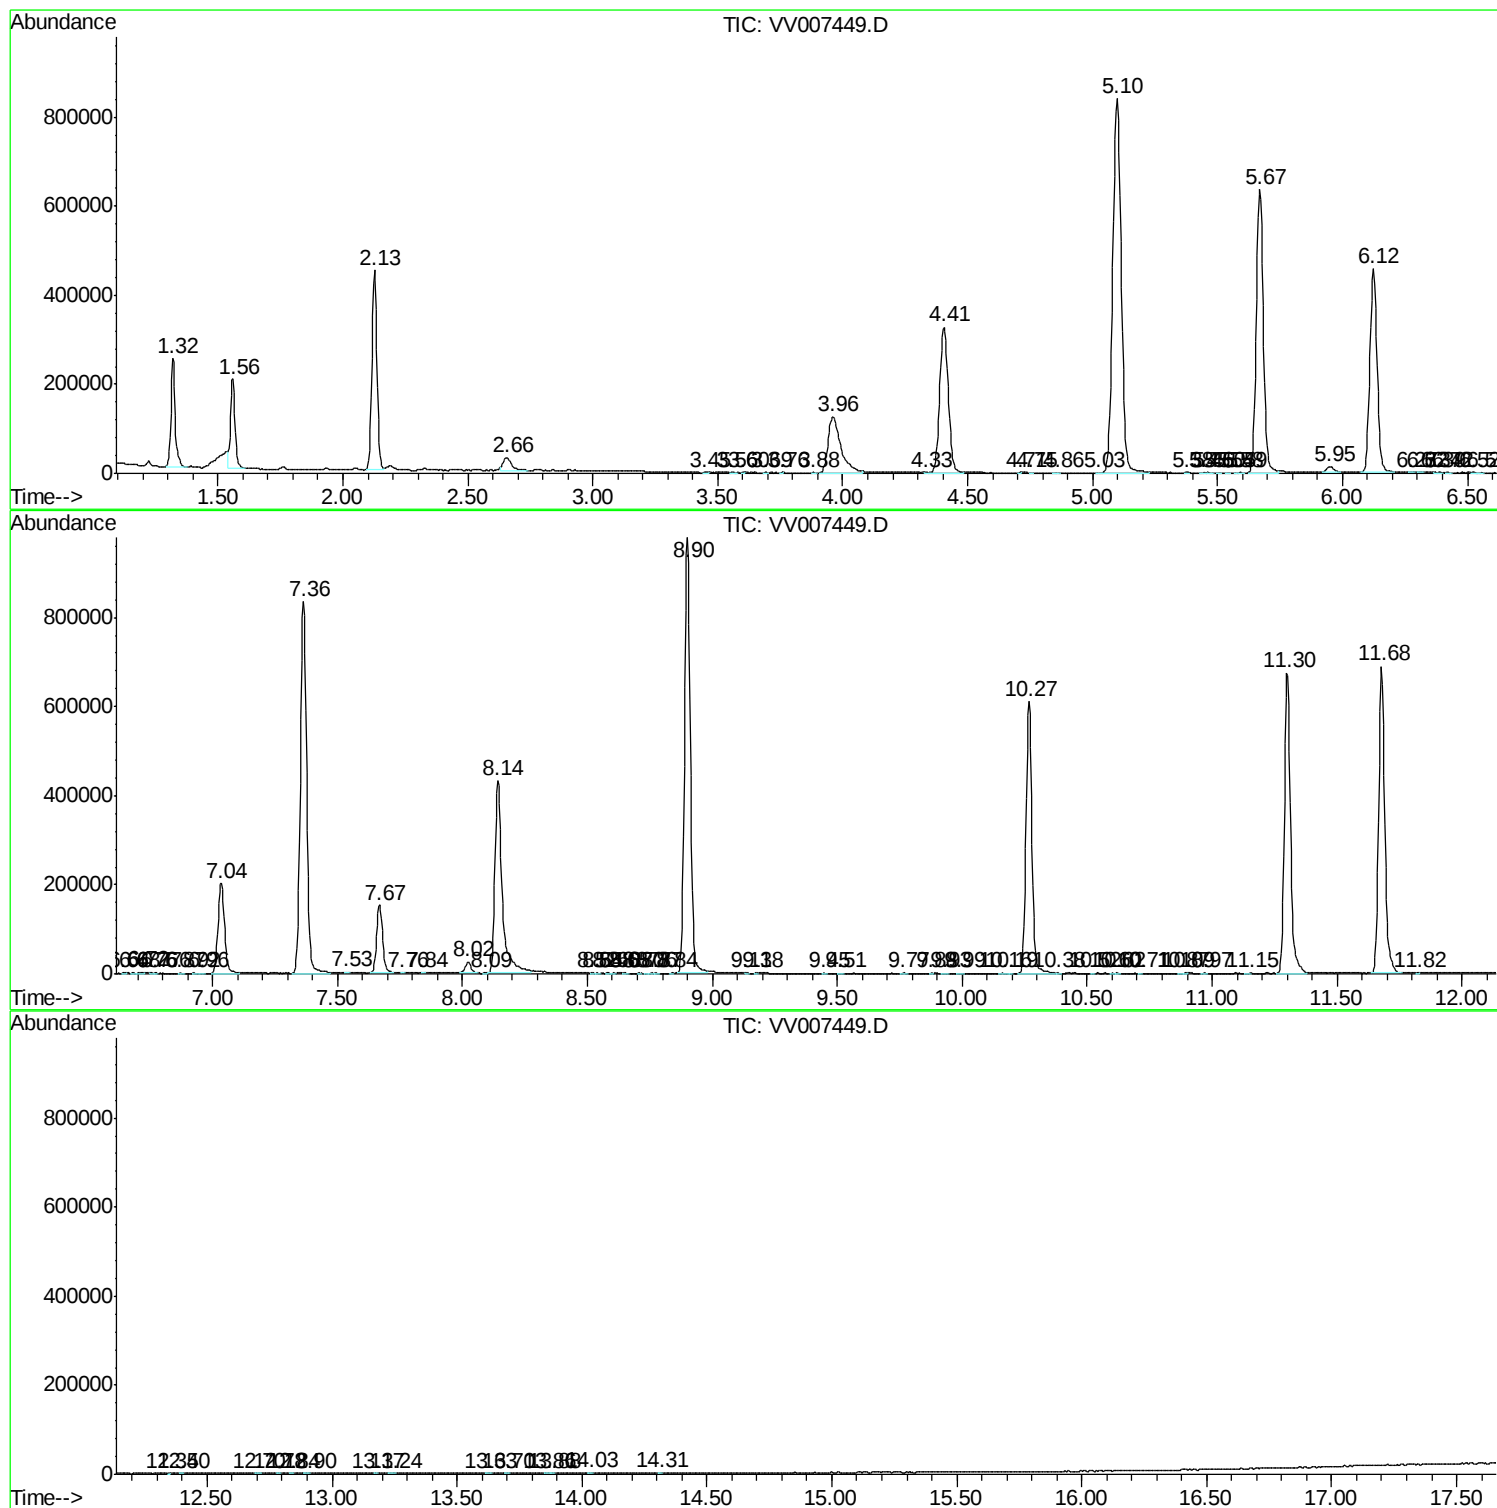

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV090618\
Data File : VV007449.D
Acq On : 07 Sep 2018 04:17
Operator : SY/MD
Sample : J4751-07DL 1000X
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGH8DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV090618\
Data File : VV007449.D
Acq On : 07 Sep 2018 04:17
Operator : SY/MD
Sample : J4751-07DL 1000X
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGH8DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc