


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090618\
Data File : VV007418.D
Acq On : 06 Sep 2018 13:53
Operator : SY/MD
Sample : BFB73
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB73

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Title : VOC Analysis
Last Update : Fri Sep 07 03:09:50 2018

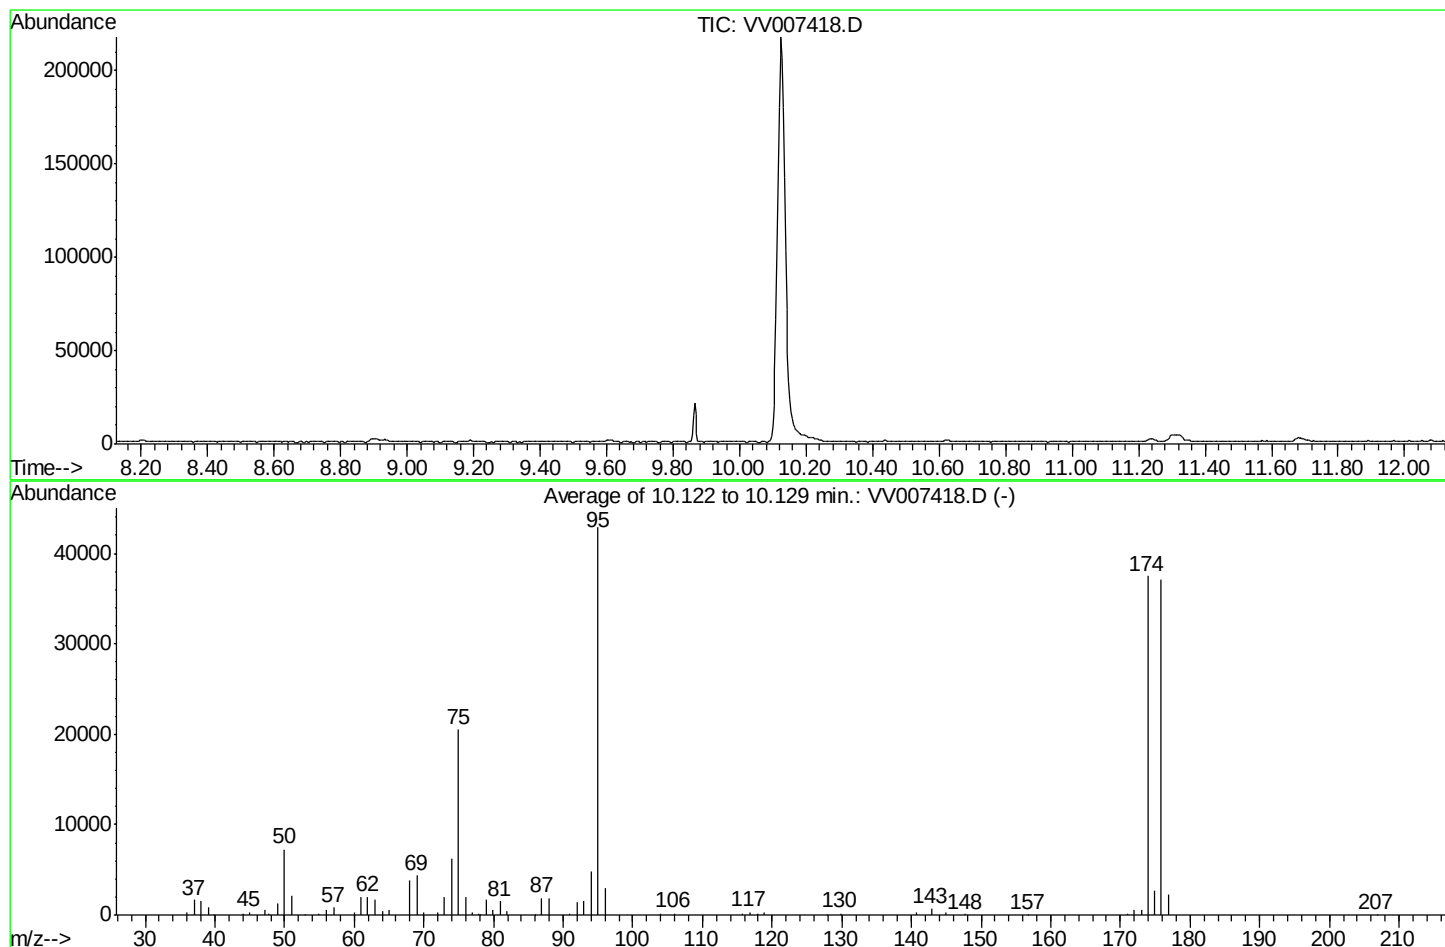

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2797

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	7225	PASS
75	95	30	80	47.9	20522	PASS
95	95	100	100	100.0	42885	PASS
96	95	5	9	6.8	2933	PASS
173	174	0.00	2	1.4	535	PASS
174	95	50	120	87.4	37482	PASS
175	174	5	9	7.1	2662	PASS
176	174	95	101	99.1	37162	PASS
177	176	5	9	5.9	2205	PASS

Scan 2797 (10.084 min): VV007418.D
BFB73

m/z	Abundance
39.90	248.0
44.00	785.0

Instrument :
MSVOA_V
ClientSampleId :
BFB73

m/z	Abundance
35.90	228.0
37.00	1620.0
38.00	1638.0
39.00	802.0
40.00	245.0
43.90	962.0
44.90	393.0
47.10	580.0
47.70	255.0
49.00	1203.0
50.00	7303.0
51.00	2175.0
54.90	136.0
56.00	540.0
57.00	819.0
60.00	330.0
61.00	1908.0
62.00	2020.0
63.00	1711.0
64.10	440.0
64.90	609.0
68.00	3753.0
69.00	4368.0
70.00	318.0
72.10	275.0
73.00	2035.0
74.00	6143.0
75.00	20592.0
76.00	2093.0
77.10	355.0
78.10	197.0
78.90	1604.0
79.80	446.0
80.90	1495.0
81.80	388.0
86.90	1930.0
88.00	1823.0
90.90	144.0
91.90	1329.0
93.00	1586.0
94.00	4689.0
95.00	42448.0
96.00	2952.0
103.80	133.0
105.90	156.0
115.80	147.0
116.80	297.0
117.90	182.0
118.70	243.0
129.80	177.0
140.80	338.0
142.90	744.0
144.90	327.0
147.70	180.0
171.10	188.0
172.00	557.0
173.00	513.0
173.90	36304.0
174.90	2640.0
175.90	36456.0
176.90	2247.0

Instrument :
MSVOA_V
ClientSampleId :
BFB73

m/z	Abundance
35.90	264.0
37.00	1782.0
38.00	1672.0
39.00	859.0
40.00	257.0
44.00	921.0
45.00	341.0
47.10	634.0
47.70	206.0
49.00	1322.0
50.00	7461.0
51.00	2252.0
52.90	102.0
54.90	135.0
56.00	592.0
57.00	863.0
60.00	349.0
61.00	1978.0
62.00	2070.0
63.00	1715.0
64.10	462.0
64.90	578.0
68.00	3968.0
69.00	4554.0
69.90	300.0
72.10	274.0
73.00	2019.0
74.00	6401.0
75.00	21336.0
76.00	2023.0
77.00	325.0
77.80	203.0
78.90	1695.0
79.90	544.0
80.90	1553.0
81.90	364.0
86.90	1947.0
88.00	1862.0
90.90	159.0
92.00	1464.0
93.00	1628.0
94.00	4990.0
95.00	44256.0
96.00	3007.0
103.90	131.0
105.90	146.0
115.80	165.0
116.80	313.0
117.90	216.0
118.80	271.0
127.80	107.0
129.80	166.0
140.80	327.0
142.90	712.0
144.90	324.0
147.70	124.0
156.70	109.0
171.10	226.0
171.90	589.0
173.00	533.0
173.90	38592.0
174.90	2715.0
175.90	38288.0
176.90	2274.0

Instrument :
MSVOA_V
ClientSampleId :
BFB73

m/z	Abundance
35.90	319.0
37.00	1610.0
38.00	1501.0
39.00	762.0
39.90	290.0
44.00	865.0
45.00	309.0
47.10	550.0
47.80	161.0
49.00	1419.0
50.00	6911.0
51.00	2005.0
52.90	109.0
54.90	128.0
56.00	592.0
57.00	838.0
60.00	346.0
61.00	1908.0
61.90	1925.0
63.00	1566.0
64.10	481.0
65.00	555.0
68.00	3808.0
69.00	4176.0
69.90	311.0
72.00	203.0
72.90	1908.0
74.00	5977.0
75.00	19640.0
76.00	1727.0
76.90	304.0
77.80	202.0
78.90	1634.0
79.90	595.0
80.90	1508.0
82.00	349.0
85.90	121.0
87.00	1764.0
88.00	1692.0
90.90	151.0
91.90	1359.0
93.00	1653.0
94.00	4836.0
95.00	41952.0
96.00	2840.0
104.00	141.0
105.90	140.0
115.80	160.0
116.80	315.0
117.90	199.0
118.90	277.0
127.80	117.0
129.90	143.0
140.80	255.0
142.90	632.0
144.90	314.0
156.80	108.0
171.00	216.0
171.80	605.0
173.00	559.0
173.90	37552.0
174.90	2632.0
175.90	36744.0
176.90	2095.0
206.80	114.0

Instrument :
MSVOA_V
ClientSampleId :
BFB73