

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090619\
 Data File : VV012615.D
 Acq On : 06 Sep 2019 23:05
 Operator : SY/MD
 Sample : K4685-06DL 5X
 Misc : 25mL/MSVOA V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFD75DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.1

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR090519WMA.M

Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.225	38	42	47	rBV	8915	8702	1.47%	0.157%
2	1.319	62	71	79	rBV	111031	118095	19.95%	2.132%
3	1.582	146	153	165	rVB	103008	118903	20.09%	2.146%
4	2.129	314	323	338	rVB2	202603	299861	50.66%	5.412%
5	2.534	443	449	456	rVB6	6959	10761	1.82%	0.194%
6	3.975	881	897	925	rBV2	51872	225914	38.17%	4.078%
7	4.399	1012	1029	1051	rBV2	110419	282202	47.68%	5.094%
8	5.093	1230	1245	1268	rBV2	237276	570619	96.41%	10.300%
9	5.663	1409	1422	1444	rBV	179433	368107	62.19%	6.644%
10	5.958	1500	1514	1537	rBV	254071	504580	85.25%	9.108%
11	6.116	1550	1563	1586	rVB	144144	296278	50.06%	5.348%
12	7.029	1837	1847	1860	rBV2	58751	105050	17.75%	1.896%
13	7.360	1935	1950	1970	rBV	223399	407681	68.88%	7.359%
14	7.666	2035	2045	2062	rBV	36655	67514	11.41%	1.219%
15	8.016	2142	2154	2171	rBV	159029	270888	45.77%	4.889%
16	8.145	2182	2194	2227	rBV2	202810	591865	100.00%	10.683%
17	8.894	2414	2427	2444	rBV	288043	483630	81.71%	8.729%
18	10.260	2841	2852	2864	rBV	91511	148162	25.03%	2.674%
19	11.293	3162	3173	3192	rBV	200944	337956	57.10%	6.100%
20	11.672	3279	3291	3311	rVB	188148	323471	54.65%	5.839%


Sum of corrected areas: 5540239

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV090619\
Data File : VV012615.D
Acq On : 06 Sep 2019 23:05
Operator : SY/MD
Sample : K4685-06DL 5X
Misc : 25mL/MSVOA V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFD75DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR090519WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

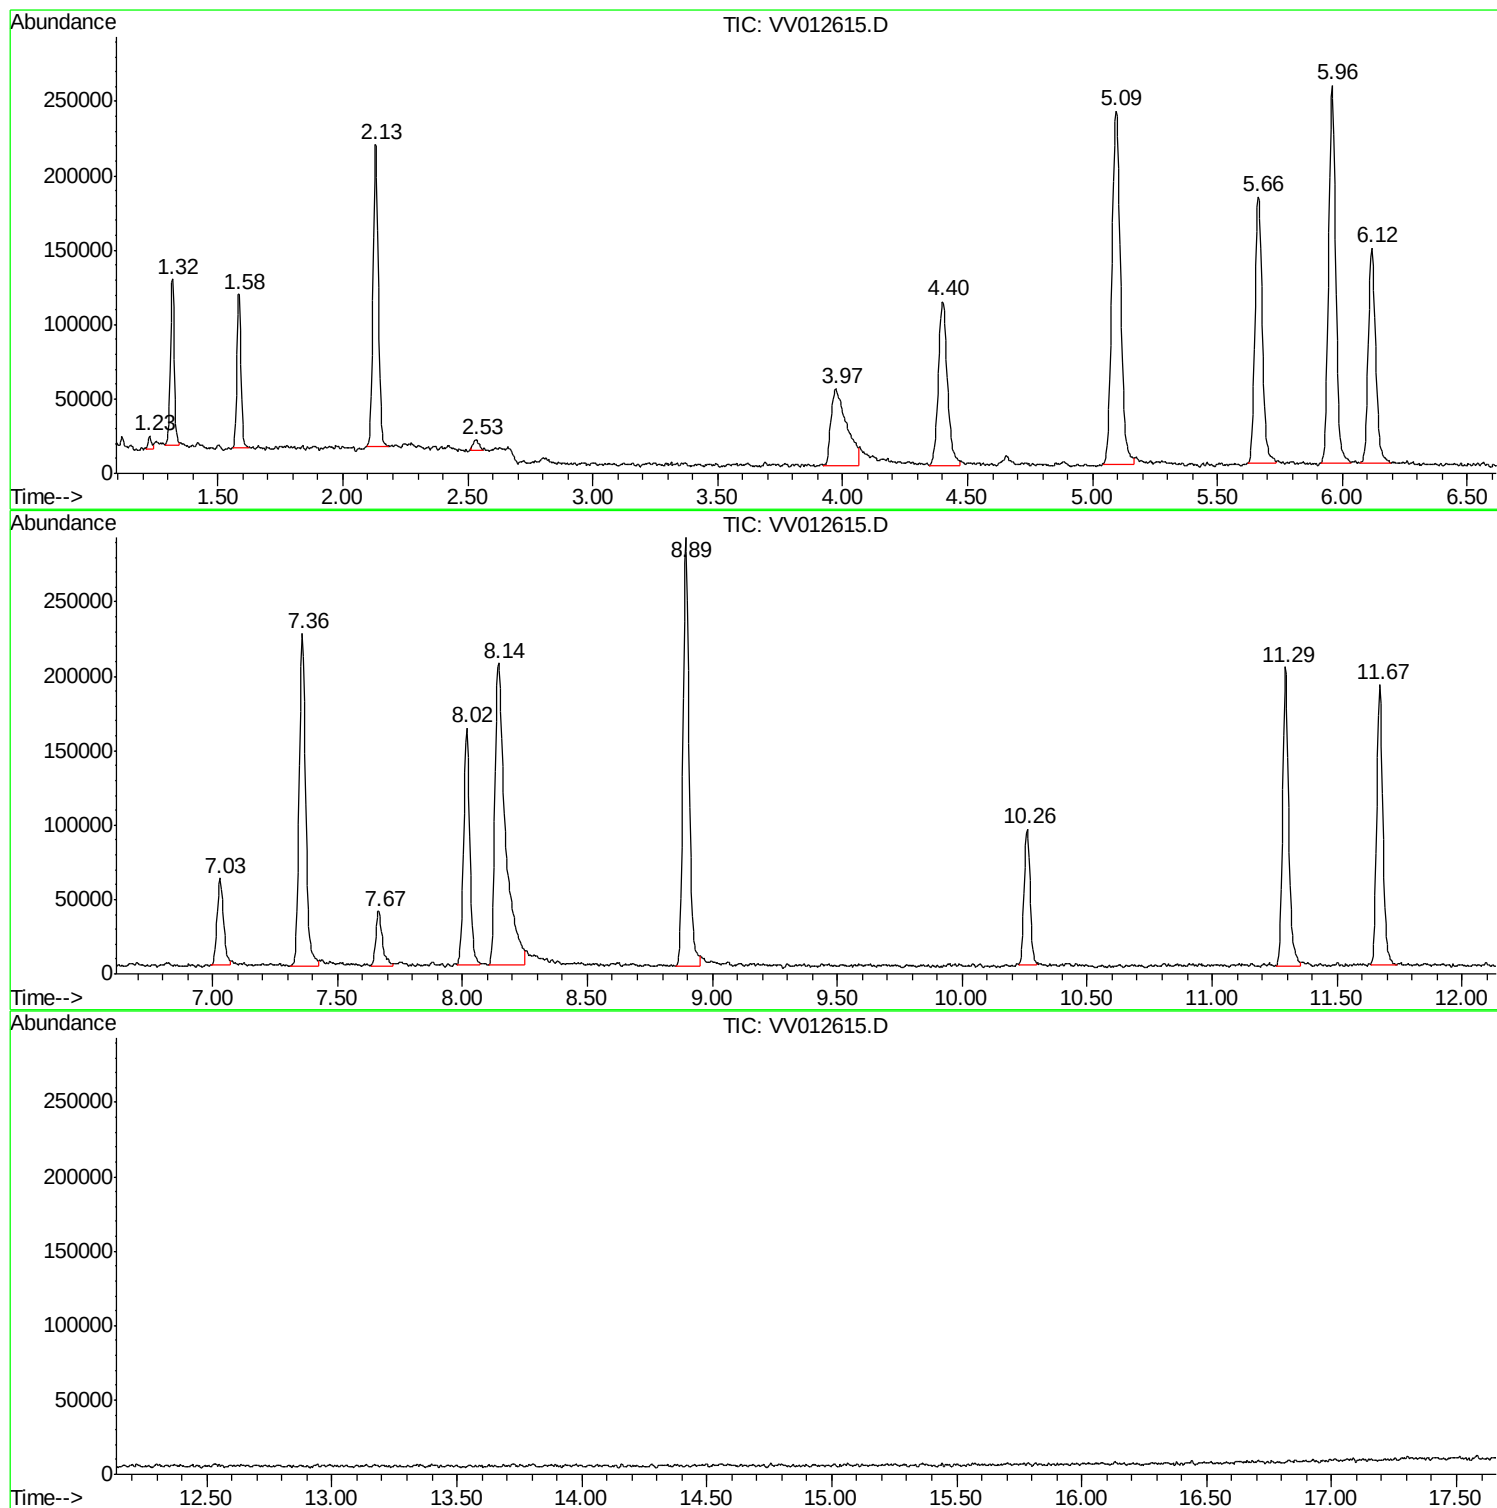

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV090619\
Data File : VV012615.D
Acq On : 06 Sep 2019 23:05
Operator : SY/MD
Sample : K4685-06DL 5X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFD75DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR090519WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV090619\
Data File : VV012615.D
Acq On : 06 Sep 2019 23:05
Operator : SY/MD
Sample : K4685-06DL 5X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFD75DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR090519WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc