

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090619\
 Data File : VV012619.D
 Acq On : 07 Sep 2019 00:51
 Operator : SY/MD
 Sample : K4685-08DL 50X
 Misc : 25mL/MSVOA V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFD77DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.1

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR090519WMA.M

Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.225	38	42	46	RBV3	9490	8124	1.21%	0.151%
2	1.319	63	71	81	rVB	112533	116473	17.30%	2.166%
3	1.582	146	153	163	rVB	99639	110073	16.35%	2.047%
4	2.129	314	323	337	rBV	190401	268729	39.91%	4.997%
5	2.534	442	449	458	rVB2	9380	13301	1.98%	0.247%
6	3.974	879	897	925	RBV2	53764	245291	36.43%	4.561%
7	4.399	1011	1029	1051	rBV	105037	266417	39.56%	4.954%
8	5.093	1229	1245	1270	RBV2	228261	559228	83.05%	10.398%
9	5.662	1408	1422	1440	rBV	171869	349002	51.83%	6.489%
10	5.949	1502	1511	1520	rVB	10296	18973	2.82%	0.353%
11	6.116	1547	1563	1579	RBV2	141502	299757	44.52%	5.573%
12	7.029	1833	1847	1863	RBV2	55592	106807	15.86%	1.986%
13	7.360	1936	1950	1967	rBV	214545	386592	57.41%	7.188%
14	7.666	2034	2045	2058	RBV2	34678	61558	9.14%	1.145%
15	8.016	2142	2154	2168	rBV	398322	673381	100.00%	12.520%
16	8.145	2182	2194	2233	RBV2	225918	626981	93.11%	11.658%
17	8.894	2415	2427	2444	rBV	270069	460403	68.37%	8.560%
18	10.260	2842	2852	2863	rBV	99486	165187	24.53%	3.071%
19	11.293	3162	3173	3192	rBV	186443	318876	47.35%	5.929%
20	11.672	3277	3291	3311	rBV	184088	323109	47.98%	6.008%


Sum of corrected areas: 5378262

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV090619\
Data File : VV012619.D
Acq On : 07 Sep 2019 00:51
Operator : SY/MD
Sample : K4685-08DL 50X
Misc : 25mL/MSVOA V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFD77DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR090519WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

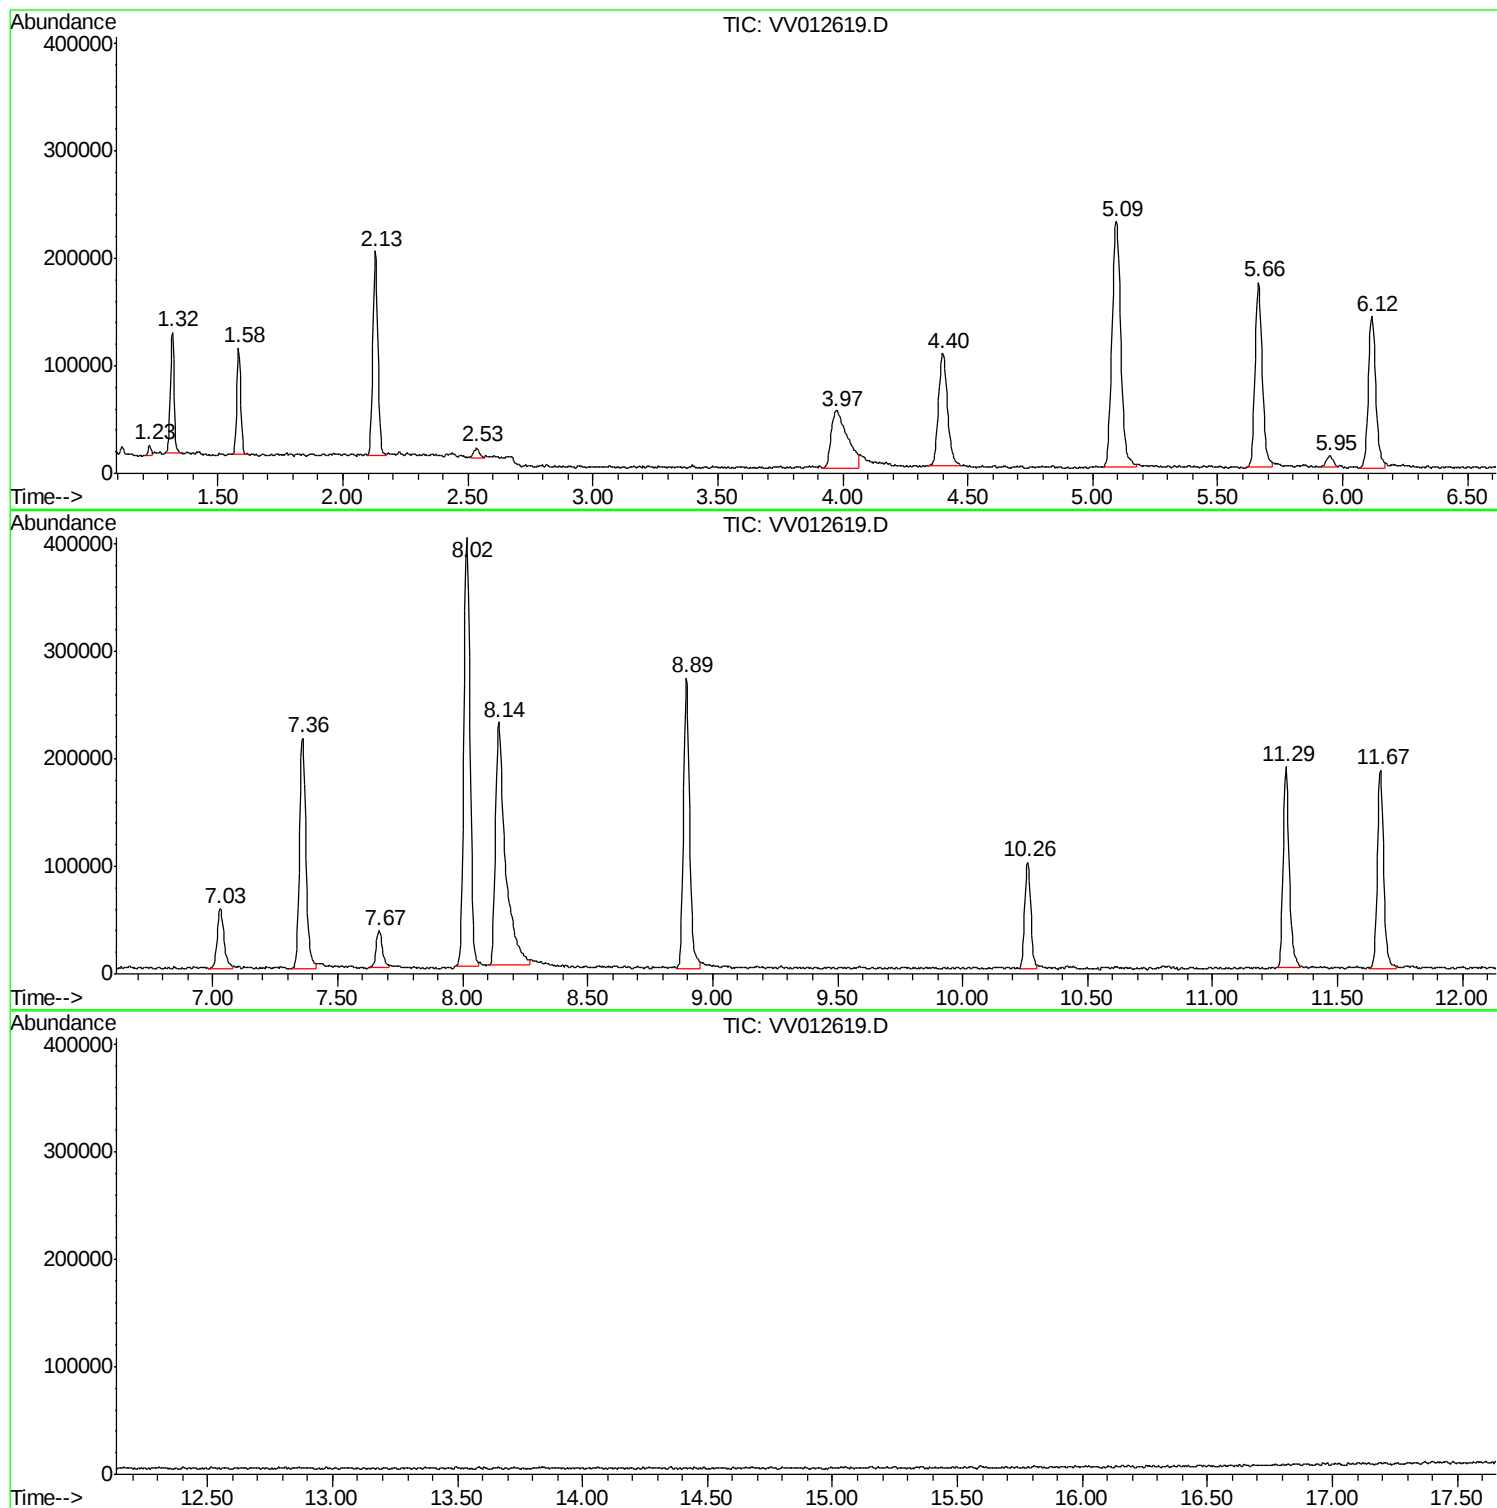

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV090619\
Data File : VV012619.D
Acq On : 07 Sep 2019 00:51
Operator : SY/MD
Sample : K4685-08DL 50X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFD77DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR090519WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV090619\
Data File : VV012619.D
Acq On : 07 Sep 2019 00:51
Operator : SY/MD
Sample : K4685-08DL 50X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFD77DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR090519WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc