


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV090619\
Data File : VV012588.D
Acq On : 06 Sep 2019 08:30
Operator : SY/MD
Sample : BFB32
Misc : 25mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB32

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR090519WMA.M
Title : TRACE VOA SOM01.0
Last Update : Sat Sep 07 01:06:07 2019

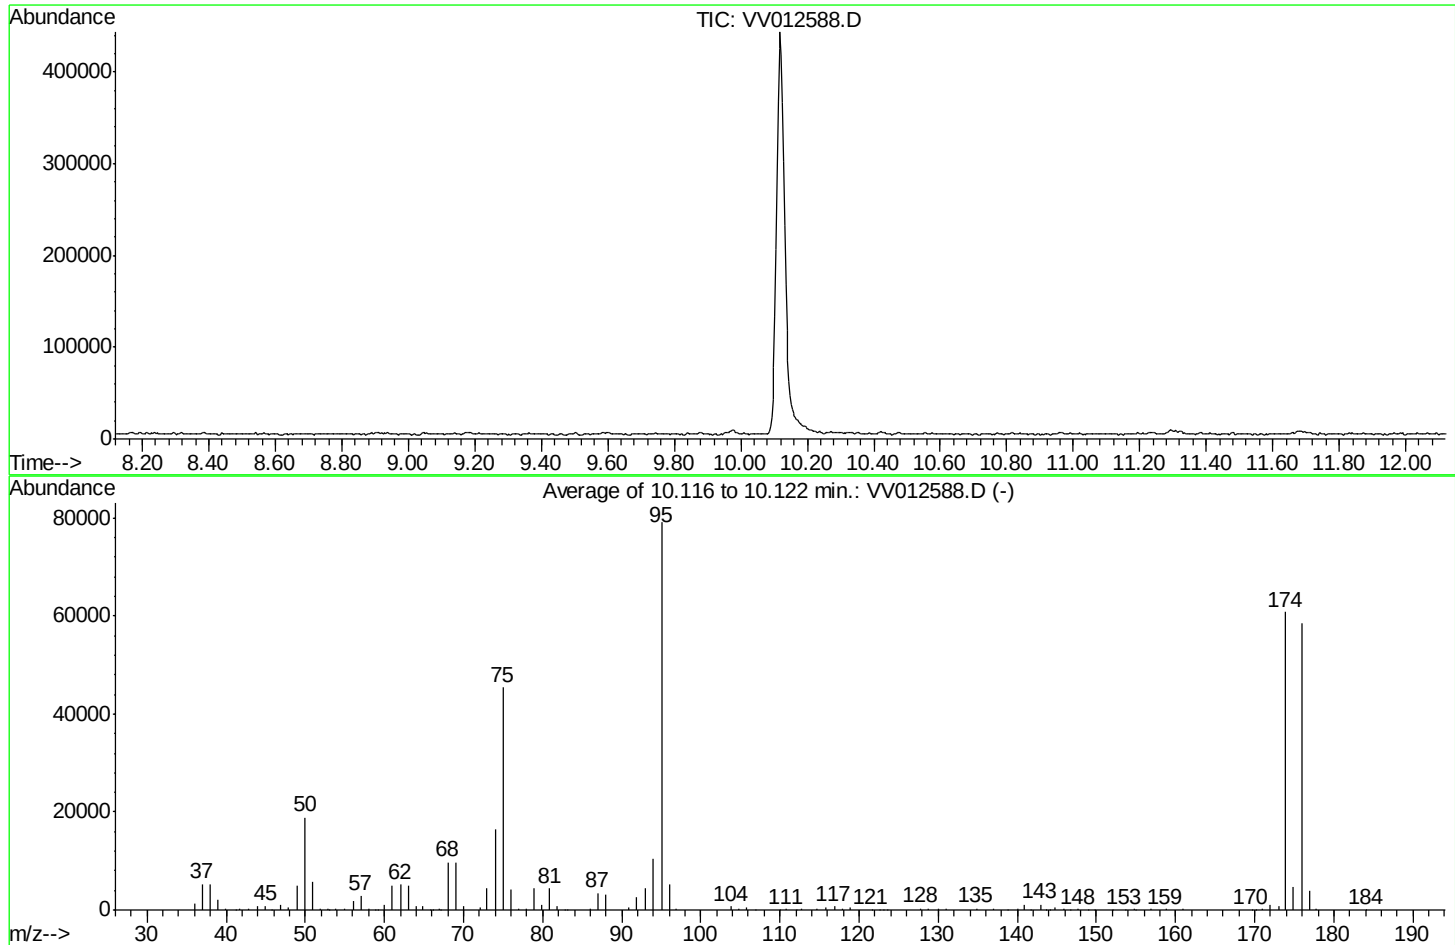

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.8	18853	PASS
75	95	30	80	57.4	45432	PASS
95	95	100	100	100.0	79138	PASS
96	95	5	9	6.8	5364	PASS
173	174	0.00	2	1.2	715	PASS
174	95	50	120	76.8	60760	PASS
175	174	5	9	7.7	4694	PASS
176	174	95	101	96.5	58634	PASS
177	176	5	9	6.9	4057	PASS

m/z	Abundance
36.00	1354.0
37.00	5414.0
38.00	5498.0
39.00	2324.0
39.90	857.0
41.10	235.0
41.60	121.0
42.20	114.0
42.80	315.0
44.00	1325.0
45.00	908.0
45.80	197.0
46.90	1190.0
47.90	679.0
49.00	4810.0
50.00	18584.0
51.00	6141.0
51.90	413.0
52.80	239.0
53.70	144.0
54.90	397.0
56.00	1794.0
57.00	3179.0
58.00	321.0
60.00	1085.0
61.00	4814.0
62.00	5391.0
63.00	4911.0
64.00	860.0
64.90	796.0
65.80	163.0
66.90	323.0
68.00	9817.0
69.00	9584.0
70.10	900.0
72.10	569.0
73.00	4280.0
74.00	16824.0
75.00	45264.0
76.00	4432.0
77.10	428.0
78.00	376.0
78.90	4402.0
79.90	1164.0
80.90	4317.0
81.80	904.0
83.10	130.0
86.00	156.0
86.90	3559.0
87.90	3131.0
90.80	473.0
91.90	2818.0
93.00	4467.0
94.00	10535.0
95.00	78416.0
96.00	5487.0
96.90	311.0
103.90	665.0
104.80	199.0
105.80	418.0
106.70	105.0
107.00	110.0
107.80	176.0
110.00	105.0
110.80	149.0
112.00	126.0
112.60	159.0
114.70	215.0
115.80	481.0
116.90	669.0
117.80	377.0
118.90	600.0
122.60	104.0
123.60	106.0
127.80	390.0
128.80	208.0
130.00	330.0
131.00	140.0
134.90	287.0
137.00	206.0
140.10	178.0
140.90	870.0
141.90	192.0
142.90	1127.0
143.60	110.0
144.10	166.0
144.80	454.0
145.90	243.0
147.70	222.0
149.00	129.0
149.70	112.0
154.80	239.0

Instrument :
MSVOA_V
ClientSampleId :
BFB32

157.00	152.0
158.70	290.0
160.80	186.0
169.60	118.0
170.90	248.0
172.00	998.0
173.00	1051.0
173.90	58696.0
174.90	4859.0
175.90	56256.0
176.90	3879.0
177.80	191.0

Instrument :
MSVOA_V
ClientSampleId :
BFB32

m/z	Abundance
36.00	1351.0
37.00	5667.0
38.00	5449.0
39.00	2328.0
39.90	816.0
41.10	213.0
41.70	139.0
42.80	240.0
44.00	1382.0
45.00	881.0
47.00	1224.0
47.90	778.0
49.00	5075.0
50.00	19448.0
51.00	6157.0
52.00	367.0
52.80	245.0
53.70	168.0
54.90	395.0
56.00	1851.0
57.00	3252.0
58.00	339.0
58.90	113.0
59.20	119.0
60.10	1190.0
61.00	5119.0
62.00	5364.0
63.00	5091.0
64.00	815.0
64.90	789.0
65.80	128.0
66.90	345.0
68.00	10009.0
69.00	9915.0
70.00	921.0
72.10	496.0
73.00	4491.0
74.00	17128.0
75.00	47024.0
76.00	4235.0
76.90	366.0
78.00	360.0
78.90	4534.0
79.90	1182.0
80.90	4516.0
81.80	868.0
83.10	143.0
86.00	209.0
87.00	3687.0
88.00	3295.0
90.90	570.0
91.90	2873.0
93.00	4560.0
94.00	10814.0
95.00	81760.0
96.00	5455.0
96.90	265.0
103.80	735.0
104.90	194.0
105.80	462.0
106.70	121.0
106.90	123.0
107.80	116.0
110.00	109.0
110.80	181.0
112.00	129.0
112.70	164.0
114.70	232.0
115.80	521.0
116.90	713.0
117.90	418.0
118.90	678.0
121.60	112.0
122.60	105.0
123.10	101.0
127.80	372.0
128.80	265.0
130.00	327.0
131.00	165.0
134.90	295.0
137.00	211.0
138.70	103.0
140.00	172.0
140.90	1025.0
141.80	175.0
142.90	1119.0
144.20	137.0
144.80	473.0
145.80	237.0
146.70	109.0
147.70	255.0
149.00	142.0

Instrument :
MSVOA_V
ClientSampleId :
BFB32

149.70	148.0
152.00	104.0
153.60	105.0
154.80	193.0
156.90	213.0
158.70	246.0
160.80	183.0
169.70	116.0
170.20	120.0
171.00	265.0
172.00	999.0
173.00	1096.0
173.90	62440.0
174.90	4860.0
175.90	60704.0
176.90	4247.0
177.80	138.0
184.10	103.0

Instrument :
MSVOA_V
ClientSampleId :
BFB32

m/z	Abundance
36.00	1200.0
37.00	5524.0
38.00	4902.0
39.00	2118.0
39.90	764.0
41.20	173.0
41.80	160.0
42.80	176.0
44.00	1362.0
44.90	820.0
47.00	1100.0
47.90	801.0
49.00	4713.0
50.00	18528.0
51.00	5699.0
52.00	326.0
53.00	227.0
53.80	178.0
54.90	365.0
56.10	1604.0
57.00	3024.0
58.00	262.0
58.90	106.0
60.10	1087.0
61.00	5101.0
62.00	4912.0
63.00	4792.0
64.00	719.0
64.90	847.0
66.10	145.0
67.10	360.0
68.00	9198.0
69.00	9501.0
70.00	877.0
72.00	466.0
72.90	4377.0
74.00	15809.0
75.00	44008.0
76.00	3799.0
76.90	352.0
78.90	4156.0
79.90	1064.0
80.90	4281.0
81.80	812.0
82.80	142.0
86.00	217.0
86.90	3276.0
88.00	3270.0
90.90	595.0
91.90	2534.0
93.00	4116.0
94.00	9928.0
95.00	77240.0
96.00	5151.0
96.90	213.0
103.80	610.0
104.90	166.0
105.80	508.0
106.90	144.0
110.80	229.0
112.00	129.0
112.70	157.0
114.60	165.0
115.80	516.0
116.90	734.0
117.90	404.0
118.90	659.0
121.60	111.0
123.10	101.0
123.60	100.0
127.80	341.0
128.80	250.0
129.90	284.0
130.90	184.0
134.80	242.0
137.00	181.0
138.70	133.0
139.90	154.0
140.90	1068.0
141.70	177.0
142.90	1079.0
144.80	435.0
145.80	264.0
147.70	224.0
149.00	128.0
149.70	144.0
155.00	207.0
156.90	227.0
158.80	192.0
160.90	156.0
170.10	147.0
170.90	228.0

Instrument :
MSVOA_V
ClientSampleId :
BFB32

172.00	879.0
173.90	61144.0
174.90	4365.0
175.90	58944.0
176.90	4045.0
177.90	107.0

Instrument :
MSVOA_V
ClientSampleId :
BFB32

m/z	Abundance
35.00	144.0
35.70	124.0
36.30	141.0
36.80	195.0
37.50	261.0
38.40	166.0
39.10	152.0
40.00	630.0
41.20	152.0
42.10	117.0
43.10	128.0
44.00	631.0
45.50	128.0
46.40	147.0
46.80	105.0
47.50	102.0
48.10	169.0
50.90	126.0
52.10	134.0
54.10	120.0
57.00	149.0
61.10	130.0
63.90	116.0
72.70	113.0
83.90	100.0
88.90	102.0
94.70	129.0
106.80	133.0
107.90	119.0
141.70	126.0

Instrument :
MSVOA_V
ClientSampleId :
BFB32