

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090622\
 Data File : VV027755.D
 Acq On : 06 Sep 2022 20:53
 Operator : SY/MD
 Sample : N4418-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBVG8

Quant Time: Sep 07 06:30:10 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Sep 07 06:13:02 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	149993	5.000	ug/L	0.02
28) Chlorobenzene-d5	8.850	117	144093	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	65487	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	53113	5.372	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	= 107.400%		
7) Chloroethane-d5	1.568	69	48106	5.736	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	= 114.800%		
11) 1,1-Dichloroethene-d2	2.105	63	86169	4.107	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	= 82.200%		
20) 2-Butanone-d5	3.899	46	79797	36.418	ug/L	-0.04
Spiked Amount	50.000	Range 40 - 130	Recovery	= 72.840%		
24) Chloroform-d	4.346	84	104822	5.178	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 103.600%		
26) 1,2-Dichloroethane-d4	5.031	65	50877	4.719	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 94.400%		
32) Benzene-d6	5.047	84	192616	4.608	ug/L	0.02
Spiked Amount	5.000	Range 70 - 125	Recovery	= 92.200%		
36) 1,2-Dichloropropane-d6	6.066	67	62577	5.113	ug/L	0.02
Spiked Amount	5.000	Range 60 - 140	Recovery	= 102.200%		
41) Toluene-d8	7.313	98	158367	4.505	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 90.200%		
43) trans-1,3-Dichloroprop...	7.625	79	18530	4.513	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	= 90.200%		
46) 2-Hexanone-d5	8.088	63	71548	46.878	ug/L	-0.03
Spiked Amount	50.000	Range 45 - 130	Recovery	= 93.760%		
56) 1,1,2,2-Tetrachloroeth...	10.214	84	37578	4.781	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	= 95.600%		
66) 1,2-Dichlorobenzene-d4	11.622	152	61153	5.684	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	= 113.600%		
Target Compounds						
13) Acetone	2.179	43	12542	7.682	ug/L	Qvalue 75
14) Carbon disulfide	2.291	76	30214	1.024	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090622\
Data File : VV027755.D
Acq On : 06 Sep 2022 20:53
Operator : SY/MD
Sample : N4418-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVG8

Quant Time: Sep 07 06:30:10 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Sep 07 06:13:02 2022
Response via : Initial Calibration




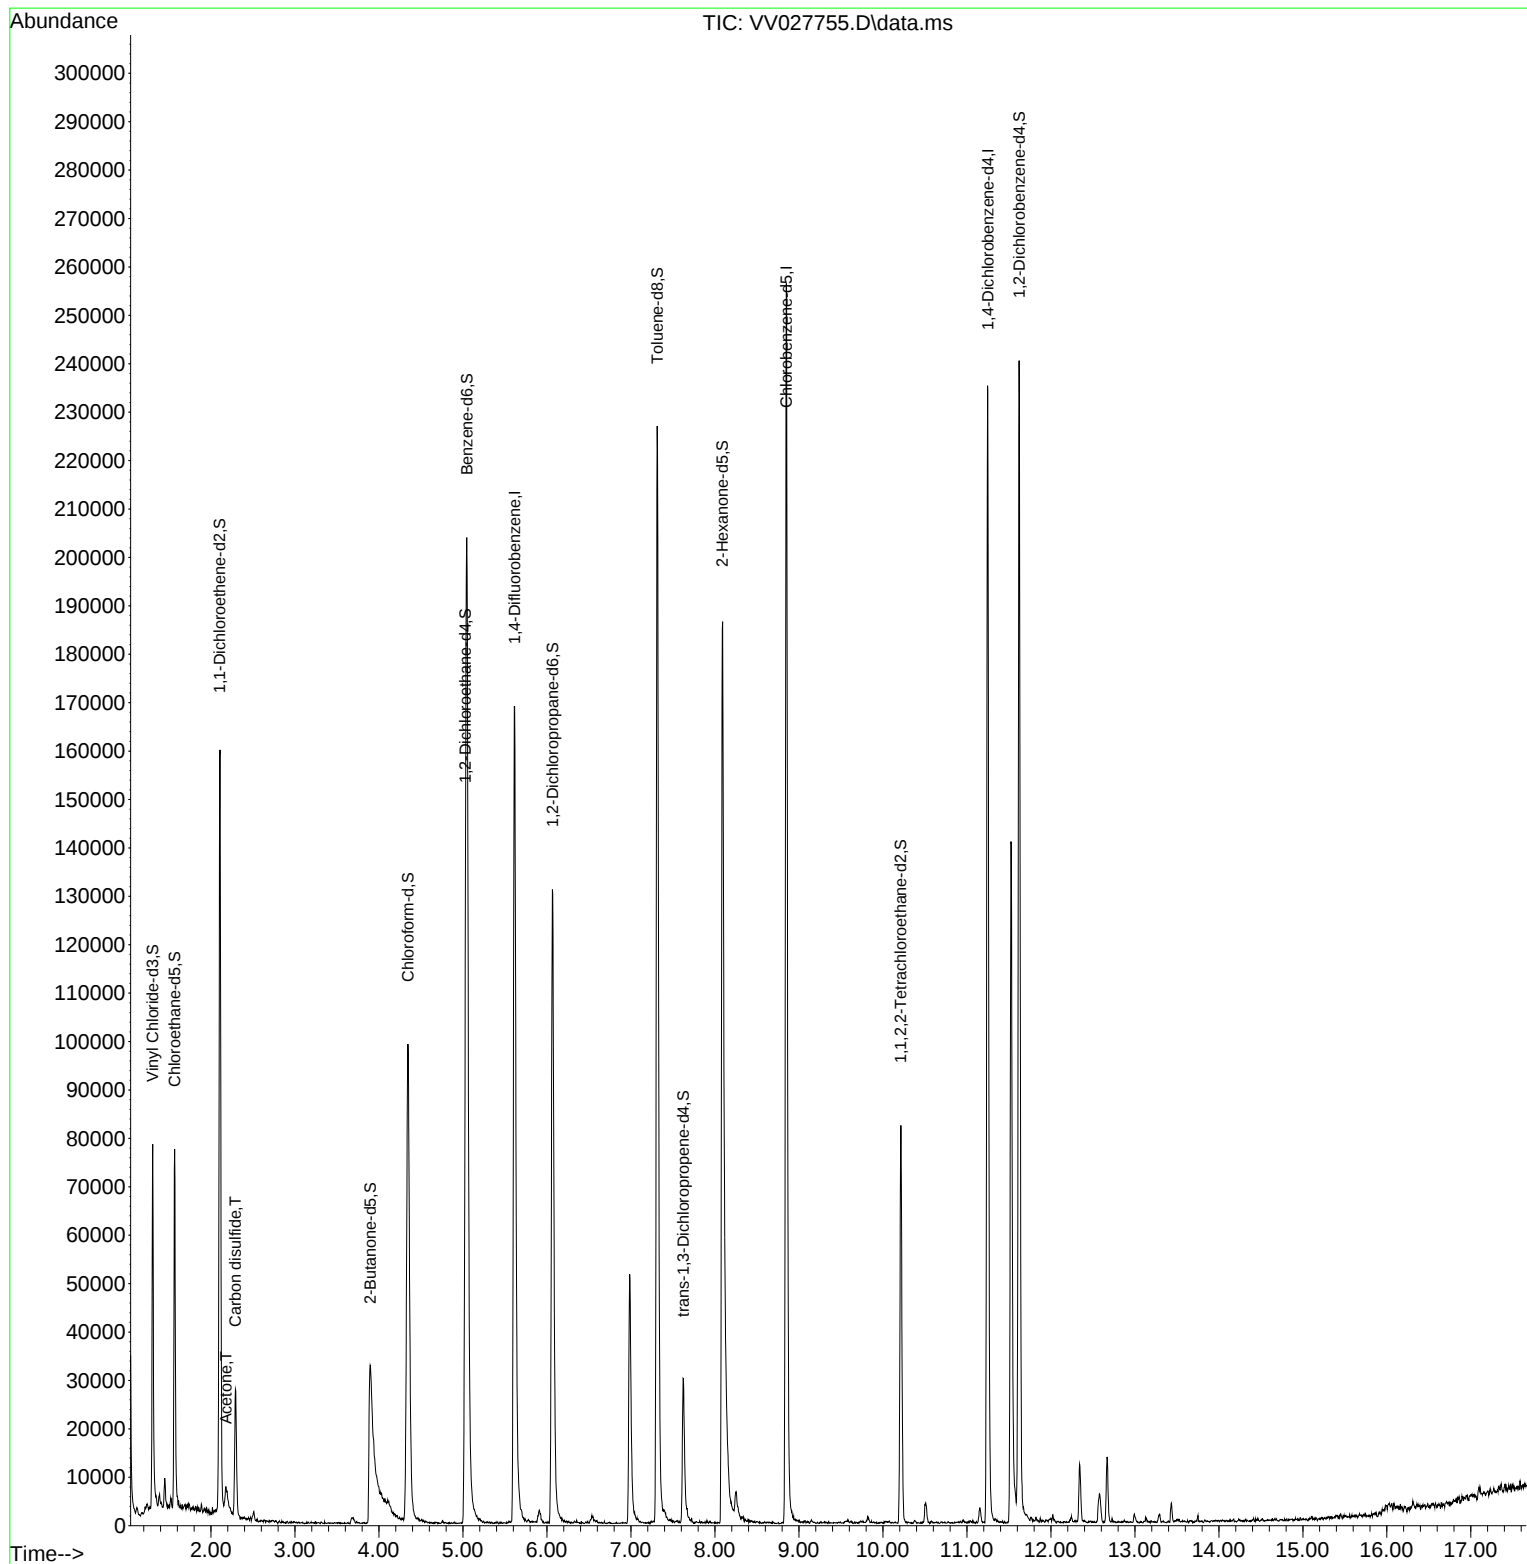


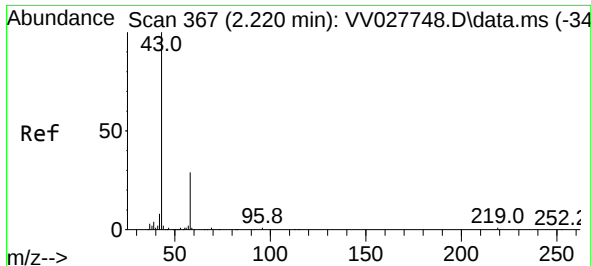

#13
Acetone
Concen: 7.682 ug/L
RT: 2.179 min Scan# 31
Delta R.T. -0.042 min
Lab File: VV027755.D
Acq: 06 Sep 2022 20:53

Instrument :
MSVOA_V
ClientSampleId :
DBVG8

Tgt Ion: 43 Resp: 12542
Ion Ratio Lower Upper
43 100
58 12.3 0.0 49.4

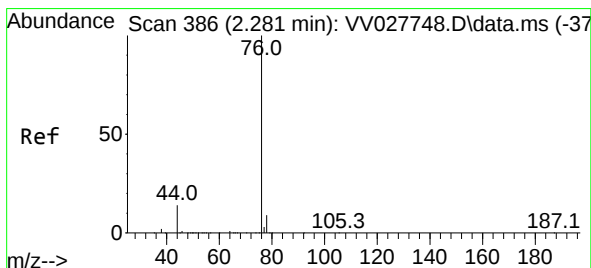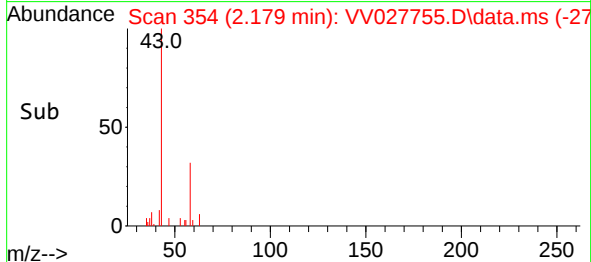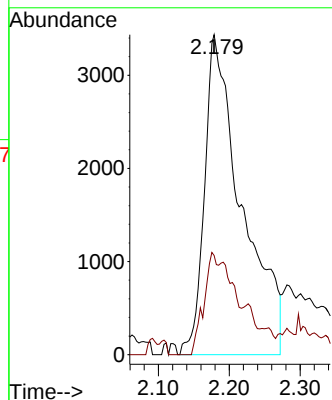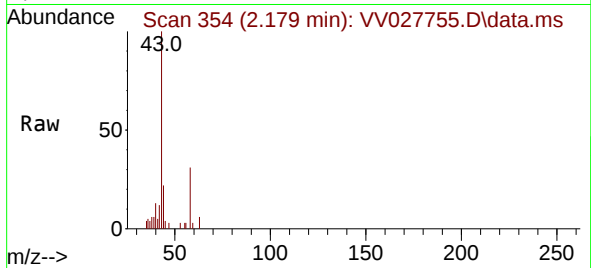

#14
Carbon disulfide
Concen: 1.024 ug/L
RT: 2.291 min Scan# 389
Delta R.T. 0.010 min
Lab File: VV027755.D
Acq: 06 Sep 2022 20:53

Tgt Ion: 76 Resp: 30214
Ion Ratio Lower Upper
76 100
78 9.5 7.7 11.5

