

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW090622\
 Data File : VW027765.D
 Acq On : 07 Sep 2022 00:57
 Operator : SY/MD
 Sample : N4402-17DL 10X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBVE9DL

Quant Time: Sep 07 06:32:47 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Sep 07 06:13:02 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	141655	5.000	ug/L	0.02
28) Chlorobenzene-d5	8.850	117	139857	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	62659	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	47035	5.037	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	= 100.800%		
7) Chloroethane-d5	1.568	69	43162	5.449	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	= 109.000%		
11) 1,1-Dichloroethene-d2	2.108	63	76370	3.854	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	= 77.000%		
20) 2-Butanone-d5	3.896	46	61165	29.558	ug/L	-0.04
Spiked Amount	50.000	Range 40 - 130	Recovery	= 59.120%		
24) Chloroform-d	4.346	84	98584	5.156	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 103.200%		
26) 1,2-Dichloroethane-d4	5.031	65	48778	4.791	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 95.800%		
32) Benzene-d6	5.047	84	178927	4.410	ug/L	0.02
Spiked Amount	5.000	Range 70 - 125	Recovery	= 88.200%		
36) 1,2-Dichloropropane-d6	6.066	67	52436	4.414	ug/L	0.02
Spiked Amount	5.000	Range 60 - 140	Recovery	= 88.200%		
41) Toluene-d8	7.313	98	147306	4.318	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 86.400%		
43) trans-1,3-Dichloroprop...	7.625	79	16460	4.130	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	= 82.600%		
46) 2-Hexanone-d5	8.088	63	67301	45.431	ug/L	-0.03
Spiked Amount	50.000	Range 45 - 130	Recovery	= 90.860%		
56) 1,1,2,2-Tetrachloroeth...	10.214	84	35389	4.639	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	= 92.800%		
66) 1,2-Dichlorobenzene-d4	11.622	152	52239	5.075	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	= 101.600%		
Target Compounds						
47) Tetrachloroethene	7.973	164	59326	6.394	ug/L	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090622\
Data File : VV027765.D
Acq On : 07 Sep 2022 00:57
Operator : SY/MD
Sample : N4402-17DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVE9DL

Quant Time: Sep 07 06:32:47 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Sep 07 06:13:02 2022
Response via : Initial Calibration

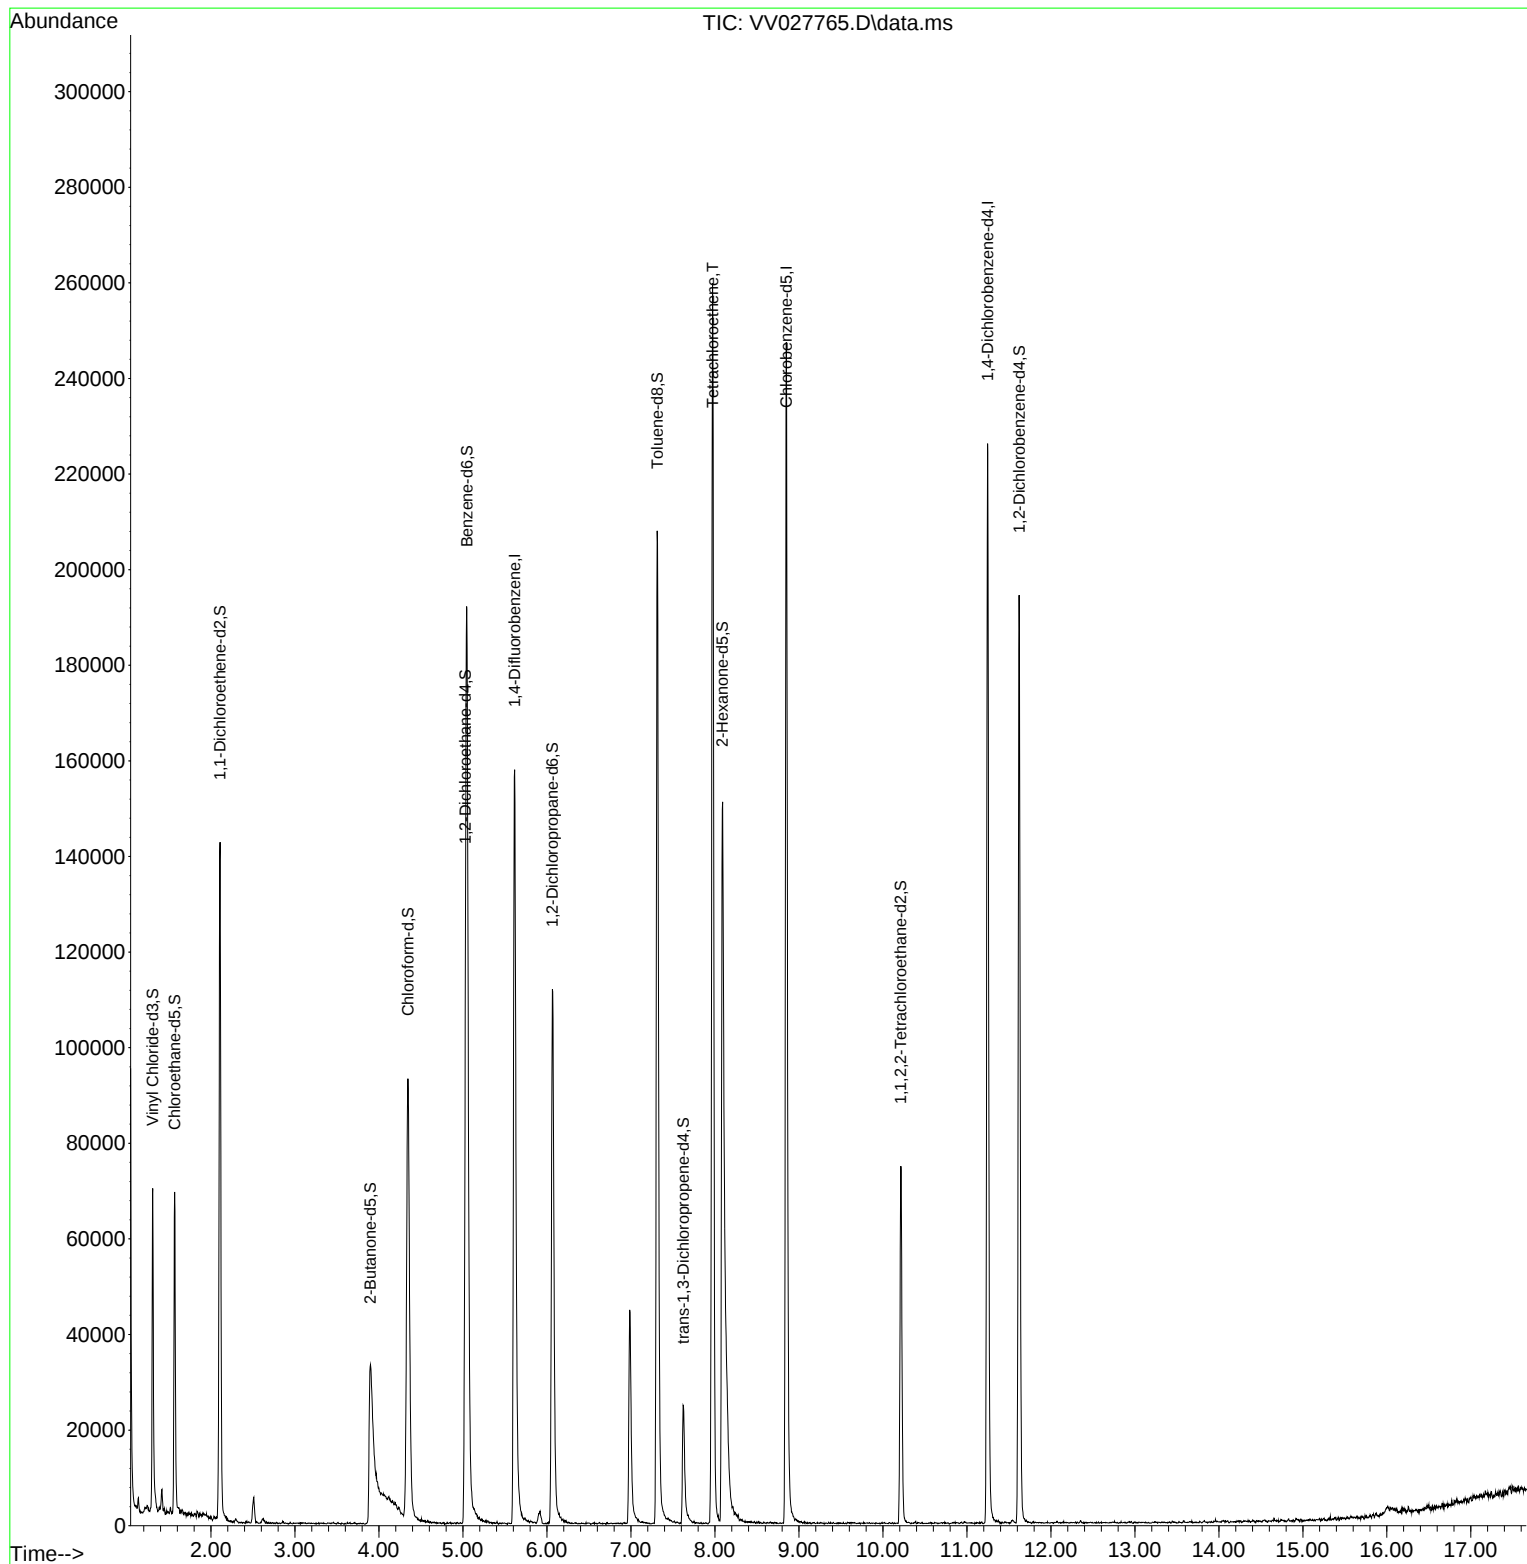

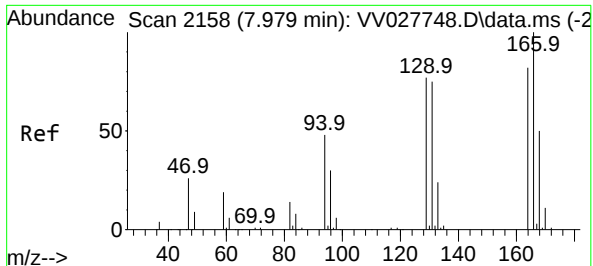

#47
 Tetrachloroethene
 Concen: 6.394 ug/L
 RT: 7.973 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: VV027765.D
 Acq: 07 Sep 2022 00:57

Instrument :
 MSVOA_V
 ClientSampleId :
 DBVE9DL

Tgt Ion:	164	Resp:	59326
Ion	Ratio	Lower	Upper
164	100		
129	92.6	67.2	124.8
131	87.2	61.5	114.3
166	125.0	91.1	169.3

