

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090622\
 Data File : VV027757.D
 Acq On : 06 Sep 2022 21:42
 Operator : SY/MD
 Sample : N4418-11DL 10X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBVE7DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV027757.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	100	rVB	74310	86941	17.55%	1.840%
2	1.413	111	116	126	rVB	5147	5853	1.18%	0.124%
3	1.568	156	164	181	rVB	68942	80688	16.29%	1.708%
4	2.105	321	331	348	rVB	145291	208773	42.15%	4.420%
5	2.506	446	456	467	rBV3	4555	7388	1.49%	0.156%
6	3.908	873	892	924	rBV3	107980	349687	70.60%	7.403%
7	4.346	1012	1028	1053	rBV2	92777	231928	46.83%	4.910%
8	5.043	1230	1245	1268	rBV2	195607	495294	100.00%	10.485%
9	5.612	1411	1422	1445	rBV	166393	348539	70.37%	7.378%
10	5.911	1501	1515	1539	rBV	108418	222800	44.98%	4.717%
11	6.066	1550	1563	1590	rBV2	118042	246224	49.71%	5.212%
12	6.985	1839	1849	1868	rBV	46820	91057	18.38%	1.928%
13	7.313	1939	1951	1971	rBV	212770	379391	76.60%	8.031%
14	7.622	2039	2047	2063	rBV2	27660	50914	10.28%	1.078%
15	7.972	2142	2156	2172	rBV2	162433	279381	56.41%	5.914%
16	8.091	2183	2193	2221	rBV	161090	391083	78.96%	8.279%
17	8.850	2418	2429	2458	rBV	260904	434868	87.80%	9.206%
18	10.214	2842	2853	2867	rBV	75163	123243	24.88%	2.609%
19	11.249	3164	3175	3199	rBV	234104	372870	75.28%	7.893%
20	11.535	3253	3264	3280	rBV6	4347	7890	1.59%	0.167%
21	11.622	3280	3291	3311	rBV	191479	308987	62.38%	6.541%




Sum of corrected areas: 4723799

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090622\
Data File : VV027757.D
Acq On : 06 Sep 2022 21:42
Operator : SY/MD
Sample : N4418-11DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVE7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

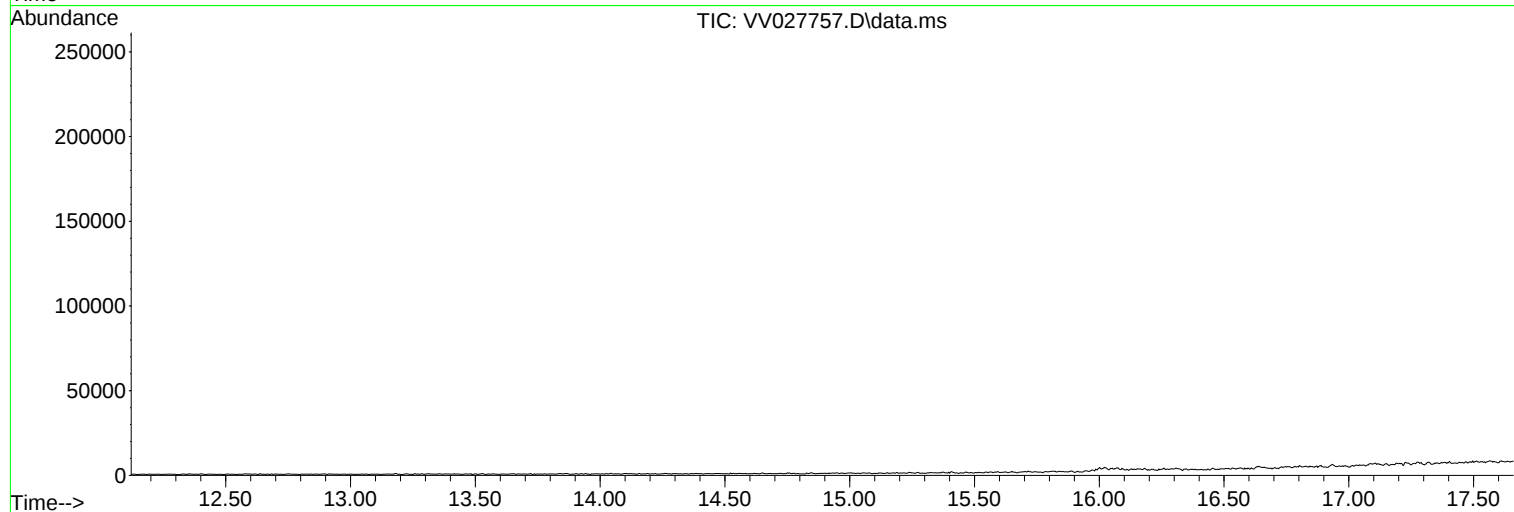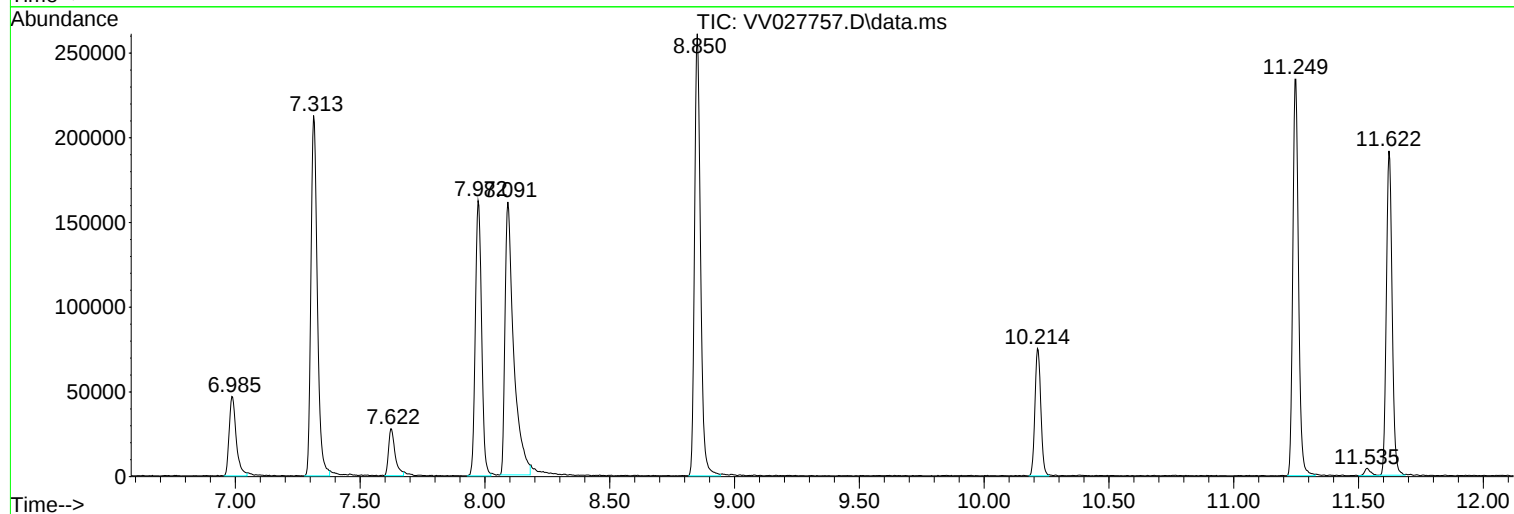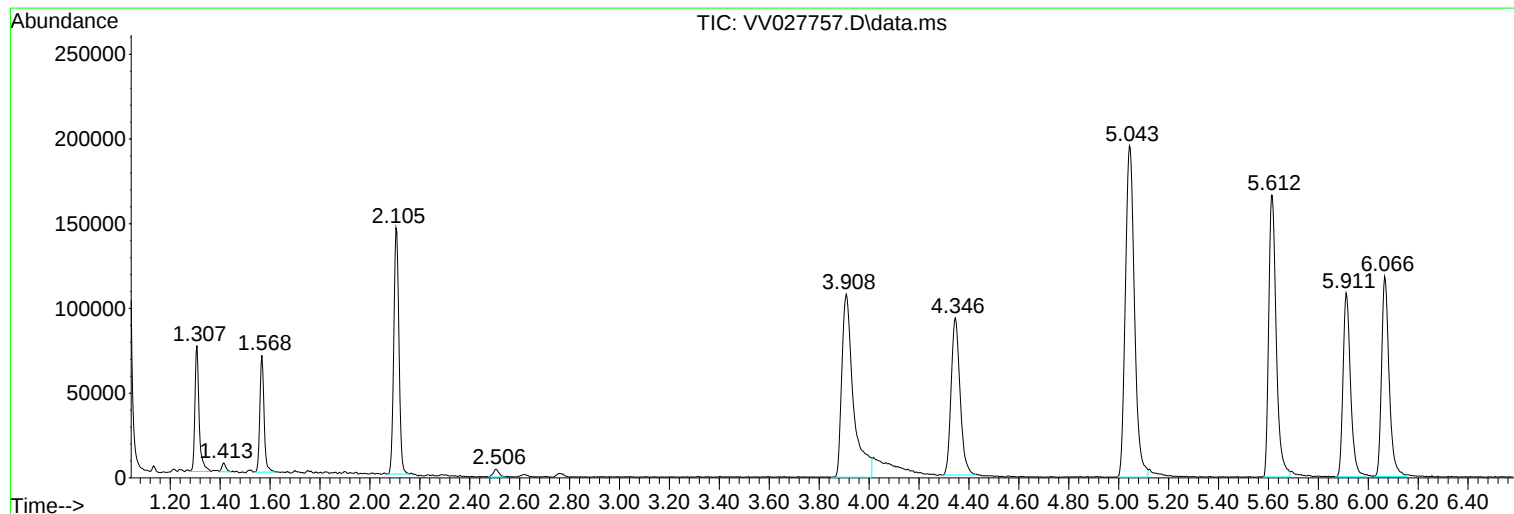

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090622\
Data File : VV027757.D
Acq On : 06 Sep 2022 21:42
Operator : SY/MD
Sample : N4418-11DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVE7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090622\
Data File : VV027757.D
Acq On : 06 Sep 2022 21:42
Operator : SY/MD
Sample : N4418-11DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVE7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
