

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090622\
 Data File : VV027759.D
 Acq On : 06 Sep 2022 22:31
 Operator : SY/MD
 Sample : N4402-19
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBVF7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027759.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	100	rBV	69061	76869	15.70%	1.902%
2	1.452	119	128	137	rVB6	4018	5140	1.05%	0.127%
3	1.568	156	164	178	rVB	69261	80240	16.39%	1.985%
4	2.108	320	332	346	rBV	148893	216230	44.16%	5.349%
5	2.767	523	537	553	rBV3	21310	46432	9.48%	1.149%
6	3.892	877	887	914	rBV	27038	93090	19.01%	2.303%
7	4.346	1011	1028	1055	rBV	93671	238480	48.70%	5.899%
8	5.043	1229	1245	1271	rBV2	194326	489704	100.00%	12.114%
9	5.616	1412	1423	1449	rBV	161002	332905	67.98%	8.235%
10	5.912	1501	1515	1527	rBV9	3262	8271	1.69%	0.205%
11	6.066	1548	1563	1584	rBV	114129	239689	48.95%	5.929%
12	6.986	1839	1849	1873	rBV	47350	92420	18.87%	2.286%
13	7.313	1939	1951	1974	rBV	213686	382526	78.11%	9.463%
14	7.622	2036	2047	2066	rBV2	27095	51906	10.60%	1.284%
15	7.976	2146	2157	2174	rVB3	23263	40654	8.30%	1.006%
16	8.092	2183	2193	2229	rBV	148247	393917	80.44%	9.744%
17	8.850	2417	2429	2456	rBV	247329	416194	84.99%	10.295%
18	10.214	2839	2853	2875	rBV	74325	122327	24.98%	3.026%
19	11.246	3164	3174	3197	rBV	229999	363818	74.29%	9.000%
20	11.532	3252	3263	3280	rBV2	18006	32508	6.64%	0.804%
21	11.622	3280	3291	3310	rVV	202610	319203	65.18%	7.896%




Sum of corrected areas: 4042523

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090622\
Data File : VV027759.D
Acq On : 06 Sep 2022 22:31
Operator : SY/MD
Sample : N4402-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVF7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

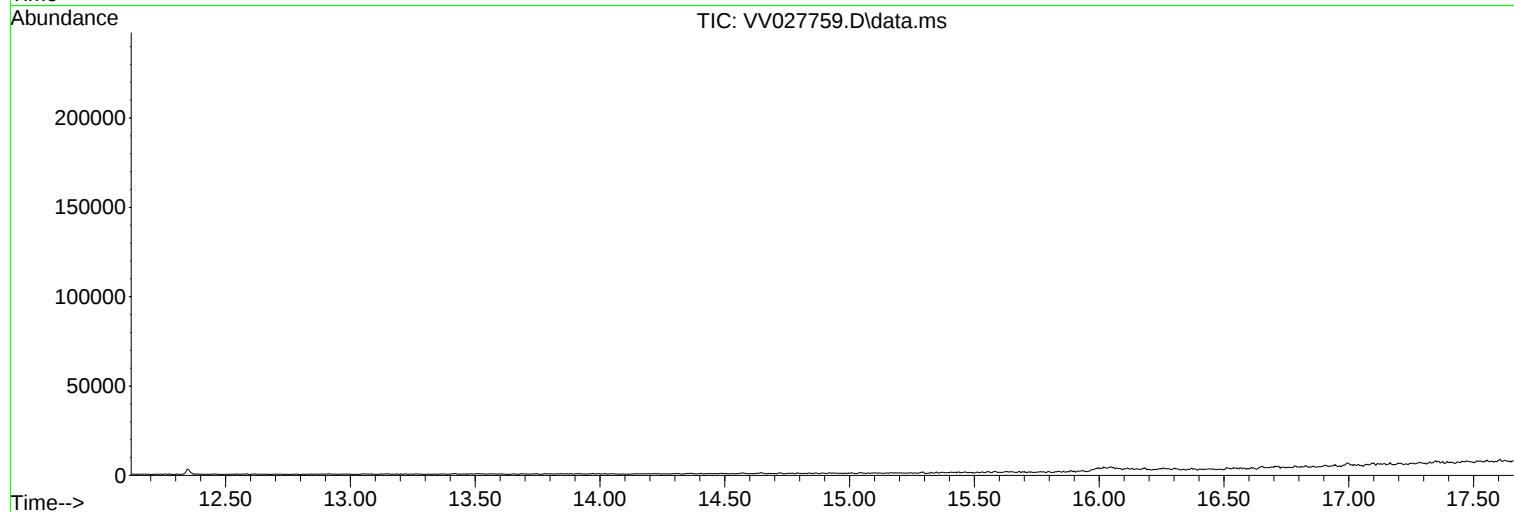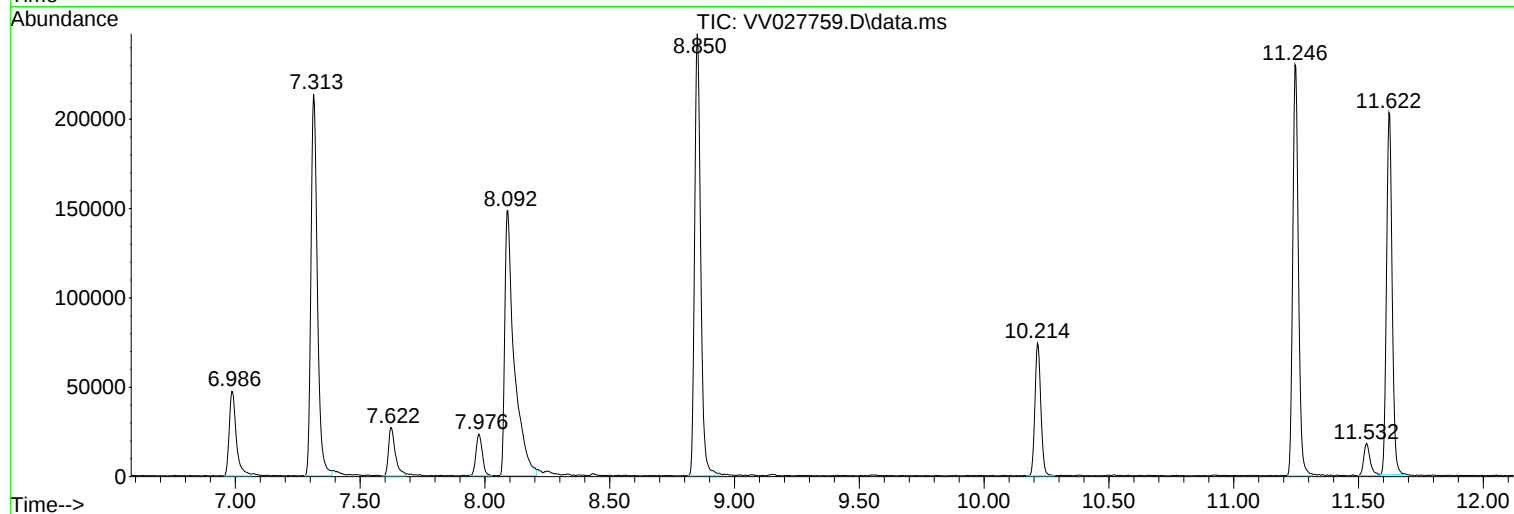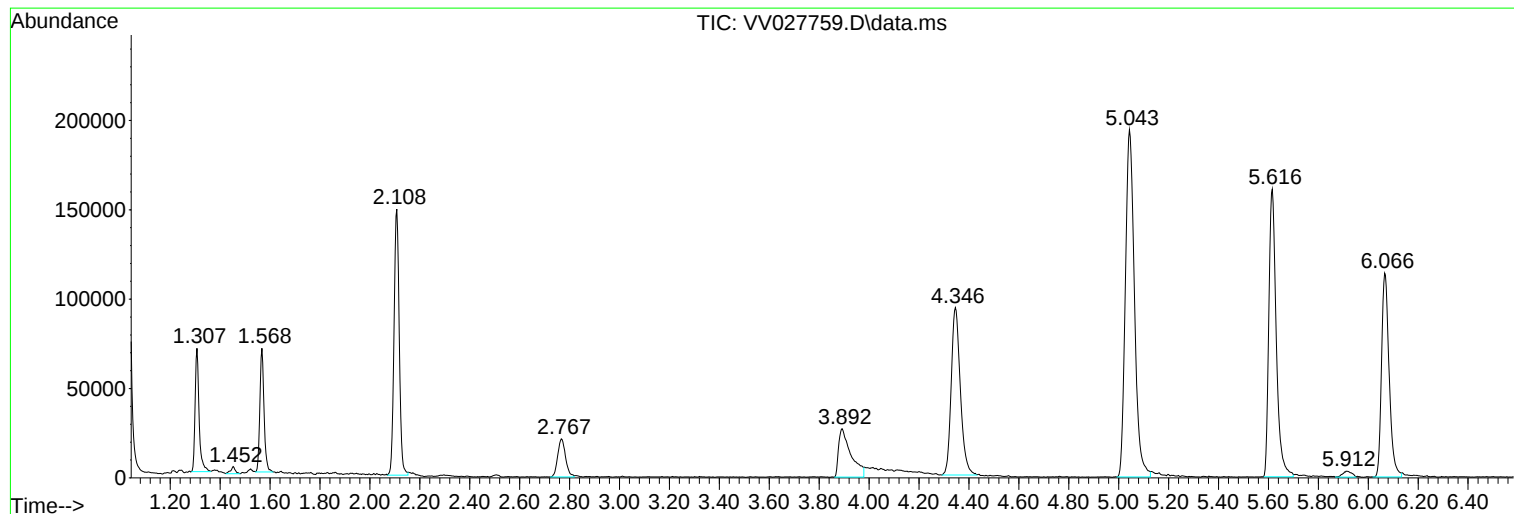

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090622\
Data File : VV027759.D
Acq On : 06 Sep 2022 22:31
Operator : SY/MD
Sample : N4402-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVF7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090622\
Data File : VV027759.D
Acq On : 06 Sep 2022 22:31
Operator : SY/MD
Sample : N4402-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVF7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------