

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090622\
 Data File : VV027761.D
 Acq On : 06 Sep 2022 23:20
 Operator : SY/MD
 Sample : N4402-12DL 4X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBVB5DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV027761.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	99	rBV	74572	82178	16.69%	1.759%
2	1.417	111	117	126	rVB	10673	12017	2.44%	0.257%
3	1.568	155	164	182	rBV	68747	83083	16.87%	1.779%
4	2.108	321	332	344	rBV	144915	209338	42.52%	4.482%
5	2.507	447	456	467	rBV2	5721	9238	1.88%	0.198%
6	3.908	872	892	917	rBV4	66895	239990	48.74%	5.138%
7	4.346	1011	1028	1056	rVB2	93618	232935	47.31%	4.987%
8	5.043	1225	1245	1273	rBV2	193064	492380	100.00%	10.542%
9	5.616	1411	1423	1452	rBV	159938	333118	67.65%	7.132%
10	5.912	1502	1515	1542	rBV	150959	309025	62.76%	6.616%
11	6.066	1550	1563	1596	rVB2	112711	233779	47.48%	5.005%
12	6.986	1839	1849	1867	rBV	44762	87093	17.69%	1.865%
13	7.313	1940	1951	1975	rBV	208910	376106	76.39%	8.053%
14	7.622	2036	2047	2068	rBV2	26272	51752	10.51%	1.108%
15	7.976	2145	2157	2171	rBV	153384	262263	53.26%	5.615%
16	8.092	2183	2193	2229	rBV2	171206	425946	86.51%	9.120%
17	8.850	2417	2429	2451	rBV	260587	429457	87.22%	9.195%
18	10.214	2843	2853	2868	rBV2	77593	124221	25.23%	2.660%
19	11.246	3164	3174	3193	rBV	225182	355224	72.14%	7.606%
20	11.535	3255	3264	3277	rBV2	6804	12366	2.51%	0.265%
21	11.622	3280	3291	3312	rVV	195426	309048	62.77%	6.617%




Sum of corrected areas: 4670557

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090622\
Data File : VV027761.D
Acq On : 06 Sep 2022 23:20
Operator : SY/MD
Sample : N4402-12DL 4X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVB5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

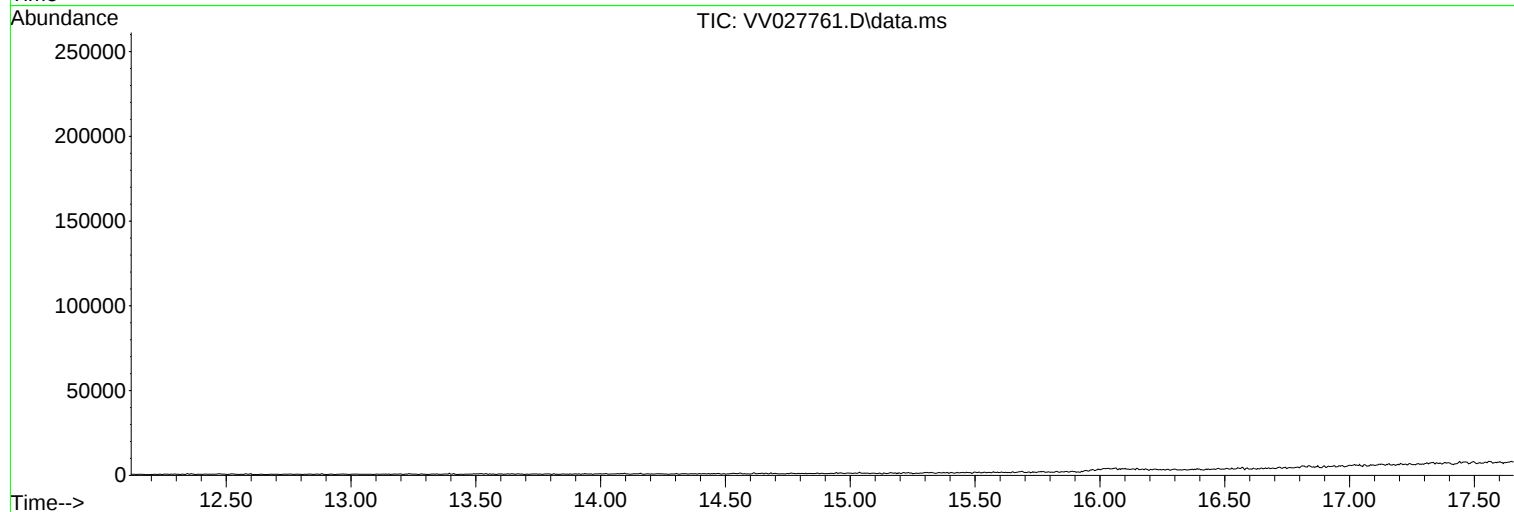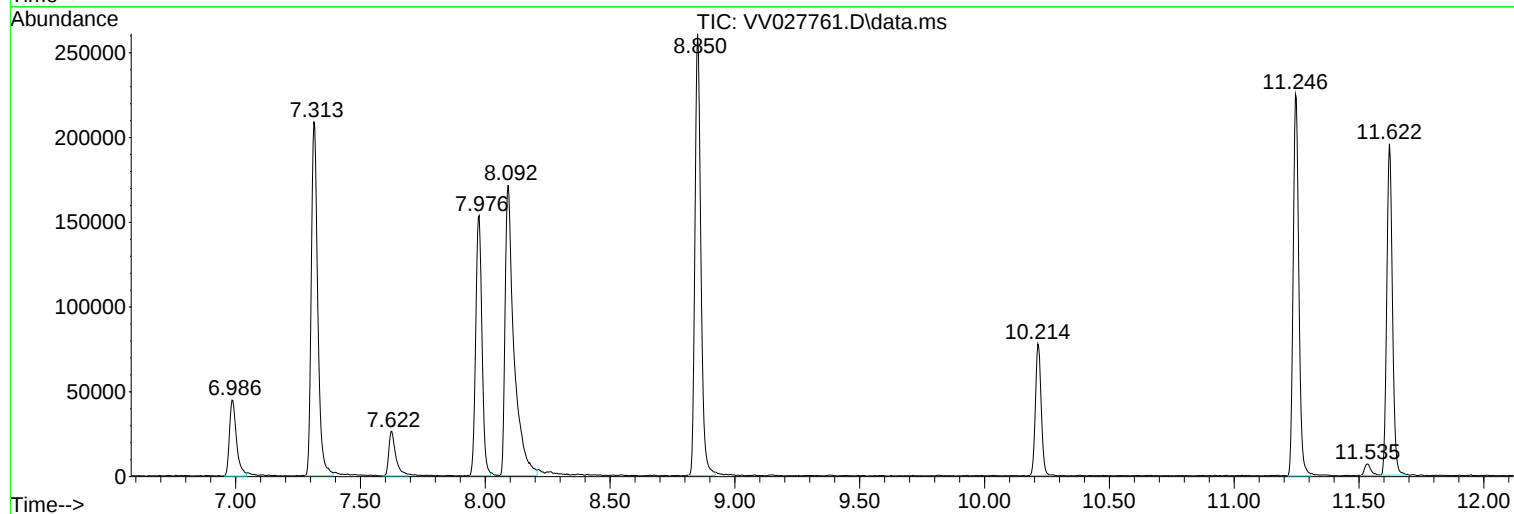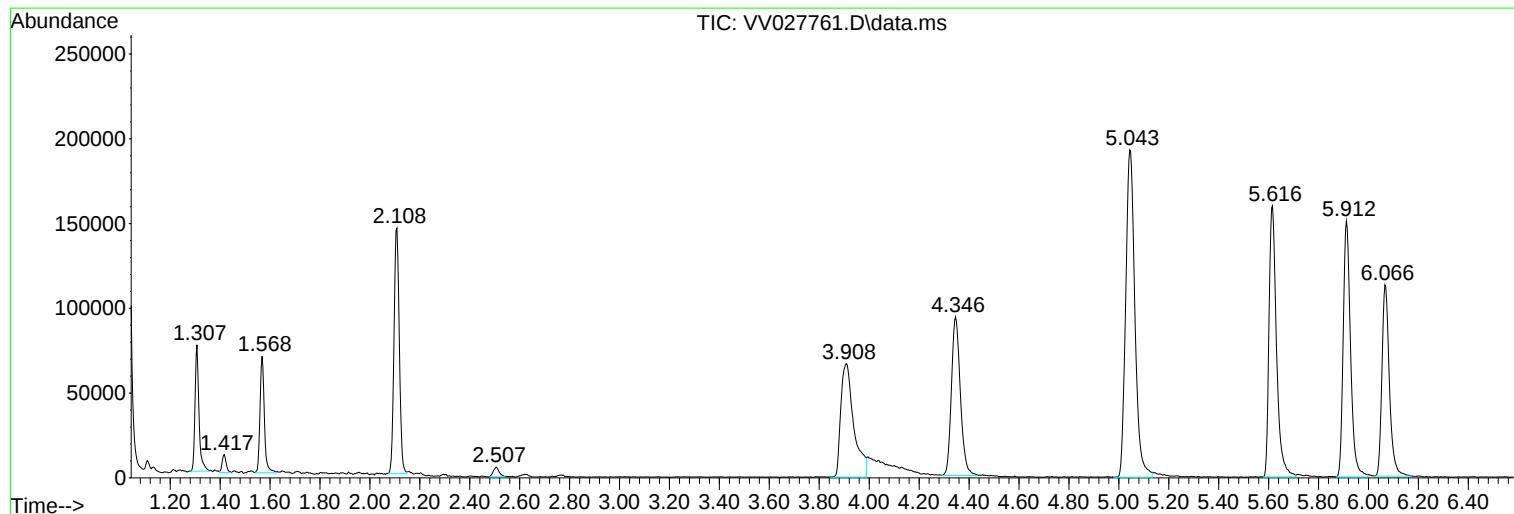

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090622\
Data File : VV027761.D
Acq On : 06 Sep 2022 23:20
Operator : SY/MD
Sample : N4402-12DL 4X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVB5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090622\
Data File : VV027761.D
Acq On : 06 Sep 2022 23:20
Operator : SY/MD
Sample : N4402-12DL 4X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVB5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc