

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090622\
 Data File : VV027762.D
 Acq On : 06 Sep 2022 23:44
 Operator : SY/MD
 Sample : N4402-14DL 10X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBVD3DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV027762.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	103	rVB	73504	84863	16.71%	1.817%
2	1.417	107	117	126	rBV	11288	14003	2.76%	0.300%
3	1.568	156	164	175	rBV	70211	82864	16.32%	1.774%
4	2.105	320	331	348	rBV	149294	219279	43.18%	4.695%
5	2.503	447	455	467	rVB3	6149	10085	1.99%	0.216%
6	3.902	870	890	919	rBV4	54112	211213	41.60%	4.522%
7	4.346	1012	1028	1050	rBV2	93534	235430	46.36%	5.040%
8	5.044	1230	1245	1273	rBV2	199408	505028	99.46%	10.812%
9	5.613	1411	1422	1456	rBV	159730	337560	66.48%	7.227%
10	5.915	1506	1516	1538	rVB8	9485	22834	4.50%	0.489%
11	6.066	1551	1563	1585	rBV	115829	242770	47.81%	5.198%
12	6.986	1838	1849	1871	rBV	47467	92221	18.16%	1.974%
13	7.314	1940	1951	1979	rBV	220293	397634	78.31%	8.513%
14	7.625	2037	2048	2063	rBV2	27275	51498	10.14%	1.103%
15	7.973	2140	2156	2176	rBV	301372	507781	100.00%	10.871%
16	8.092	2182	2193	2239	rBV	165515	424973	83.69%	9.098%
17	8.850	2417	2429	2451	rBV	250490	418276	82.37%	8.955%
18	10.214	2843	2853	2868	rBV	79493	126729	24.96%	2.713%
19	11.246	3163	3174	3198	rBV	230188	363793	71.64%	7.789%
20	11.622	3280	3291	3317	rBV	199448	322052	63.42%	6.895%




Sum of corrected areas: 4670886

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090622\
Data File : VV027762.D
Acq On : 06 Sep 2022 23:44
Operator : SY/MD
Sample : N4402-14DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVD3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

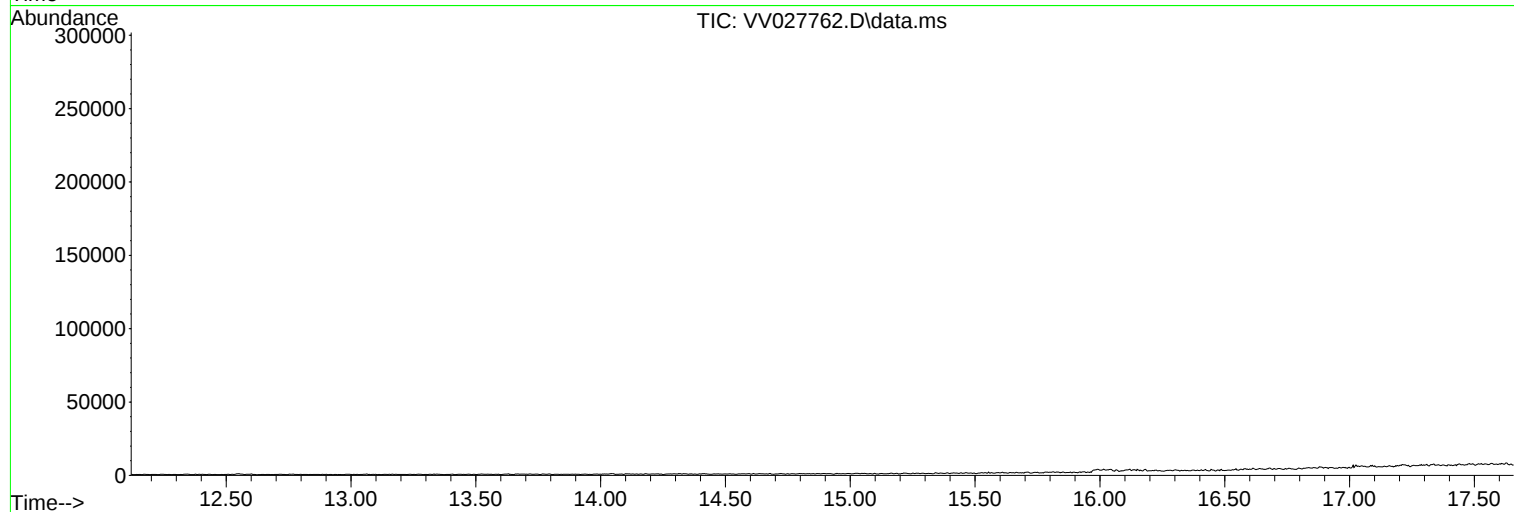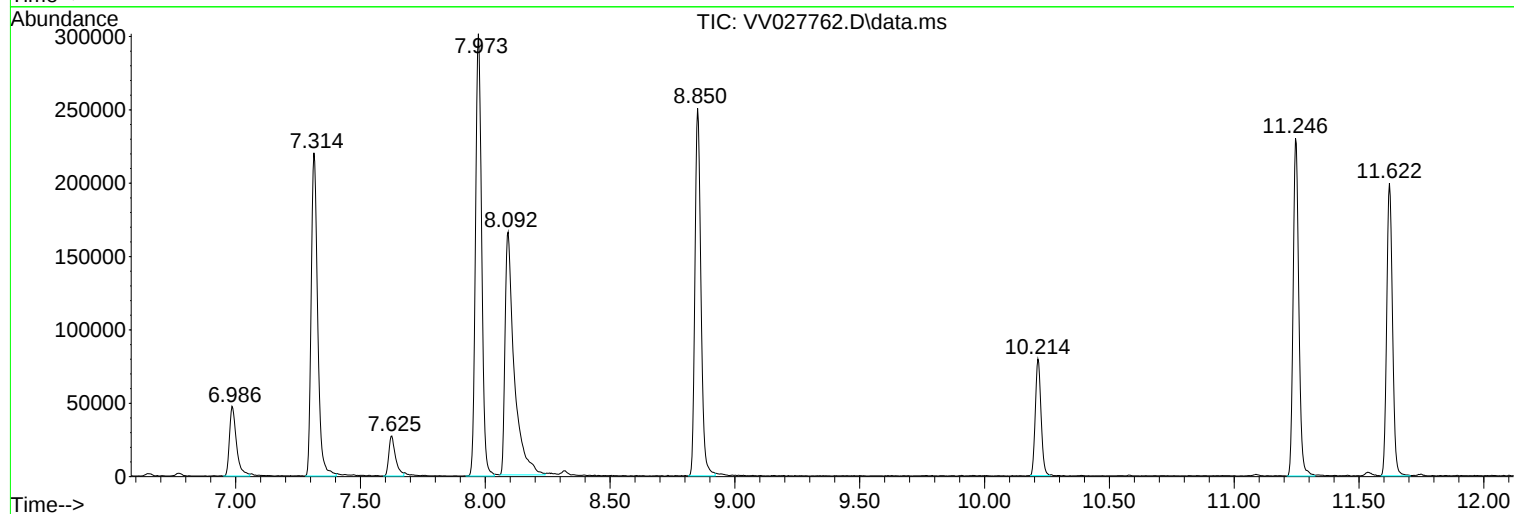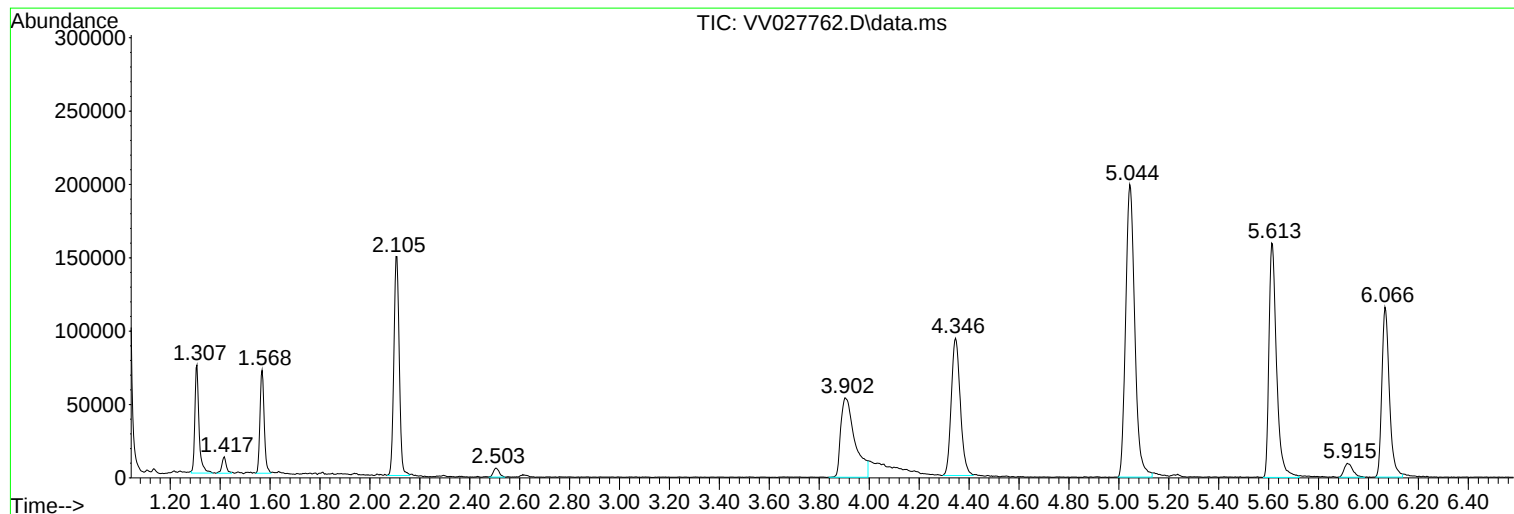

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090622\
Data File : VV027762.D
Acq On : 06 Sep 2022 23:44
Operator : SY/MD
Sample : N4402-14DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVD3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090622\
Data File : VV027762.D
Acq On : 06 Sep 2022 23:44
Operator : SY/MD
Sample : N4402-14DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVD3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc