

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090622\
 Data File : VV027764.D
 Acq On : 07 Sep 2022 00:33
 Operator : SY/MD
 Sample : N4402-16DL 10X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBVE8DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV027764.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	72	83	100	rBV	74013	81262	16.64%	1.847%
2	1.417	108	117	124	rVB	7243	8757	1.79%	0.199%
3	1.568	156	164	179	rVB	70099	82693	16.94%	1.879%
4	2.108	321	332	347	rBV	142975	206847	42.36%	4.701%
5	2.507	445	456	467	rVB2	6077	10073	2.06%	0.229%
6	3.902	874	890	912	rBV2	38058	141623	29.00%	3.219%
7	4.346	1011	1028	1054	rVB	92047	230398	47.18%	5.236%
8	5.047	1228	1246	1275	rBV2	193651	488296	100.00%	11.098%
9	5.616	1410	1423	1458	rBV	161253	334972	68.60%	7.613%
10	6.066	1550	1563	1595	rBV2	110589	236413	48.42%	5.373%
11	6.985	1837	1849	1873	rBV	45242	89371	18.30%	2.031%
12	7.313	1940	1951	1974	rBV	213545	382328	78.30%	8.689%
13	7.625	2039	2048	2064	rBV	26511	49504	10.14%	1.125%
14	7.973	2144	2156	2179	rBV	267017	448492	91.85%	10.193%
15	8.091	2183	2193	2235	rBV2	155279	396448	81.19%	9.010%
16	8.850	2418	2429	2453	rBV	252503	419900	85.99%	9.543%
17	10.214	2843	2853	2872	rBV	77173	123447	25.28%	2.806%
18	11.249	3164	3175	3198	rBV	229455	361950	74.13%	8.226%
19	11.622	3279	3291	3306	rBV	193879	307142	62.90%	6.981%




Sum of corrected areas: 4399916

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090622\
Data File : VV027764.D
Acq On : 07 Sep 2022 00:33
Operator : SY/MD
Sample : N4402-16DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVE8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

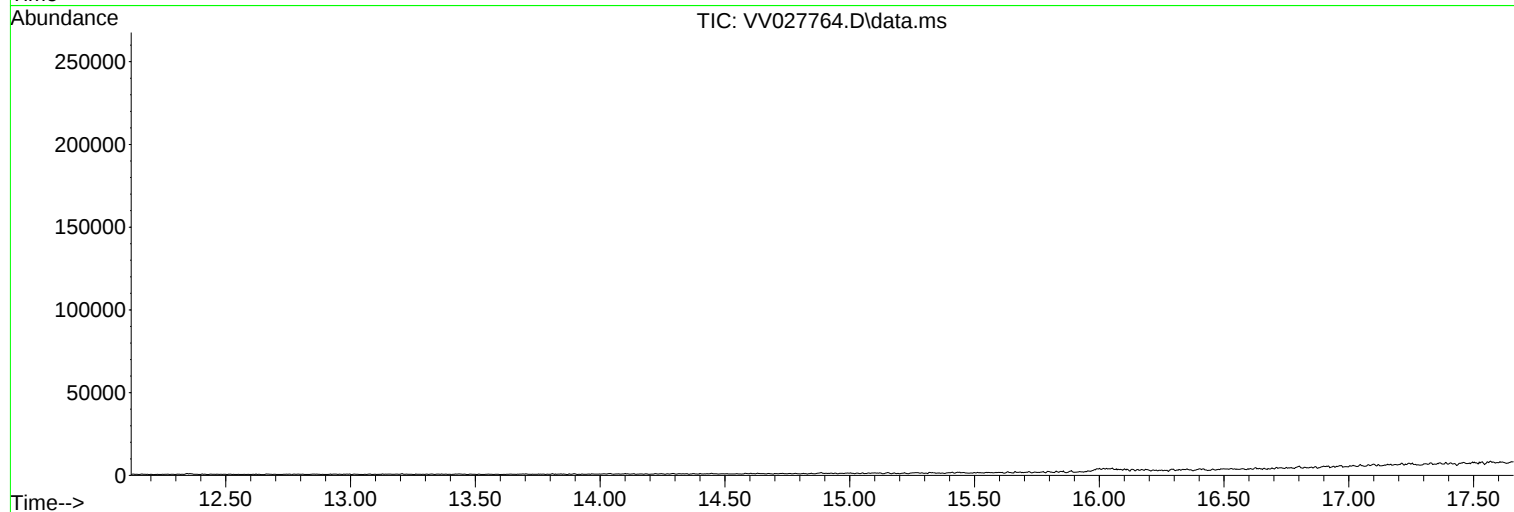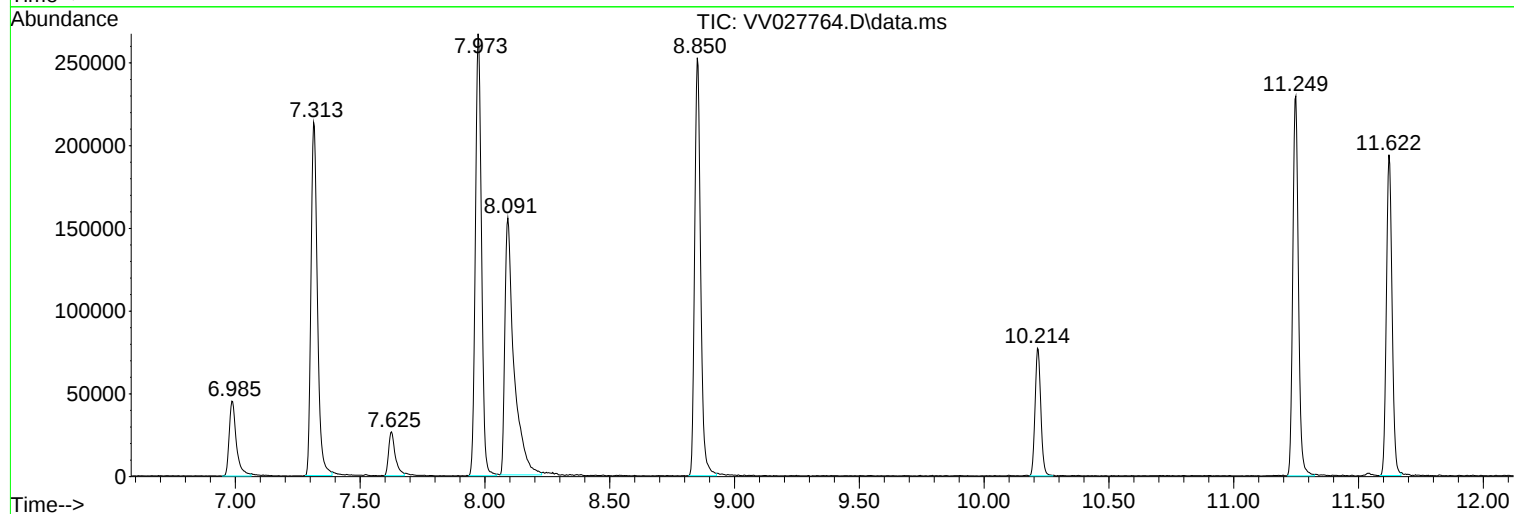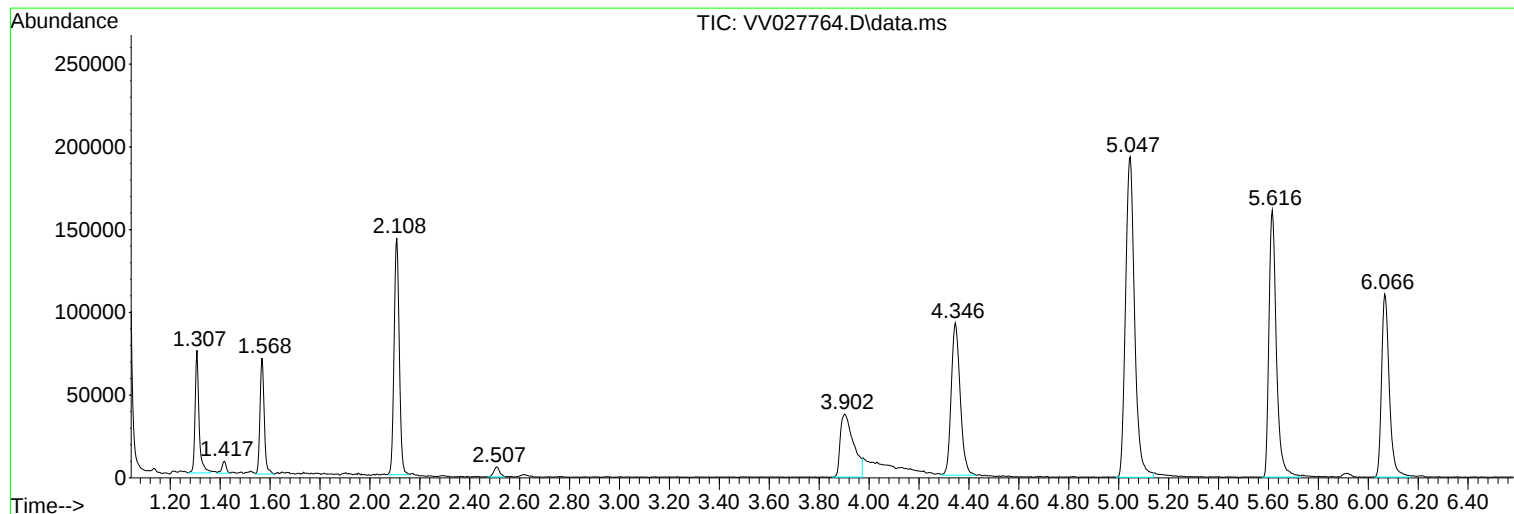

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090622\
Data File : VV027764.D
Acq On : 07 Sep 2022 00:33
Operator : SY/MD
Sample : N4402-16DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVE8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090622\
Data File : VV027764.D
Acq On : 07 Sep 2022 00:33
Operator : SY/MD
Sample : N4402-16DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVE8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc