

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090622\
 Data File : VV027766.D
 Acq On : 07 Sep 2022 01:22
 Operator : SY/MD
 Sample : N4402-21
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBVF9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027766.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	73	83	97	rBV	67316	77509	15.67%	1.957%
2	1.568	156	164	175	rBV	67914	77670	15.70%	1.961%
3	2.108	320	332	353	rVB	145807	209981	42.45%	5.301%
4	2.770	525	538	554	rBV3	13287	29367	5.94%	0.741%
5	3.902	880	890	918	rBV	23938	91226	18.44%	2.303%
6	4.346	1012	1028	1053	rVB2	93028	244929	49.51%	6.184%
7	5.043	1230	1245	1273	rBV2	196997	494701	100.00%	12.490%
8	5.616	1409	1423	1458	rBV	161018	332627	67.24%	8.398%
9	6.066	1551	1563	1591	rBV	109914	234293	47.36%	5.915%
10	6.989	1838	1850	1871	rBV	43132	86109	17.41%	2.174%
11	7.313	1939	1951	1971	rBV	208394	373156	75.43%	9.421%
12	7.625	2039	2048	2067	rBV2	27267	51183	10.35%	1.292%
13	7.976	2148	2157	2172	rBV3	14216	25370	5.13%	0.641%
14	8.091	2183	2193	2232	rBV3	149201	396417	80.13%	10.008%
15	8.850	2418	2429	2457	rBV	248105	414171	83.72%	10.456%
16	10.217	2840	2854	2878	rBV	74809	121606	24.58%	3.070%
17	11.249	3162	3175	3191	rBV	228834	358080	72.38%	9.040%
18	11.532	3252	3263	3279	rBV3	17736	30090	6.08%	0.760%
19	11.622	3279	3291	3309	rVV	199015	312417	63.15%	7.888%




Sum of corrected areas: 3960902

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090622\
Data File : VV027766.D
Acq On : 07 Sep 2022 01:22
Operator : SY/MD
Sample : N4402-21
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVF9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

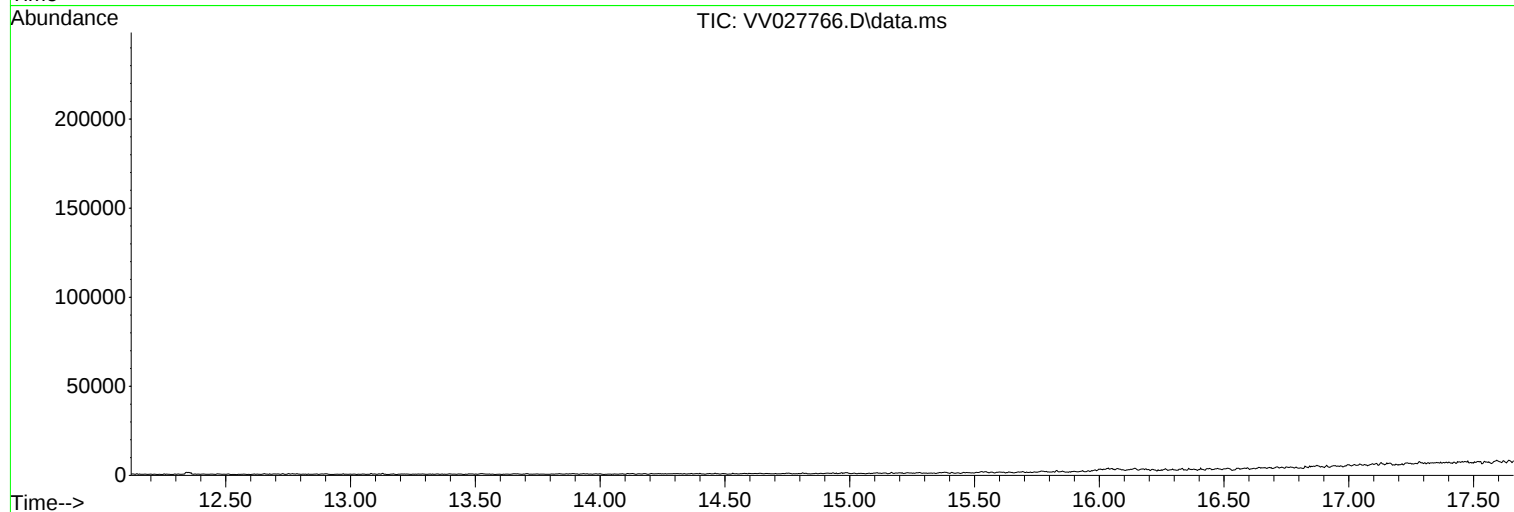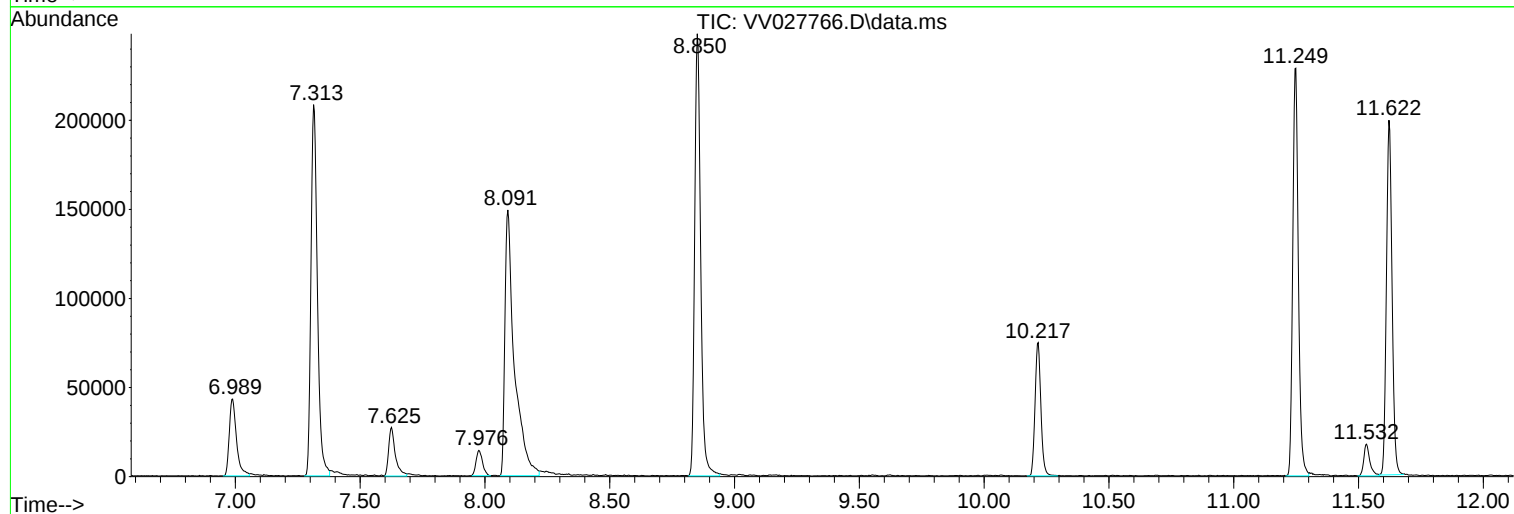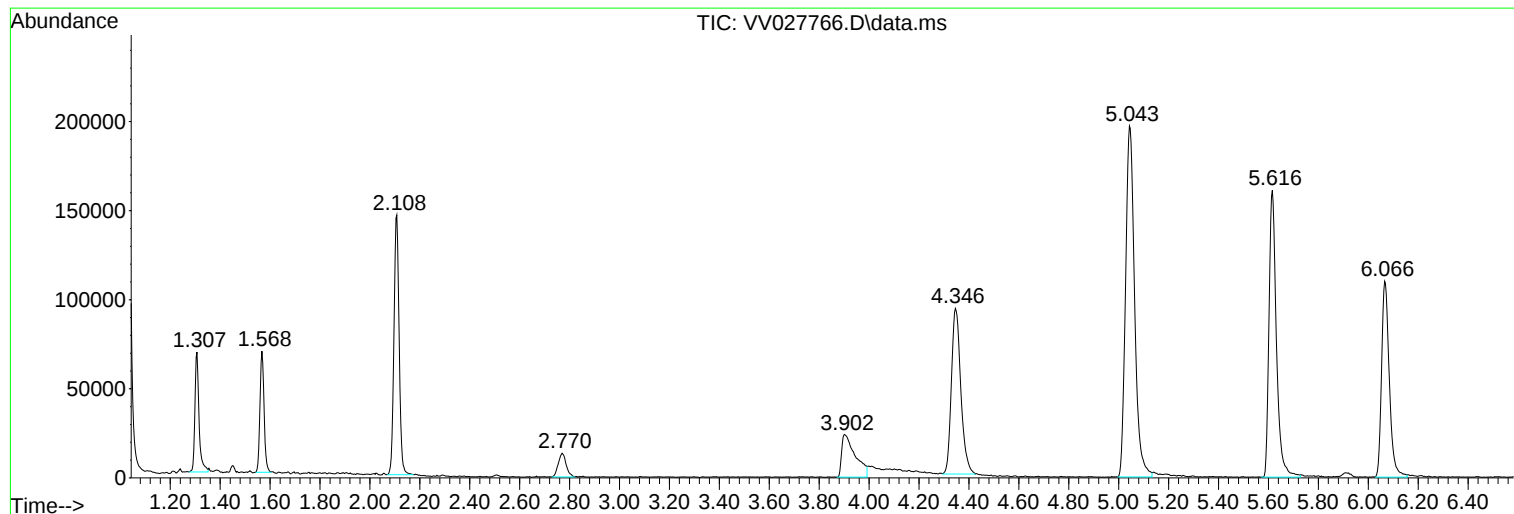

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090622\
Data File : VV027766.D
Acq On : 07 Sep 2022 01:22
Operator : SY/MD
Sample : N4402-21
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVF9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090622\
Data File : VV027766.D
Acq On : 07 Sep 2022 01:22
Operator : SY/MD
Sample : N4402-21
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVF9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc