
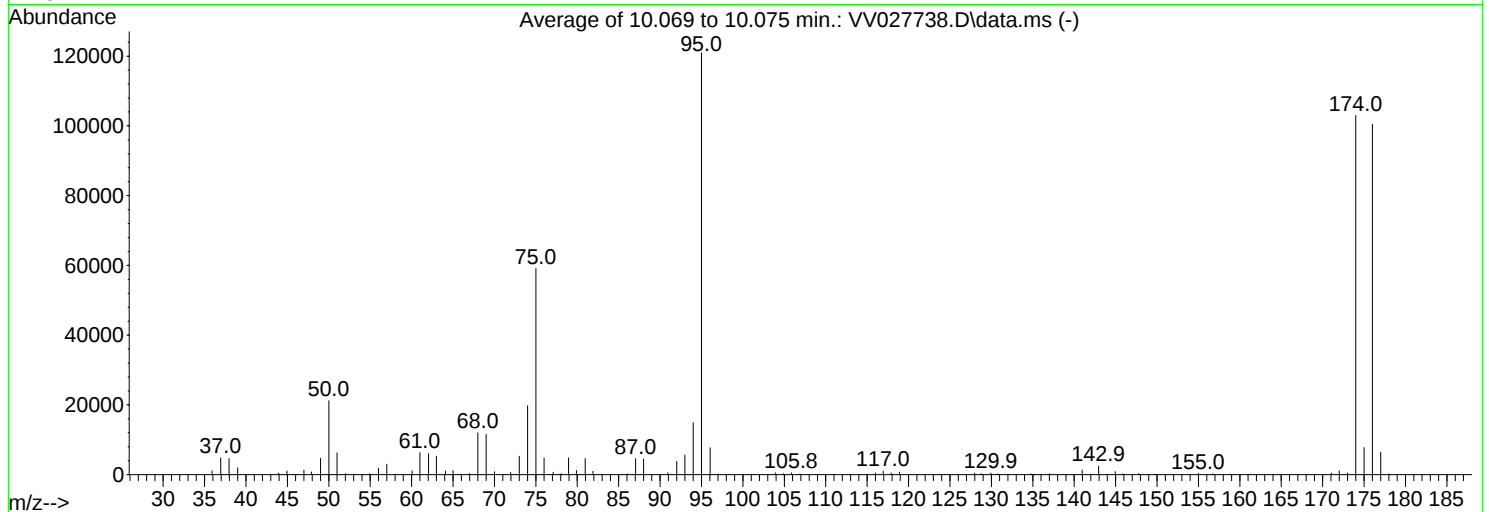


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090622\
Data File : VV027738.D
Acq On : 06 Sep 2022 10:13
Operator : SY/MD
Sample : BFB367
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB367

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed Sep 07 06:13:02 2022

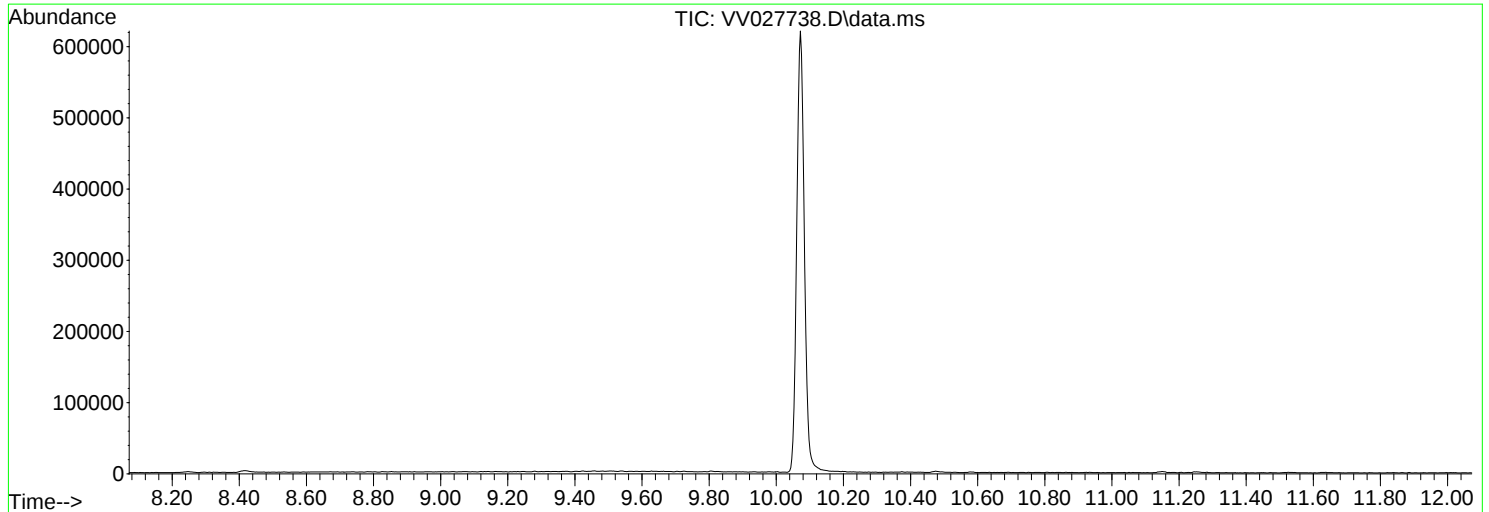

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	21221	PASS
75	95	30	80	48.9	59128	PASS
95	95	100	100	100.0	120949	PASS
96	95	5	9	6.4	7731	PASS
173	174	0.00	2	0.4	450	PASS
174	95	50	120	85.2	103003	PASS
175	174	5	9	7.5	7751	PASS
176	174	95	105	97.6	100488	PASS
177	176	5	10	6.4	6445	PASS

m/z	Abundance
35.90	1303.0
36.90	146.0
37.90	512.0
39.90	328.0
44.00	202.0

Instrument :
MSVOA_V
ClientSampleId :
BFB367

m/z	Abundance
36.00	2422.0
37.00	5145.0
38.00	5438.0
39.00	1990.0
39.90	420.0
42.90	103.0
44.10	624.0
45.00	1083.0
47.00	1228.0
47.90	712.0
49.00	4741.0
50.00	21264.0
51.00	6334.0
52.00	350.0
53.00	184.0
54.10	142.0
54.90	292.0
56.00	1784.0
57.00	2895.0
58.10	148.0
60.00	1123.0
61.00	6265.0
62.00	6011.0
63.00	5309.0
64.10	1134.0
65.00	1117.0
66.00	135.0
67.00	313.0
68.00	11985.0
69.00	11121.0
70.00	827.0
71.20	116.0
71.90	525.0
73.00	5127.0
74.00	19608.0
75.00	59144.0
76.00	4960.0
77.20	553.0
77.80	462.0
79.00	4846.0
79.90	1183.0
81.00	4380.0
81.90	778.0
86.00	243.0
87.10	4467.0
88.00	4481.0
91.00	531.0
92.00	3583.0
93.00	5314.0
94.00	14872.0
95.00	119696.0
96.00	7620.0
97.00	188.0
103.00	101.0
104.00	506.0
104.90	249.0
105.80	496.0
106.90	167.0
111.00	134.0
112.80	131.0
115.10	159.0
116.00	526.0
116.90	1013.0
117.90	476.0
118.90	849.0
128.00	405.0
128.70	236.0
130.00	494.0
130.70	215.0
134.80	220.0
137.00	267.0
141.00	1324.0
142.00	180.0
143.00	2310.0
144.10	175.0
145.00	882.0
145.80	202.0
147.80	289.0
149.70	119.0
151.90	113.0
155.00	328.0
156.70	221.0
158.90	154.0
160.80	141.0
171.00	480.0
172.00	904.0
173.00	1349.0
174.00	100656.0
175.00	7780.0
176.00	97872.0
177.00	6258.0
178.00	287.0

Instrument :
MSVOA_V
ClientSampleId :
BFB367

m/z	Abundance
36.00	2443.0
37.00	5165.0
38.00	5264.0
39.00	2074.0
40.00	343.0
42.90	106.0
43.90	662.0
44.90	1071.0
45.80	162.0
46.20	169.0
47.00	1318.0
47.90	829.0
49.00	4822.0
50.00	21896.0
51.00	6469.0
52.00	356.0
53.00	169.0
54.20	107.0
54.90	278.0
56.00	1918.0
57.00	3090.0
58.10	155.0
60.10	1143.0
61.00	6574.0
62.00	6112.0
63.00	5477.0
64.10	1055.0
65.00	1201.0
66.00	139.0
67.00	347.0
68.00	12385.0
69.00	11928.0
70.00	850.0
71.20	122.0
72.00	690.0
73.00	5480.0
74.00	20432.0
75.00	60880.0
76.00	4928.0
77.10	674.0
78.00	438.0
79.00	5047.0
79.90	1192.0
80.90	4788.0
81.90	984.0
82.90	119.0
85.50	104.0
86.10	247.0
87.00	4747.0
88.00	4621.0
90.90	566.0
92.00	3981.0
93.00	5811.0
94.00	15517.0
95.00	125560.0
96.10	8018.0
97.10	175.0
103.90	550.0
104.90	279.0
105.90	524.0
106.90	181.0
111.00	135.0
112.90	117.0
115.00	148.0
116.00	571.0
117.00	1044.0
117.90	464.0
119.00	773.0
123.80	129.0
128.00	406.0
128.80	281.0
129.90	479.0
130.80	208.0
134.80	234.0
135.20	167.0
137.00	272.0
140.90	1375.0
142.00	171.0
142.90	2552.0
144.10	156.0
145.00	889.0
145.80	226.0
147.80	321.0
149.00	105.0
149.80	133.0
151.90	128.0
152.90	112.0
155.00	357.0
156.70	233.0
158.90	167.0
160.80	111.0
171.00	489.0

Instrument :
MSVOA_V
ClientSampleId :
BFB367

172.00	1092.0
174.00	106312.0
175.00	8057.0
176.00	103960.0
177.00	6648.0
178.00	269.0

Instrument :
MSVOA_V
ClientSampleId :
BFB367

m/z	Abundance
36.00	2317.0
37.00	4528.0
38.00	4702.0
39.00	1924.0
40.10	306.0
43.90	723.0
44.90	946.0
45.80	174.0
46.10	165.0
47.00	1261.0
47.90	869.0
49.00	4426.0
50.00	20504.0
51.00	5950.0
52.10	330.0
53.10	144.0
54.90	258.0
56.00	1865.0
57.00	2939.0
58.00	171.0
60.10	1088.0
61.00	6166.0
62.10	5873.0
63.00	5106.0
64.10	902.0
65.00	1067.0
66.10	132.0
67.00	332.0
68.00	11551.0
69.00	11472.0
70.00	755.0
71.00	105.0
72.00	758.0
73.00	5215.0
74.00	19224.0
75.00	57360.0
76.00	4391.0
77.00	786.0
78.10	453.0
78.90	4523.0
79.90	1154.0
80.90	4706.0
81.90	1099.0
82.90	116.0
86.10	233.0
87.00	4623.0
88.00	4381.0
90.90	551.0
92.00	3876.0
93.00	5708.0
94.00	14441.0
95.00	117592.0
96.10	7554.0
97.10	181.0
103.90	526.0
104.90	260.0
105.90	569.0
106.90	169.0
110.90	112.0
112.90	100.0
115.00	132.0
116.00	492.0
116.90	976.0
117.90	432.0
118.80	651.0
123.70	129.0
127.80	411.0
128.80	315.0
129.90	450.0
130.90	228.0
134.80	243.0
135.20	198.0
137.10	250.0
140.90	1279.0
141.90	149.0
142.90	2374.0
143.90	151.0
144.90	848.0
145.80	252.0
147.80	294.0
149.80	143.0
151.90	117.0
153.00	111.0
155.00	346.0
156.80	253.0
158.90	169.0
160.90	102.0
171.10	391.0
172.00	1218.0
174.00	102040.0
175.00	7417.0
176.00	99632.0

Instrument :
MSVOA_V
ClientSampleId :
BFB367

177.006430.0

178.00199.0

Instrument :
MSVOA_V
ClientSampleId :
BFB367