

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090718\
 Data File : VV007457.D
 Acq On : 07 Sep 2018 13:33
 Operator : SY/MD
 Sample : J4719-03 25X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGD9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.322	65	72	91	rVB	281935	346966	11.39%	1.630%
2	1.560	141	146	163	rVB	232925	289001	9.49%	1.358%
3	2.129	312	323	335	rBV	538600	765668	25.13%	3.598%
4	2.534	444	449	461	rVB	12572	17735	0.58%	0.083%
5	3.428	722	727	729	rBV2	601	576	0.02%	0.003%
6	3.550	762	765	769	rBV3	348	286	0.01%	0.001%
7	3.598	778	780	788	rVB4	780	685	0.02%	0.003%
8	3.672	801	803	807	rVB2	394	292	0.01%	0.001%
9	3.749	821	827	829	rBV3	378	462	0.02%	0.002%
10	3.811	843	846	849	rBV2	363	232	0.01%	0.001%
11	3.955	870	891	931	rBV3	148710	513031	16.84%	2.411%
12	4.319	1002	1004	1007	rBV2	365	245	0.01%	0.001%
13	4.402	1011	1030	1064	rBV	401625	970845	31.87%	4.562%
14	4.656	1105	1109	1112	rBV3	533	430	0.01%	0.002%
15	4.701	1121	1123	1125	rBV	712	426	0.01%	0.002%
16	4.720	1125	1129	1130	rBV2	688	465	0.02%	0.002%
17	4.811	1154	1157	1160	rVV2	414	322	0.01%	0.002%
18	4.830	1160	1163	1167	rVB	317	264	0.01%	0.001%
19	4.891	1179	1182	1185	rBV	288	220	0.01%	0.001%
20	4.907	1185	1187	1191	rVB2	365	261	0.01%	0.001%
21	4.929	1191	1194	1199	rVB3	301	241	0.01%	0.001%
22	5.097	1226	1246	1283	rBV2	1025120	2459924	80.75%	11.559%
23	5.347	1321	1324	1329	rVB2	576	380	0.01%	0.002%
24	5.521	1374	1378	1382	rVB4	556	549	0.02%	0.003%
25	5.547	1382	1386	1389	rBV3	423	360	0.01%	0.002%
26	5.666	1404	1423	1456	rBV	782468	1560381	51.22%	7.332%
27	5.901	1493	1496	1499	rBV2	669	471	0.02%	0.002%
28	5.958	1500	1514	1534	rVB4	47213	104623	3.43%	0.492%
29	6.032	1534	1537	1541	rBV4	857	733	0.02%	0.003%
30	6.122	1546	1565	1589	rBV	564048	1141670	37.48%	5.365%
31	6.450	1663	1667	1670	rVV4	382	282	0.01%	0.001%
32	6.650	1723	1729	1734	rBV3	779	939	0.03%	0.004%
33	6.672	1734	1736	1738	rBV	401	250	0.01%	0.001%
34	6.714	1743	1749	1755	rBV6	1969	3089	0.10%	0.015%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090718\
 Data File : VV007457.D
 Acq On : 07 Sep 2018 13:33
 Operator : SY/MD
 Sample : J4719-03 25X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGD9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

35	6.762	1762	1764	1770	rVB3	727	564	0.02%	0.003%
36	6.791	1770	1773	1777	rVB3	821	511	0.02%	0.002%
37	6.926	1811	1815	1817	rVB3	482	274	0.01%	0.001%
38	7.032	1834	1848	1876	rBV	279262	492808	16.18%	2.316%
39	7.164	1886	1889	1893	rBV2	640	416	0.01%	0.002%
40	7.187	1894	1896	1903	rVB5	981	846	0.03%	0.004%
41	7.273	1919	1923	1924	rBV	596	304	0.01%	0.001%
42	7.286	1924	1927	1930	rVB4	672	456	0.01%	0.002%
43	7.360	1935	1950	1988	rBV	1074239	1875674	61.57%	8.814%
44	7.576	2014	2017	2019	rVB2	663	369	0.01%	0.002%
45	7.666	2032	2045	2074	rBV	204753	348109	11.43%	1.636%
46	7.830	2092	2096	2098	rBV4	716	515	0.02%	0.002%
47	8.019	2141	2155	2180	rBV	1832266	3046367	100.00%	14.315%
48	8.138	2181	2192	2224	rBV2	537835	1084892	35.61%	5.098%
49	8.482	2294	2299	2302	rBV5	837	703	0.02%	0.003%
50	8.630	2341	2345	2349	rBV4	415	371	0.01%	0.002%
51	8.675	2354	2359	2363	rVB4	512	409	0.01%	0.002%
52	8.801	2393	2398	2403	rBV4	675	879	0.03%	0.004%
53	8.839	2406	2410	2412	rBV4	497	335	0.01%	0.002%
54	8.897	2412	2428	2450	rBV	1176939	1926760	63.25%	9.054%
55	9.177	2509	2515	2516	rBV3	890	648	0.02%	0.003%
56	9.286	2544	2549	2555	rVV3	396	467	0.02%	0.002%
57	9.527	2620	2624	2631	rBV6	500	664	0.02%	0.003%
58	9.556	2631	2633	2637	rVV2	449	299	0.01%	0.001%
59	9.579	2637	2640	2643	rVV	334	317	0.01%	0.001%
60	9.605	2646	2648	2657	rVB3	1027	1209	0.04%	0.006%
61	9.691	2672	2675	2679	rVB2	420	338	0.01%	0.002%
62	9.939	2749	2752	2755	rVB2	458	263	0.01%	0.001%
63	9.974	2759	2763	2766	rBV2	383	341	0.01%	0.002%
64	10.016	2774	2776	2779	rVB2	439	245	0.01%	0.001%
65	10.039	2779	2783	2786	rBV	441	350	0.01%	0.002%
66	10.093	2798	2800	2804	rVB2	427	224	0.01%	0.001%
67	10.183	2825	2828	2833	rVB3	304	264	0.01%	0.001%
68	10.267	2838	2854	2885	rBV	735614	1213175	39.82%	5.701%
69	10.421	2900	2902	2907	rVB2	458	285	0.01%	0.001%
70	10.466	2912	2916	2920	rBV	324	325	0.01%	0.002%
71	10.543	2936	2940	2943	rBV3	458	406	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090718\
 Data File : VV007457.D
 Acq On : 07 Sep 2018 13:33
 Operator : SY/MD
 Sample : J4719-03 25X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGD9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

72	10.572	2947	2949	2957	rVB3	427	523	0.02%	0.002%
73	10.675	2976	2981	2984	rBV2	348	262	0.01%	0.001%
74	10.707	2987	2991	2996	rVB2	240	242	0.01%	0.001%
75	10.740	2998	3001	3006	rVB3	529	450	0.01%	0.002%
76	10.781	3006	3014	3023	rBV4	612	1107	0.04%	0.005%
77	10.833	3028	3030	3035	rVB2	315	291	0.01%	0.001%
78	10.865	3035	3040	3043	rBV	535	525	0.02%	0.002%
79	11.026	3087	3090	3092	rBV4	452	266	0.01%	0.001%
80	11.100	3109	3113	3117	rBV3	364	458	0.02%	0.002%
81	11.228	3149	3153	3163	rVB4	1158	1634	0.05%	0.008%
82	11.299	3163	3175	3203	rBV	879300	1513888	49.69%	7.114%
83	11.505	3235	3239	3241	rBV4	420	309	0.01%	0.001%
84	11.678	3279	3293	3327	rBV	895445	1570617	51.56%	7.380%
85	12.048	3405	3408	3409	rBV2	453	227	0.01%	0.001%
86	12.151	3437	3440	3444	rBV3	408	334	0.01%	0.002%
87	12.193	3450	3453	3456	rBV2	486	356	0.01%	0.002%
88	12.241	3466	3468	3474	rVB2	528	319	0.01%	0.001%
89	12.395	3514	3516	3522	rVB3	629	319	0.01%	0.001%
90	12.440	3528	3530	3533	rBV	373	227	0.01%	0.001%
91	12.620	3583	3586	3588	rBV2	337	235	0.01%	0.001%
92	12.701	3605	3611	3614	rBV4	1317	1121	0.04%	0.005%
93	12.987	3697	3700	3703	rBV2	503	352	0.01%	0.002%
94	13.157	3750	3753	3758	rBV3	415	525	0.02%	0.002%
95	13.235	3774	3777	3780	rBV4	695	510	0.02%	0.002%
96	13.366	3815	3818	3820	rBV3	561	391	0.01%	0.002%
97	13.408	3827	3831	3838	rVB3	715	705	0.02%	0.003%
98	13.550	3873	3875	3880	rBV4	603	449	0.01%	0.002%
99	13.807	3952	3955	3957	rBV3	737	472	0.02%	0.002%
100	13.939	3993	3996	3997	rBV	666	409	0.01%	0.002%


Sum of corrected areas: 21281209

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV090718\
Data File : VV007457.D
Acq On : 07 Sep 2018 13:33
Operator : SY/MD
Sample : J4719-03 25X
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGD9

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

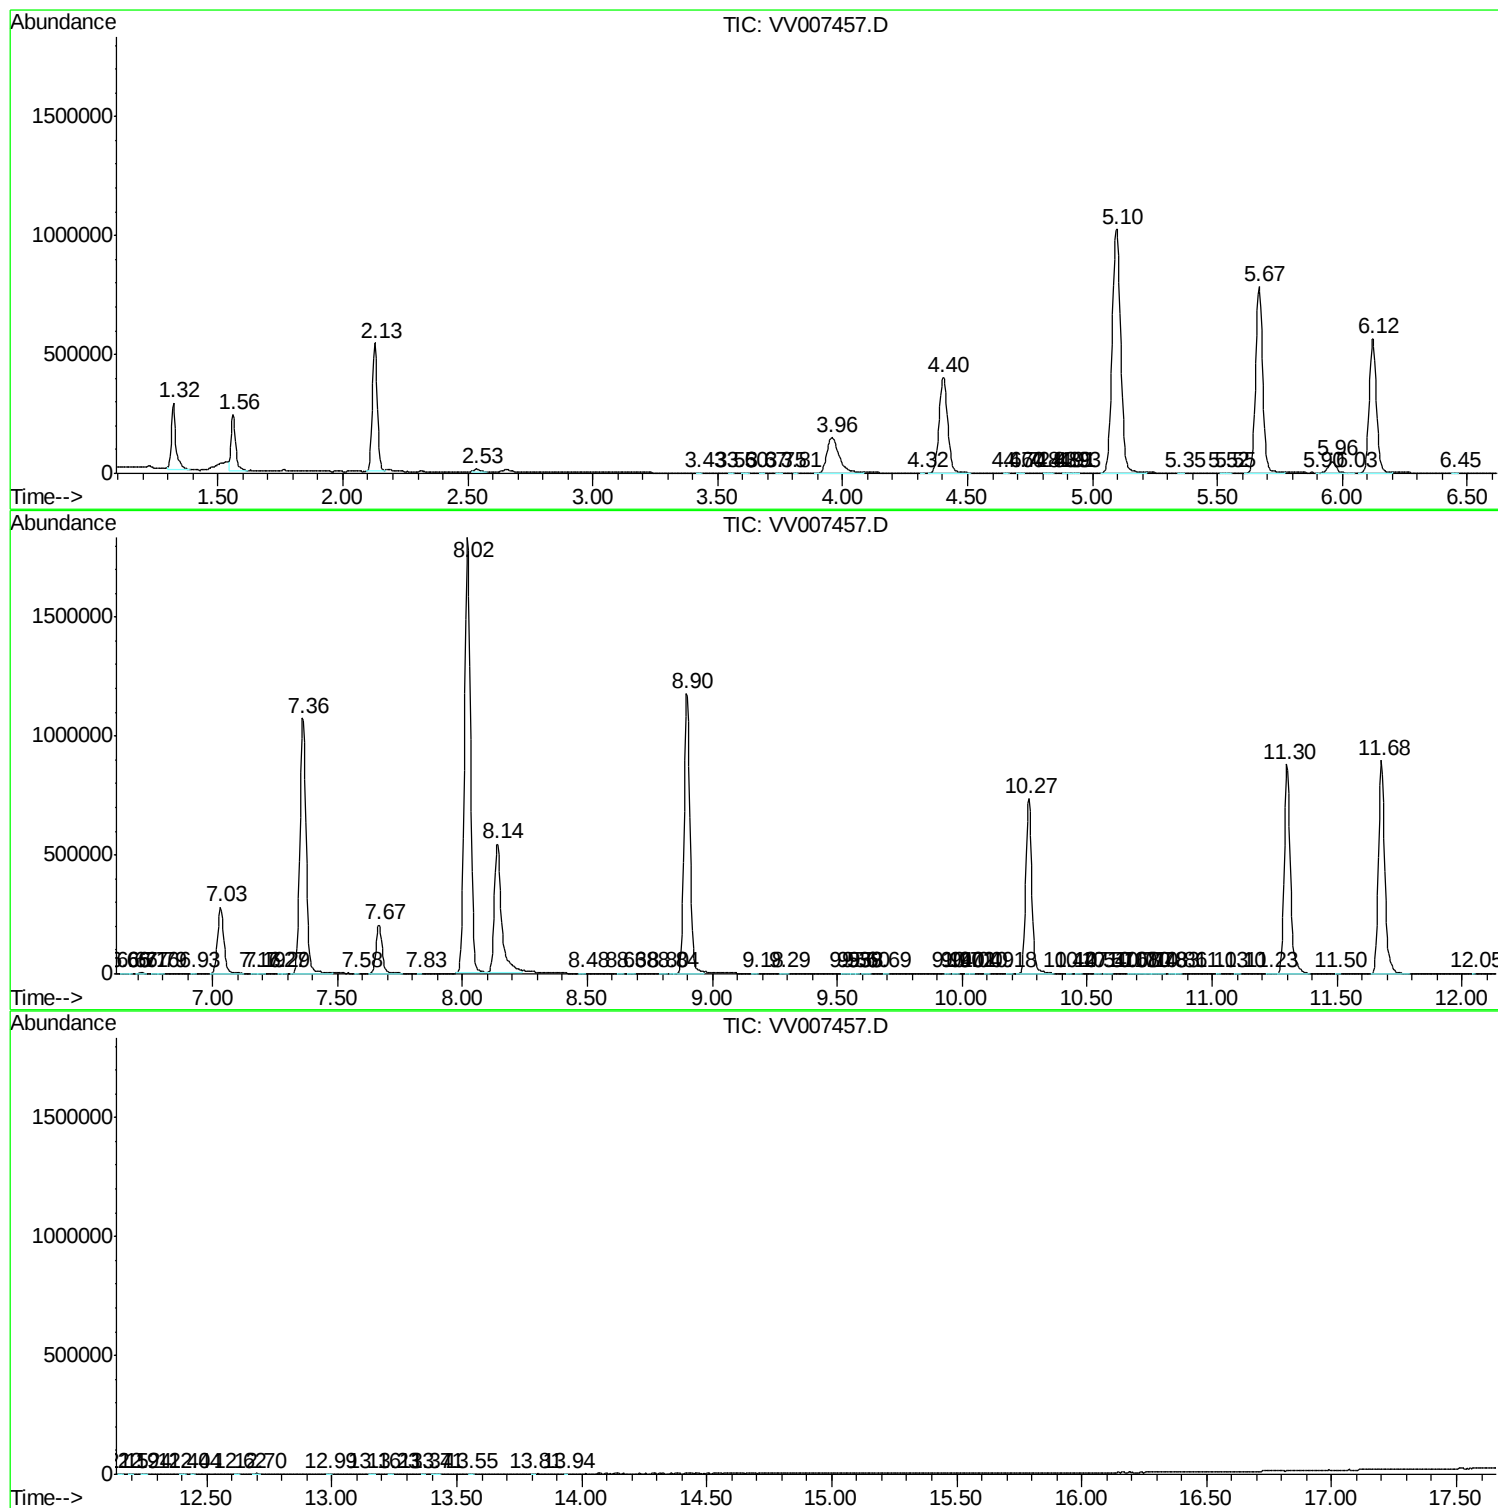

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV090718\
Data File : VV007457.D
Acq On : 07 Sep 2018 13:33
Operator : SY/MD
Sample : J4719-03 25X
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGD9

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV090718\
Data File : VV007457.D
Acq On : 07 Sep 2018 13:33
Operator : SY/MD
Sample : J4719-03 25X
Misc : 5.0 mL/MSV0A_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
BEGD9

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc