

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090718\
 Data File : VV007460.D
 Acq On : 07 Sep 2018 14:47
 Operator : SY/MD
 Sample : J4751-01DL 500X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGH2DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.322	64	72	89	rVB	220979	267960	13.88%	1.661%
2	1.560	140	146	162	rVB	189934	244465	12.67%	1.515%
3	2.126	312	322	335	rBV	424382	602022	31.20%	3.731%
4	2.656	480	487	503	rVB	22736	46624	2.42%	0.289%
5	3.502	746	750	753	rVB3	404	314	0.02%	0.002%
6	3.524	753	757	759	rVB	463	320	0.02%	0.002%
7	3.540	759	762	765	rBV2	552	346	0.02%	0.002%
8	3.608	780	783	786	rBV	293	266	0.01%	0.002%
9	3.769	830	833	840	rBV2	613	432	0.02%	0.003%
10	3.817	845	848	851	rBV2	369	276	0.01%	0.002%
11	3.859	858	861	863	rBV	480	323	0.02%	0.002%
12	3.962	875	893	933	rBV4	127102	445511	23.09%	2.761%
13	4.309	998	1001	1004	rBV3	530	413	0.02%	0.003%
14	4.405	1012	1031	1055	rBV	316751	766409	39.71%	4.750%
15	4.688	1117	1119	1122	rVB2	534	271	0.01%	0.002%
16	4.717	1122	1128	1131	rBV3	720	823	0.04%	0.005%
17	4.884	1177	1180	1183	rVV	455	287	0.01%	0.002%
18	4.910	1183	1188	1190	rVV2	262	274	0.01%	0.002%
19	4.978	1206	1209	1213	rBV2	395	320	0.02%	0.002%
20	5.100	1227	1247	1281	rBV2	816602	1929865	100.00%	11.961%
21	5.299	1307	1309	1313	rBV3	537	380	0.02%	0.002%
22	5.408	1341	1343	1346	rBV	342	254	0.01%	0.002%
23	5.453	1351	1357	1360	rBV2	786	753	0.04%	0.005%
24	5.511	1371	1375	1377	rBV3	695	581	0.03%	0.004%
25	5.669	1408	1424	1447	rBV	638233	1269600	65.79%	7.869%
26	5.955	1501	1513	1530	rVB5	18229	42107	2.18%	0.261%
27	6.039	1535	1539	1543	rBV4	708	733	0.04%	0.005%
28	6.122	1550	1565	1594	rBV	438409	901695	46.72%	5.588%
29	6.315	1623	1625	1628	rBV4	573	260	0.01%	0.002%
30	6.434	1659	1662	1668	rVB3	560	509	0.03%	0.003%
31	6.495	1679	1681	1685	rVV3	470	330	0.02%	0.002%
32	6.576	1703	1706	1708	rVB3	522	297	0.02%	0.002%
33	6.601	1708	1714	1717	rBV3	539	530	0.03%	0.003%
34	6.621	1718	1720	1722	rBV2	437	269	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090718\
 Data File : VV007460.D
 Acq On : 07 Sep 2018 14:47
 Operator : SY/MD
 Sample : J4751-01DL 500X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGH2DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

35	6.723	1745	1752	1759	rBV5	2240	3329	0.17%	0.021%
36	6.817	1777	1781	1783	rBV2	504	386	0.02%	0.002%
37	6.859	1792	1794	1795	rBV2	550	262	0.01%	0.002%
38	6.907	1806	1809	1813	rBV	695	508	0.03%	0.003%
39	7.035	1836	1849	1867	rBV	212842	377350	19.55%	2.339%
40	7.215	1903	1905	1908	rVB4	530	254	0.01%	0.002%
41	7.273	1919	1923	1926	rVB3	496	388	0.02%	0.002%
42	7.293	1926	1929	1932	rBV3	591	351	0.02%	0.002%
43	7.363	1935	1951	1984	rBV	824738	1422701	73.72%	8.817%
44	7.617	2023	2030	2032	rBV4	800	1048	0.05%	0.006%
45	7.669	2034	2046	2062	rBV	158542	265529	13.76%	1.646%
46	7.878	2107	2111	2112	rBV2	503	390	0.02%	0.002%
47	8.022	2141	2156	2180	rBV	1014073	1687764	87.46%	10.460%
48	8.141	2182	2193	2237	rVV2	432757	891091	46.17%	5.523%
49	8.585	2327	2331	2336	rBV6	415	414	0.02%	0.003%
50	8.653	2345	2352	2356	rBV4	719	1057	0.05%	0.007%
51	8.694	2363	2365	2370	rVB2	546	472	0.02%	0.003%
52	8.900	2415	2429	2461	rBV	970787	1580374	81.89%	9.795%
53	9.177	2513	2515	2518	rBV3	620	381	0.02%	0.002%
54	9.225	2526	2530	2532	rBV	366	328	0.02%	0.002%
55	9.270	2542	2544	2547	rVV	481	290	0.02%	0.002%
56	9.309	2554	2556	2558	rVV	592	319	0.02%	0.002%
57	9.383	2574	2579	2585	rBV3	548	594	0.03%	0.004%
58	9.411	2585	2588	2592	rVB4	484	269	0.01%	0.002%
59	9.437	2592	2596	2601	rBV	478	414	0.02%	0.003%
60	9.582	2635	2641	2642	rVV3	456	470	0.02%	0.003%
61	9.592	2642	2644	2647	rVB2	672	386	0.02%	0.002%
62	9.633	2655	2657	2662	rVB2	459	321	0.02%	0.002%
63	9.743	2688	2691	2694	rBV2	367	267	0.01%	0.002%
64	9.884	2733	2735	2739	rVB2	612	399	0.02%	0.002%
65	9.907	2739	2742	2748	rBV3	628	808	0.04%	0.005%
66	10.055	2786	2788	2793	rVB2	447	287	0.01%	0.002%
67	10.087	2793	2798	2804	rBV2	380	568	0.03%	0.004%
68	10.161	2813	2821	2827	rVB2	575	891	0.05%	0.006%
69	10.267	2841	2854	2889	rVB	597094	972289	50.38%	6.026%
70	10.489	2919	2923	2926	rVB3	397	298	0.02%	0.002%
71	10.543	2936	2940	2944	rBV4	552	400	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090718\
 Data File : VV007460.D
 Acq On : 07 Sep 2018 14:47
 Operator : SY/MD
 Sample : J4751-01DL 500X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGH2DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

72	10.643	2968	2971	2973	rBV2	444	302	0.02%	0.002%
73	10.836	3028	3031	3033	rBV3	387	283	0.01%	0.002%
74	10.865	3036	3040	3043	rBV	435	340	0.02%	0.002%
75	10.900	3048	3051	3054	rVB5	626	399	0.02%	0.002%
76	11.000	3079	3082	3088	rVB2	570	488	0.03%	0.003%
77	11.141	3123	3126	3130	rVB2	421	276	0.01%	0.002%
78	11.167	3130	3134	3139	rBV3	310	358	0.02%	0.002%
79	11.299	3163	3175	3203	rBV	696663	1190368	61.68%	7.377%
80	11.399	3204	3206	3211	rVV2	513	357	0.02%	0.002%
81	11.591	3263	3266	3271	rBV3	629	407	0.02%	0.003%
82	11.678	3280	3293	3320	rBV	679236	1178527	61.07%	7.304%
83	12.026	3399	3401	3406	rBV2	358	256	0.01%	0.002%
84	12.415	3519	3522	3524	rBV3	426	285	0.01%	0.002%
85	12.646	3591	3594	3597	rBV3	612	502	0.03%	0.003%
86	12.698	3608	3610	3614	rBV3	486	320	0.02%	0.002%
87	12.723	3616	3618	3623	rVV3	456	355	0.02%	0.002%
88	12.775	3631	3634	3636	rBV	532	331	0.02%	0.002%
89	12.836	3650	3653	3656	rBV	411	354	0.02%	0.002%
90	12.932	3680	3683	3691	rVB4	840	822	0.04%	0.005%
91	13.051	3717	3720	3722	rBV2	766	507	0.03%	0.003%
92	13.318	3799	3803	3807	rBV6	883	1003	0.05%	0.006%
93	13.437	3838	3840	3843	rBV2	547	268	0.01%	0.002%
94	13.501	3858	3860	3862	rBV2	516	254	0.01%	0.002%
95	13.540	3870	3872	3877	rBV3	624	413	0.02%	0.003%
96	13.640	3901	3903	3909	rVB3	903	724	0.04%	0.004%
97	13.739	3932	3934	3936	rBV2	510	257	0.01%	0.002%
98	14.302	4107	4109	4111	rBV3	769	376	0.02%	0.002%
99	14.492	4165	4168	4171	rBV3	1226	934	0.05%	0.006%
100	14.823	4267	4271	4275	rBV	28580	15608	0.81%	0.097%


Sum of corrected areas: 16135140

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV090718\
Data File : VV007460.D
Acq On : 07 Sep 2018 14:47
Operator : SY/MD
Sample : J4751-01DL 500X
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGH2DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

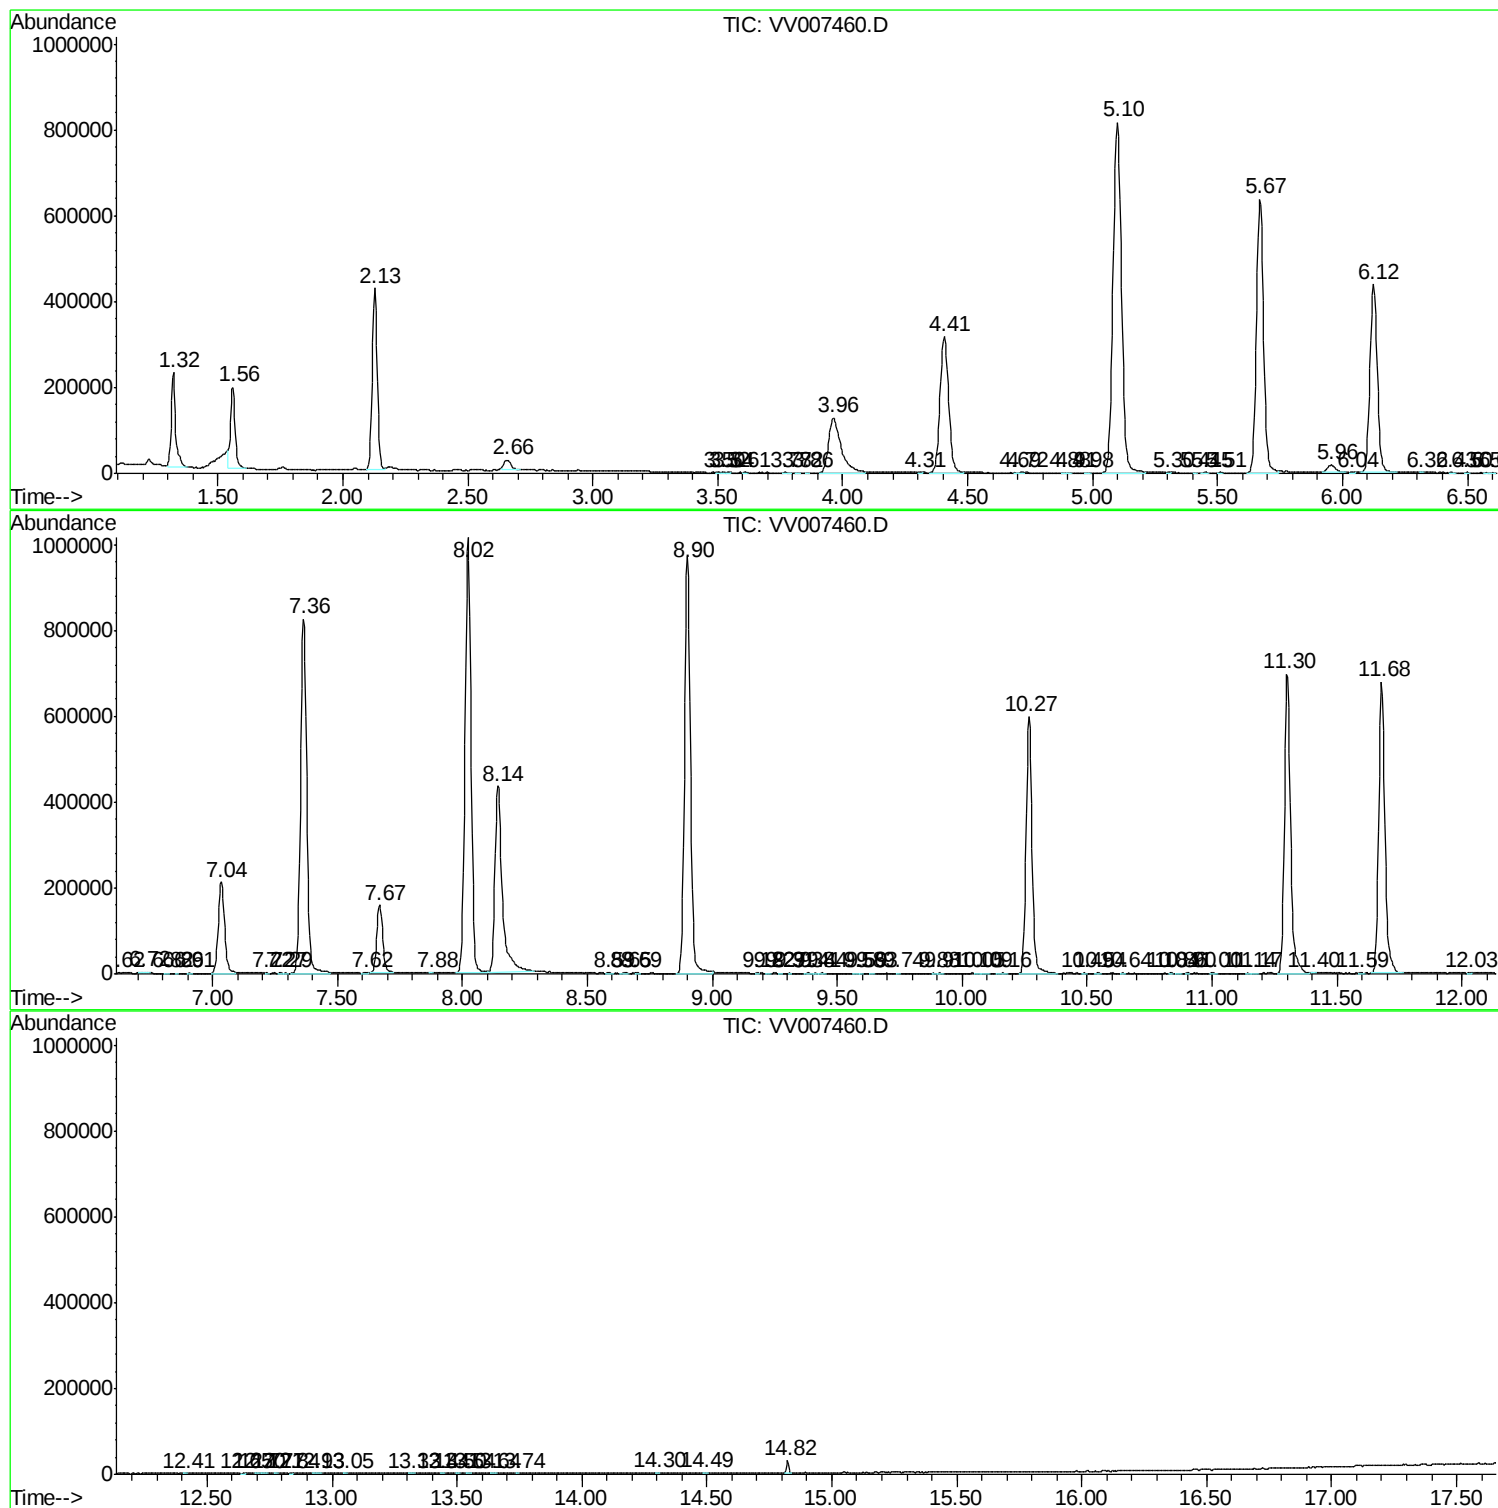

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV090718\
Data File : VV007460.D
Acq On : 07 Sep 2018 14:47
Operator : SY/MD
Sample : J4751-01DL 500X
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGH2DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV090718\
Data File : VV007460.D
Acq On : 07 Sep 2018 14:47
Operator : SY/MD
Sample : J4751-01DL 500X
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGH2DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc