

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090718\
 Data File : VV007463.D
 Acq On : 07 Sep 2018 16:02
 Operator : SY/MD
 Sample : J4751-07DL 1000X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGH8DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.322	64	72	88	rVB	213429	258875	13.59%	1.662%
2	1.557	140	145	165	rVB	190899	239842	12.60%	1.540%
3	2.126	312	322	335	rBV	418906	592266	31.10%	3.803%
4	2.656	480	487	504	rVB	25038	52016	2.73%	0.334%
5	3.425	722	726	730	rVB3	583	519	0.03%	0.003%
6	3.463	735	738	740	rBV2	694	448	0.02%	0.003%
7	3.505	748	751	756	rBV3	626	704	0.04%	0.005%
8	3.704	811	813	817	rVV	499	307	0.02%	0.002%
9	3.769	828	833	840	rBV4	444	572	0.03%	0.004%
10	3.962	875	893	933	rBV3	131578	453630	23.82%	2.913%
11	4.335	1007	1009	1012	rVB2	745	399	0.02%	0.003%
12	4.405	1012	1031	1053	rBV	317407	760419	39.93%	4.883%
13	4.646	1103	1106	1108	rVB2	494	290	0.02%	0.002%
14	4.720	1124	1129	1131	rBV	532	499	0.03%	0.003%
15	4.920	1186	1191	1196	rVB2	374	447	0.02%	0.003%
16	5.097	1224	1246	1277	rBV2	808387	1904239	100.00%	12.227%
17	5.354	1324	1326	1331	rVB2	465	275	0.01%	0.002%
18	5.428	1345	1349	1350	rBV3	481	279	0.01%	0.002%
19	5.508	1370	1374	1376	rBV	599	457	0.02%	0.003%
20	5.669	1408	1424	1452	rBV	641431	1270512	66.72%	8.158%
21	5.958	1501	1514	1528	rVB6	21760	50298	2.64%	0.323%
22	6.126	1549	1566	1597	rBV	441173	897470	47.13%	5.763%
23	6.447	1663	1666	1672	rVB2	536	375	0.02%	0.002%
24	6.544	1693	1696	1701	rVB3	790	613	0.03%	0.004%
25	6.569	1701	1704	1707	rBV4	669	462	0.02%	0.003%
26	6.637	1721	1725	1726	rBV	612	416	0.02%	0.003%
27	6.653	1726	1730	1733	rVV5	891	735	0.04%	0.005%
28	6.733	1744	1755	1767	rVB5	2338	5211	0.27%	0.033%
29	6.778	1767	1769	1777	rVB4	667	738	0.04%	0.005%
30	6.817	1777	1781	1783	rVB3	392	278	0.01%	0.002%
31	6.868	1793	1797	1802	rBV2	579	448	0.02%	0.003%
32	6.926	1813	1815	1821	rVB3	493	431	0.02%	0.003%
33	6.952	1821	1823	1827	rVB3	500	385	0.02%	0.002%
34	6.984	1827	1833	1836	rBV4	698	747	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090718\
 Data File : VV007463.D
 Acq On : 07 Sep 2018 16:02
 Operator : SY/MD
 Sample : J4751-07DL 1000X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGH8DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

35	7.035	1836	1849	1872	rBV	208668	373887	19.63%	2.401%
36	7.363	1937	1951	1969	rBV	798659	1375337	72.23%	8.831%
37	7.550	2007	2009	2013	rVB2	1050	588	0.03%	0.004%
38	7.669	2034	2046	2066	rBV	156101	264582	13.89%	1.699%
39	7.801	2085	2087	2091	rVB3	675	424	0.02%	0.003%
40	8.023	2142	2156	2175	rBV	723000	1210991	63.59%	7.776%
41	8.145	2182	2194	2233	rBV2	439380	901825	47.36%	5.791%
42	8.579	2326	2329	2332	rBV3	574	417	0.02%	0.003%
43	8.656	2351	2353	2359	rVB4	718	632	0.03%	0.004%
44	8.688	2360	2363	2367	rBV2	416	279	0.01%	0.002%
45	8.775	2387	2390	2392	rVB2	515	279	0.01%	0.002%
46	8.791	2392	2395	2397	rBV3	759	450	0.02%	0.003%
47	8.900	2412	2429	2459	rBV	978316	1577863	82.86%	10.132%
48	9.125	2497	2499	2506	rVB3	1116	920	0.05%	0.006%
49	9.183	2514	2517	2523	rVB5	831	911	0.05%	0.006%
50	9.219	2523	2528	2531	rBV2	351	360	0.02%	0.002%
51	9.386	2577	2580	2583	rVB3	419	303	0.02%	0.002%
52	9.415	2583	2589	2594	rBV2	611	660	0.03%	0.004%
53	9.553	2629	2632	2638	rVV3	466	348	0.02%	0.002%
54	9.585	2641	2642	2648	rVB2	487	445	0.02%	0.003%
55	9.617	2648	2652	2654	rBV	328	272	0.01%	0.002%
56	9.707	2676	2680	2685	rVB2	389	312	0.02%	0.002%
57	9.752	2689	2694	2695	rBV3	553	439	0.02%	0.003%
58	9.791	2701	2706	2708	rBV3	472	303	0.02%	0.002%
59	9.810	2709	2712	2717	rVB	388	298	0.02%	0.002%
60	9.865	2726	2729	2733	rBV3	411	285	0.01%	0.002%
61	10.022	2772	2778	2781	rVV3	322	404	0.02%	0.003%
62	10.061	2788	2790	2796	rBV4	638	491	0.03%	0.003%
63	10.154	2813	2819	2823	rBV3	486	626	0.03%	0.004%
64	10.267	2840	2854	2892	rVB	605008	985573	51.76%	6.329%
65	10.399	2892	2895	2898	rBV2	649	431	0.02%	0.003%
66	10.431	2898	2905	2906	rBV3	760	724	0.04%	0.005%
67	10.592	2952	2955	2958	rBV2	518	297	0.02%	0.002%
68	10.624	2958	2965	2968	rVB4	563	597	0.03%	0.004%
69	10.662	2972	2977	2978	rBV2	355	283	0.01%	0.002%
70	10.694	2983	2987	2990	rVB3	452	342	0.02%	0.002%
71	10.768	3007	3010	3014	rBV	427	342	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090718\
 Data File : VV007463.D
 Acq On : 07 Sep 2018 16:02
 Operator : SY/MD
 Sample : J4751-07DL 1000X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGH8DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

72	10.910	3050	3054	3056	rVB2	611	416	0.02%	0.003%
73	11.067	3099	3103	3107	rVB4	484	479	0.03%	0.003%
74	11.106	3109	3115	3116	rBV2	441	409	0.02%	0.003%
75	11.157	3127	3131	3135	rBV3	308	290	0.02%	0.002%
76	11.203	3143	3145	3150	rBV3	428	313	0.02%	0.002%
77	11.231	3150	3154	3156	rVV2	396	331	0.02%	0.002%
78	11.299	3160	3175	3206	rVV	700488	1193339	62.67%	7.663%
79	11.453	3220	3223	3227	rBV4	596	635	0.03%	0.004%
80	11.627	3273	3277	3279	rBV2	570	421	0.02%	0.003%
81	11.678	3280	3293	3324	rVV	690612	1168106	61.34%	7.501%
82	11.903	3361	3363	3371	rVB5	1016	1085	0.06%	0.007%
83	12.029	3400	3402	3406	rBV3	467	334	0.02%	0.002%
84	12.109	3424	3427	3430	rBV3	437	368	0.02%	0.002%
85	12.145	3436	3438	3442	rVB2	427	307	0.02%	0.002%
86	12.276	3474	3479	3485	rVB5	763	811	0.04%	0.005%
87	12.305	3485	3488	3491	rBV3	512	485	0.03%	0.003%
88	12.444	3529	3531	3534	rBV3	425	320	0.02%	0.002%
89	12.485	3540	3544	3548	rBV3	455	366	0.02%	0.002%
90	12.521	3552	3555	3559	rBV2	562	417	0.02%	0.003%
91	12.739	3621	3623	3628	rVB4	424	284	0.01%	0.002%
92	13.318	3800	3803	3805	rBV3	662	334	0.02%	0.002%
93	13.379	3820	3822	3824	rBV2	452	276	0.01%	0.002%
94	13.450	3837	3844	3847	rBV4	610	787	0.04%	0.005%
95	13.710	3919	3925	3929	rBV5	653	811	0.04%	0.005%
96	13.749	3935	3937	3941	rBV2	518	386	0.02%	0.002%
97	13.813	3953	3957	3960	rBV3	1048	963	0.05%	0.006%
98	13.910	3983	3987	3988	rBV4	641	489	0.03%	0.003%
99	14.029	4022	4024	4028	rBV3	608	396	0.02%	0.003%
100	14.067	4034	4036	4039	rBV2	863	384	0.02%	0.002%


Sum of corrected areas: 15573464

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV090718\
Data File : VV007463.D
Acq On : 07 Sep 2018 16:02
Operator : SY/MD
Sample : J4751-07DL 1000X
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGH8DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

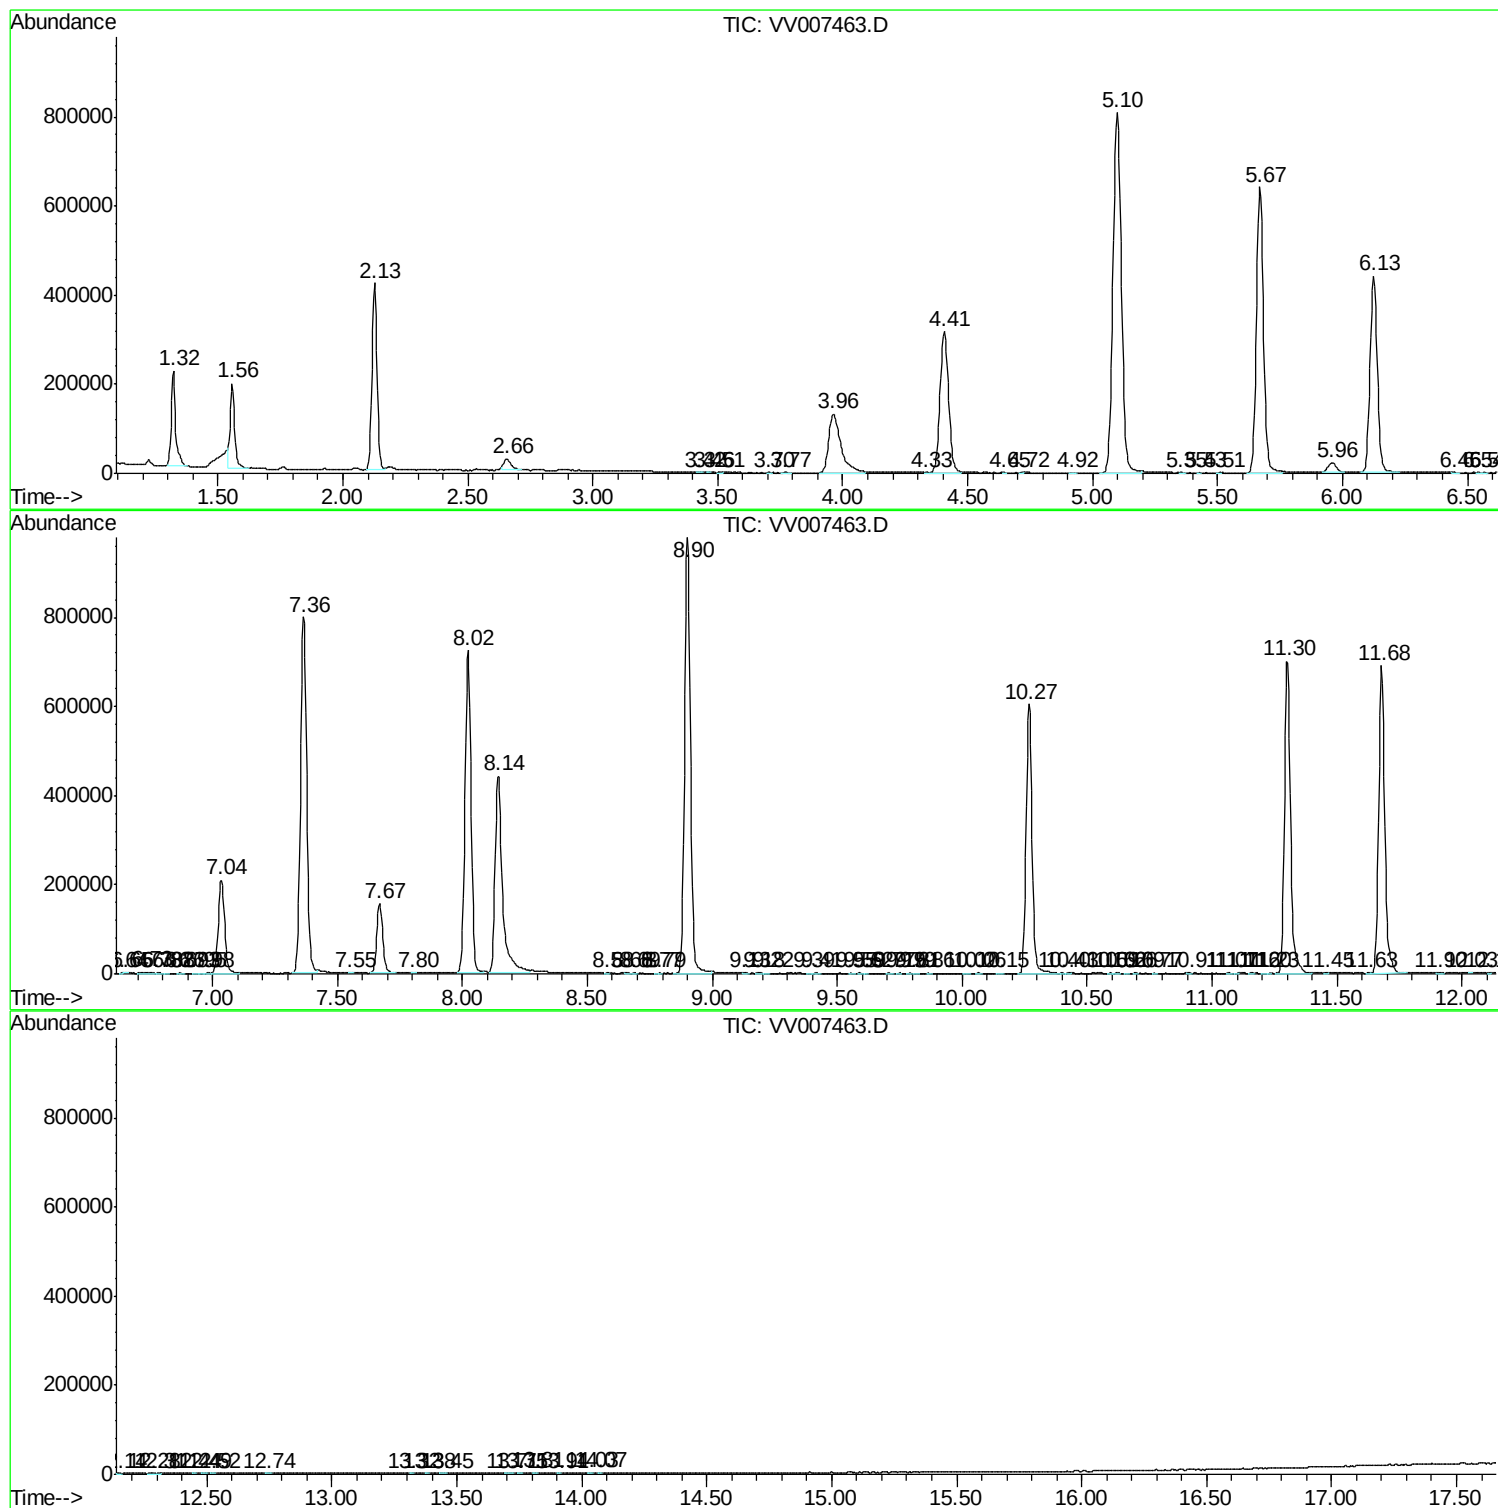

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV090718\
Data File : VV007463.D
Acq On : 07 Sep 2018 16:02
Operator : SY/MD
Sample : J4751-07DL 1000X
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGH8DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV090718\
Data File : VV007463.D
Acq On : 07 Sep 2018 16:02
Operator : SY/MD
Sample : J4751-07DL 1000X
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGH8DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc