


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090718\
 Data File : VV007454.D
 Acq On : 07 Sep 2018 09:22
 Operator : SY/MD
 Sample : BFB74
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB74

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis
 Last Update : Sat Sep 08 05:06:23 2018

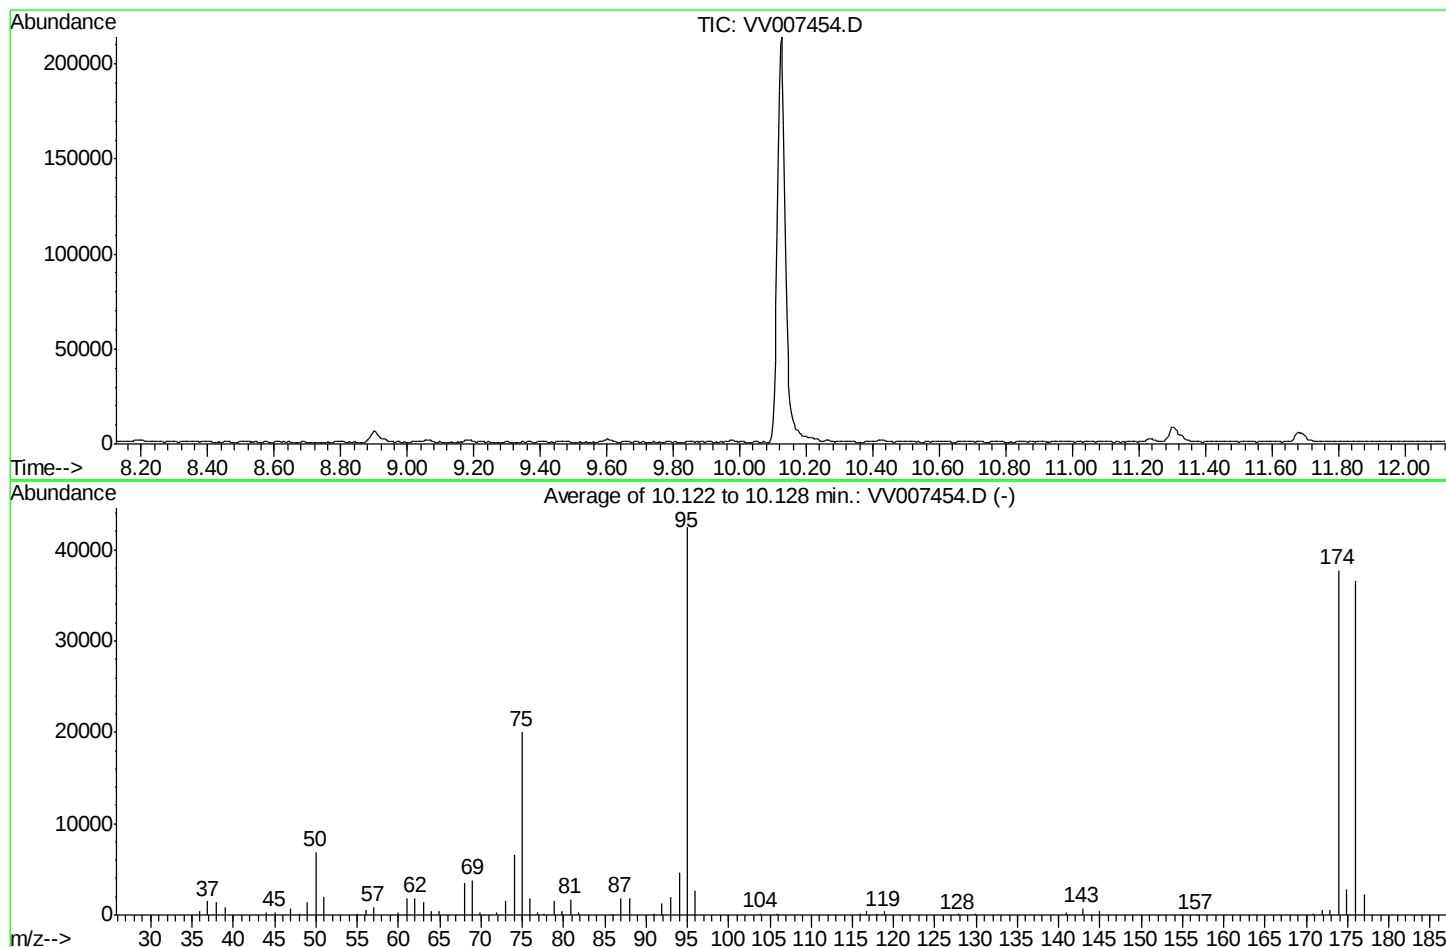

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2798

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.2	6882	PASS
75	95	30	80	47.3	20056	PASS
95	95	100	100	100.0	42442	PASS
96	95	5	9	6.2	2645	PASS
173	174	0.00	2	1.5	555	PASS
174	95	50	120	88.9	37730	PASS
175	174	5	9	7.5	2846	PASS
176	174	95	101	96.8	36525	PASS
177	176	5	9	6.3	2312	PASS

Scan 2798 (10.087 min): VV007454.D
BFB74

m/z	Abundance
39.80	298.0
44.10	678.0

Instrument :
MSVOA_V
ClientSampleId :
BFB74

m/z	Abundance
35.90	373.0
36.90	1608.0
38.00	1432.0
39.00	900.0
39.90	212.0
44.00	1060.0
45.00	300.0
46.90	635.0
48.00	190.0
49.00	1417.0
50.00	7104.0
51.00	2140.0
55.00	127.0
56.10	601.0
57.00	981.0
60.00	314.0
61.00	1987.0
62.00	1916.0
63.00	1499.0
64.00	333.0
64.90	413.0
66.90	105.0
68.00	3500.0
69.00	3954.0
70.00	261.0
71.90	291.0
73.00	1664.0
74.00	6679.0
75.00	20784.0
76.00	2025.0
76.90	297.0
77.60	147.0
78.80	1726.0
79.80	419.0
80.80	1788.0
81.80	396.0
86.90	2026.0
88.00	1866.0
90.90	127.0
91.90	1275.0
93.00	2089.0
94.00	4667.0
95.00	42784.0
96.00	2666.0
103.90	202.0
105.90	136.0
115.90	128.0
116.70	373.0
117.90	159.0
118.90	380.0
127.80	135.0
129.80	118.0
140.90	382.0
142.90	739.0
144.90	334.0
154.80	105.0
156.70	108.0
170.80	143.0
172.00	577.0
172.90	557.0
173.90	37320.0
174.90	2746.0
175.90	36048.0
176.90	2246.0

Instrument :
MSVOA_V
ClientSampleId :
BFB74

m/z	Abundance
35.90	376.0
36.90	1561.0
38.00	1371.0
39.00	956.0
39.90	256.0
44.00	948.0
45.00	301.0
46.90	691.0
48.00	193.0
49.00	1444.0
50.00	7142.0
51.00	1928.0
55.00	130.0
56.10	591.0
57.00	902.0
60.00	291.0
61.00	1817.0
62.00	1871.0
63.10	1462.0
64.00	398.0
64.90	434.0
68.00	3509.0
69.00	3946.0
69.90	256.0
71.90	278.0
73.00	1620.0
74.00	6866.0
75.00	20704.0
76.00	1957.0
76.90	284.0
77.70	189.0
78.90	1611.0
79.80	427.0
80.90	1814.0
81.90	346.0
86.90	1919.0
88.00	1954.0
90.90	129.0
91.90	1306.0
93.00	2048.0
94.00	4787.0
95.00	43880.0
96.00	2699.0
103.80	172.0
105.90	143.0
116.00	109.0
116.70	366.0
117.90	188.0
118.80	408.0
127.80	131.0
129.80	125.0
140.90	328.0
142.90	741.0
144.90	392.0
156.70	104.0
170.80	194.0
171.90	602.0
172.90	588.0
173.90	38888.0
174.90	2960.0
175.90	37832.0
177.00	2430.0

Instrument :
MSVOA_V
ClientSampleId :
BFB74

m/z	Abundance
35.90	345.0
36.90	1302.0
38.00	1271.0
39.00	822.0
39.90	313.0
44.00	823.0
45.00	335.0
46.90	637.0
48.00	175.0
49.00	1374.0
50.00	6400.0
51.00	1717.0
55.00	113.0
56.00	541.0
56.90	748.0
60.00	301.0
61.00	1601.0
62.00	1682.0
63.00	1376.0
64.00	413.0
64.90	399.0
68.00	3406.0
69.00	3537.0
70.00	247.0
71.90	208.0
73.00	1432.0
74.00	6419.0
75.00	18680.0
76.00	1652.0
76.90	258.0
77.80	192.0
78.90	1389.0
79.90	407.0
80.90	1552.0
81.90	270.0
85.90	119.0
86.90	1722.0
87.90	1819.0
90.90	130.0
91.90	1220.0
93.00	1782.0
94.00	4507.0
95.00	40664.0
96.00	2572.0
103.80	137.0
105.90	136.0
116.80	339.0
117.90	204.0
118.80	351.0
127.80	113.0
129.90	128.0
140.90	273.0
142.90	710.0
144.90	388.0
170.80	187.0
171.90	632.0
172.80	521.0
173.90	36984.0
174.90	2832.0
175.90	35696.0
176.90	2260.0

Instrument :
MSVOA_V
ClientSampleId :
BFB74