


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090721\
Data File : VV022099.D
Acq On : 07 Sep 2021 13:47
Operator : SY/MD
Sample : M3651-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKM2

Manual Integrations
APPROVED

MMDadoda
9/8/2021 10:17:10 AM

Quant Time: Sep 08 01:16:40 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Sep 08 01:14:49 2021
Response via : Initial Calibration

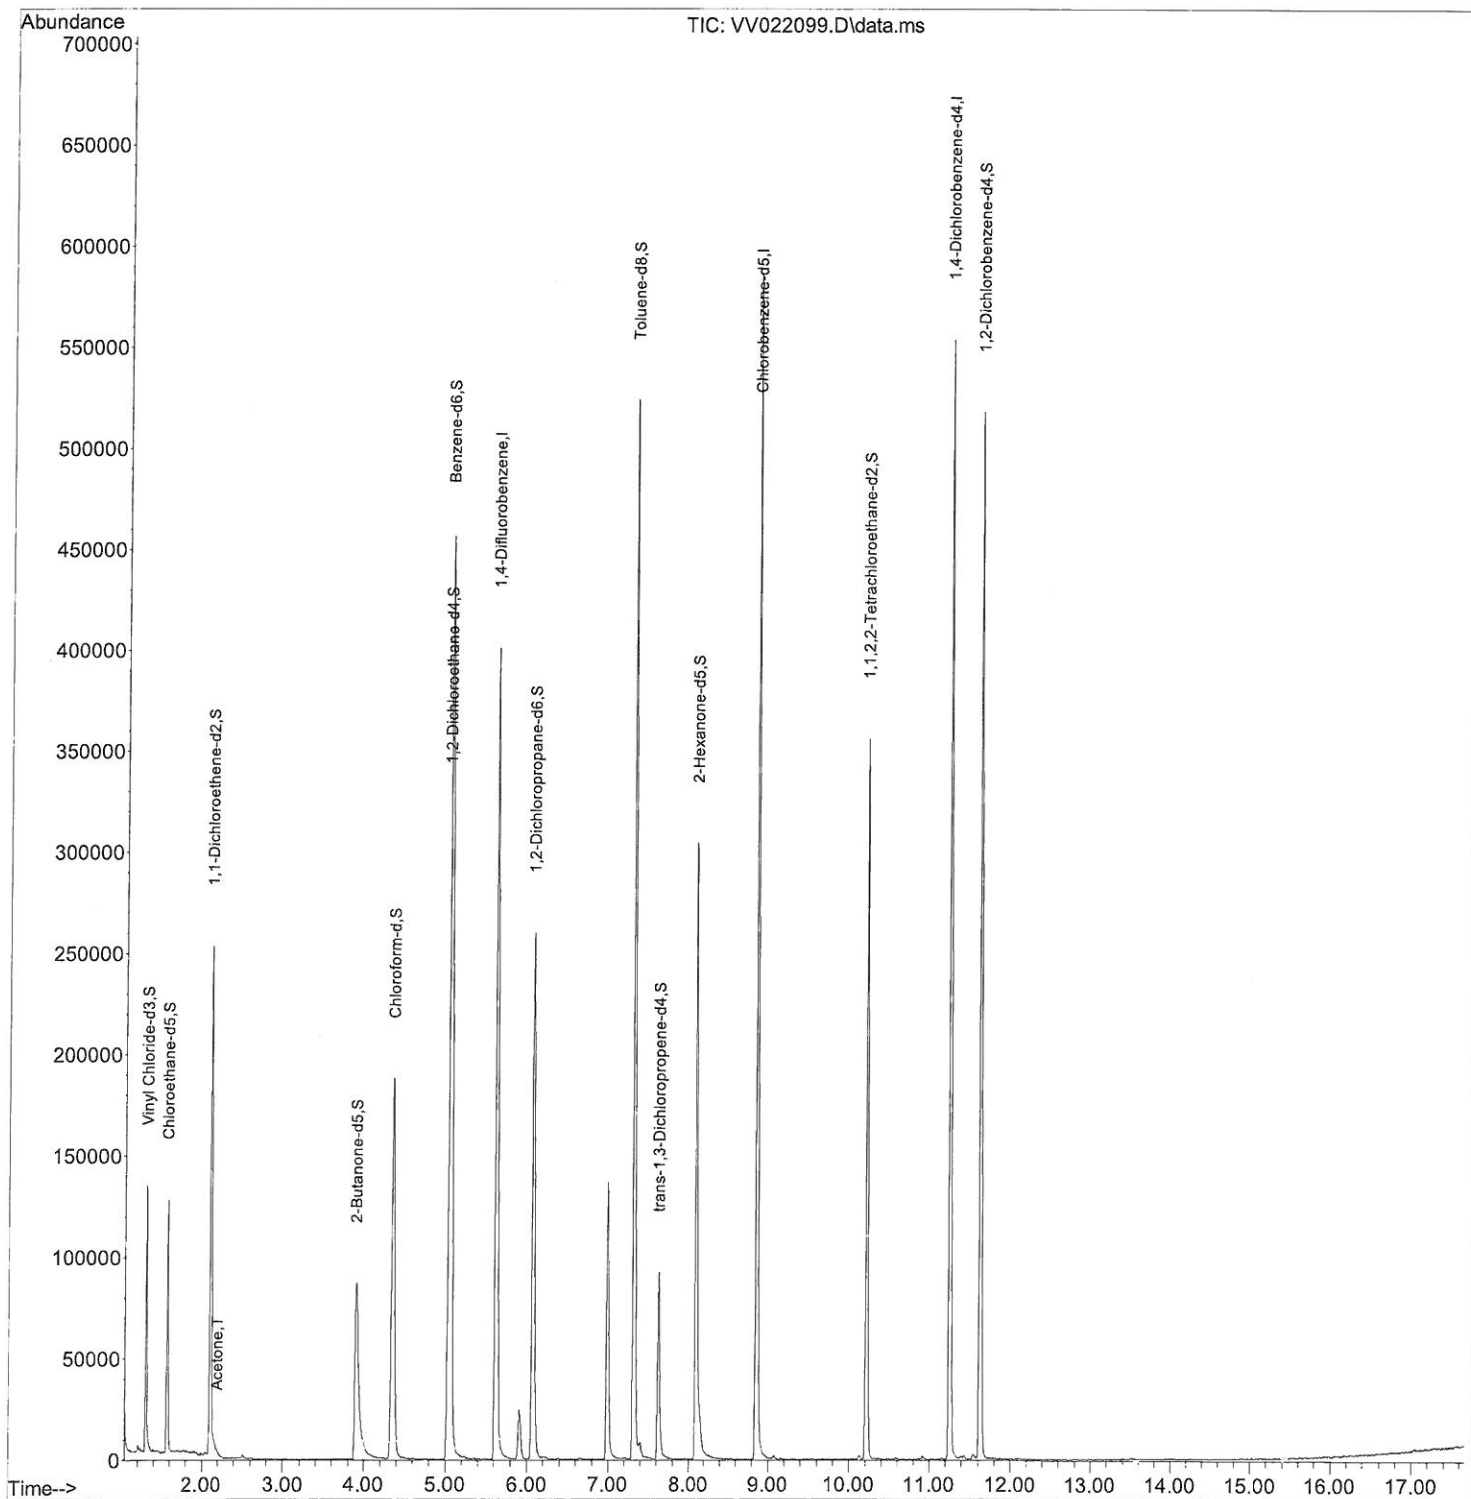

Quantitation Report (Qedit)


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090721\
Data File : VV022099.D
Acq On : 07 Sep 2021 13:47
Operator : SY/MD
Sample : M3651-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKM2

Manual Integrations
APPROVED

MMDadoda
9/8/2021 10:17:10 AM

Quant Time: Sep 08 01:16:40 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Sep 08 01:14:49 2021
Response via : Initial Calibration

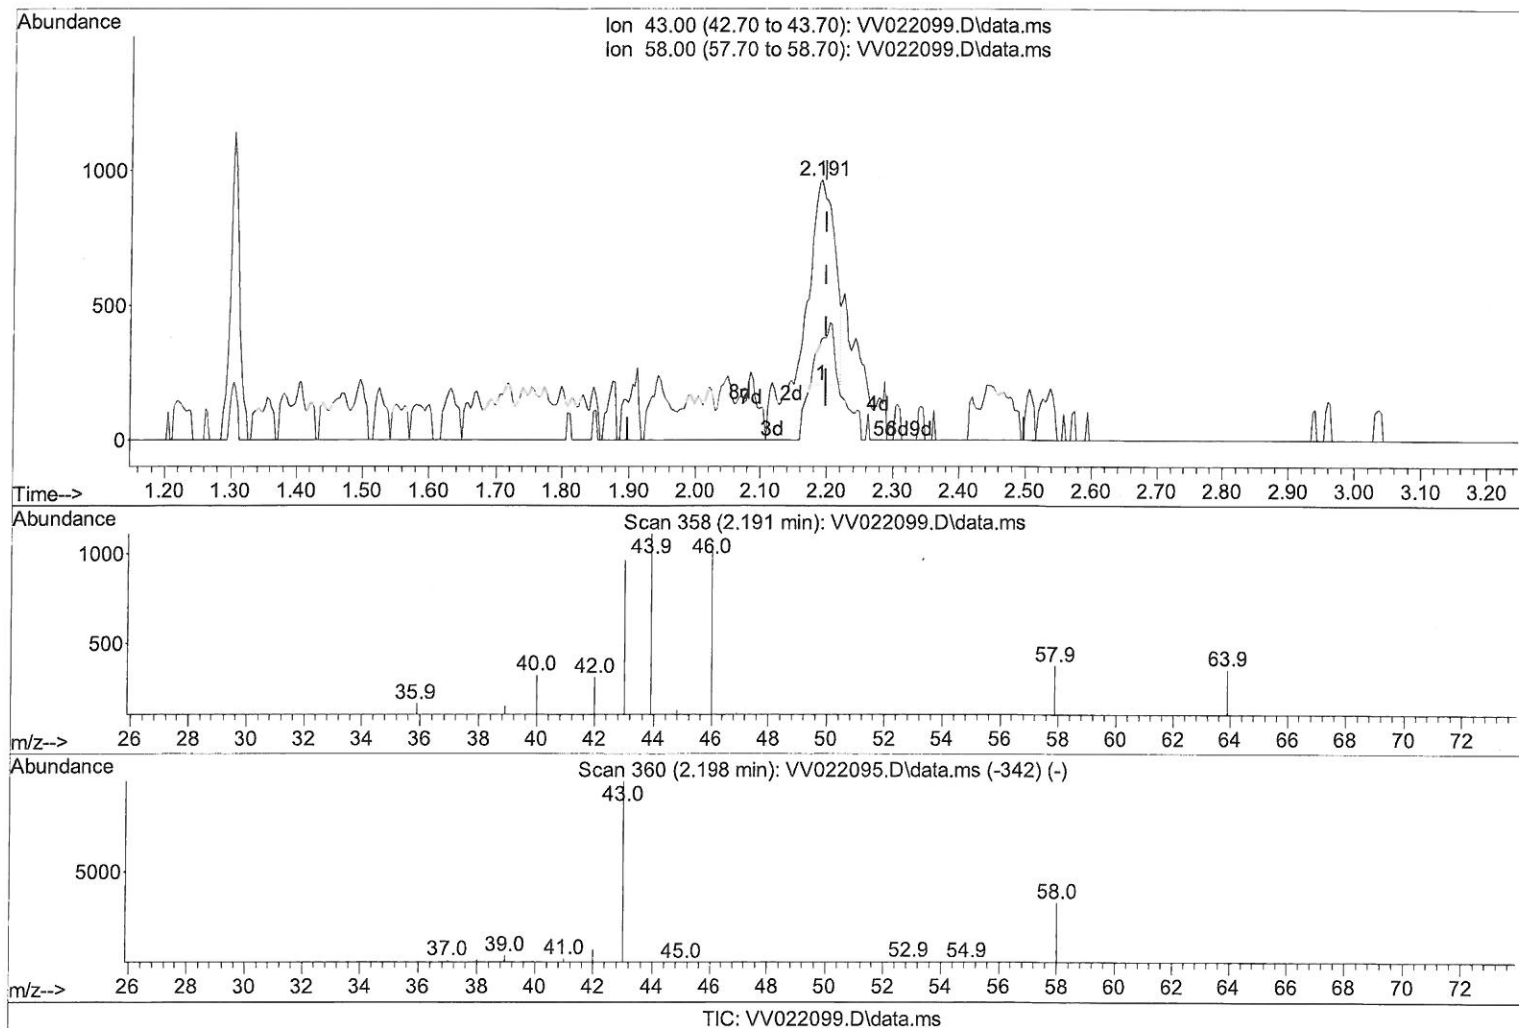

(13) Acetone (T)

2.191min (-0.006) 1.35 ug/L

response 1927

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	0.20	32.12#
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090721\
 Data File : VV022099.D
 Acq On : 07 Sep 2021 13:47
 Operator : SY/MD
 Sample : M3651-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKM2

Manual Integrations
 APPROVED

MMDadoda
 9/8/2021 10:17:10 AM

Quant Time: Sep 08 01:16:40 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Sep 08 01:14:49 2021
 Response via : Initial Calibration

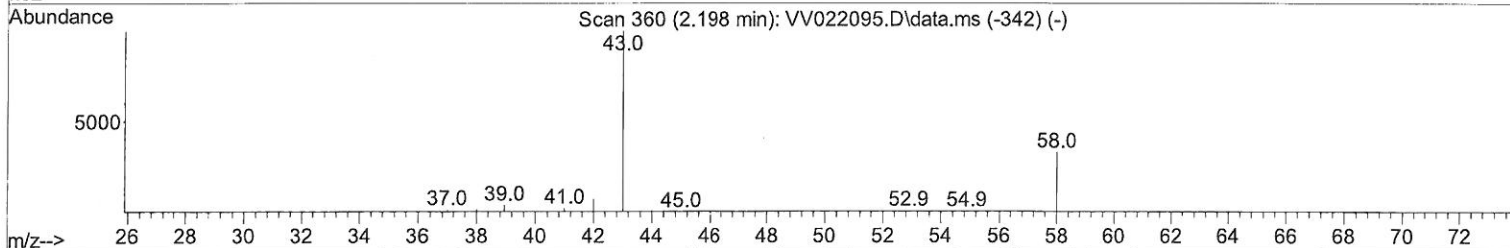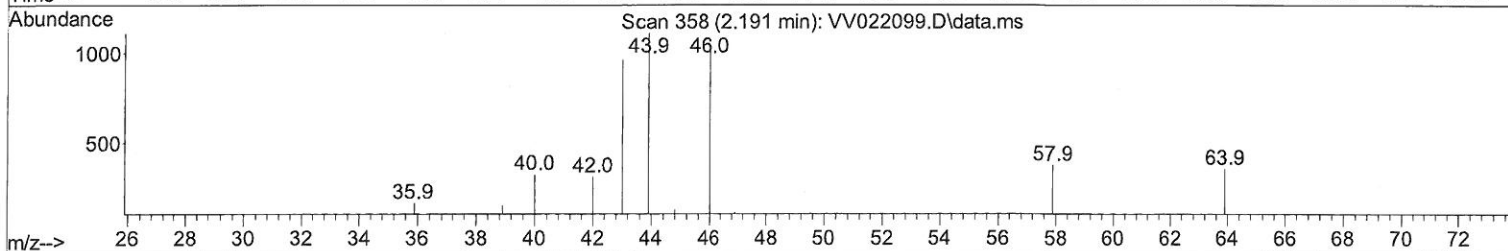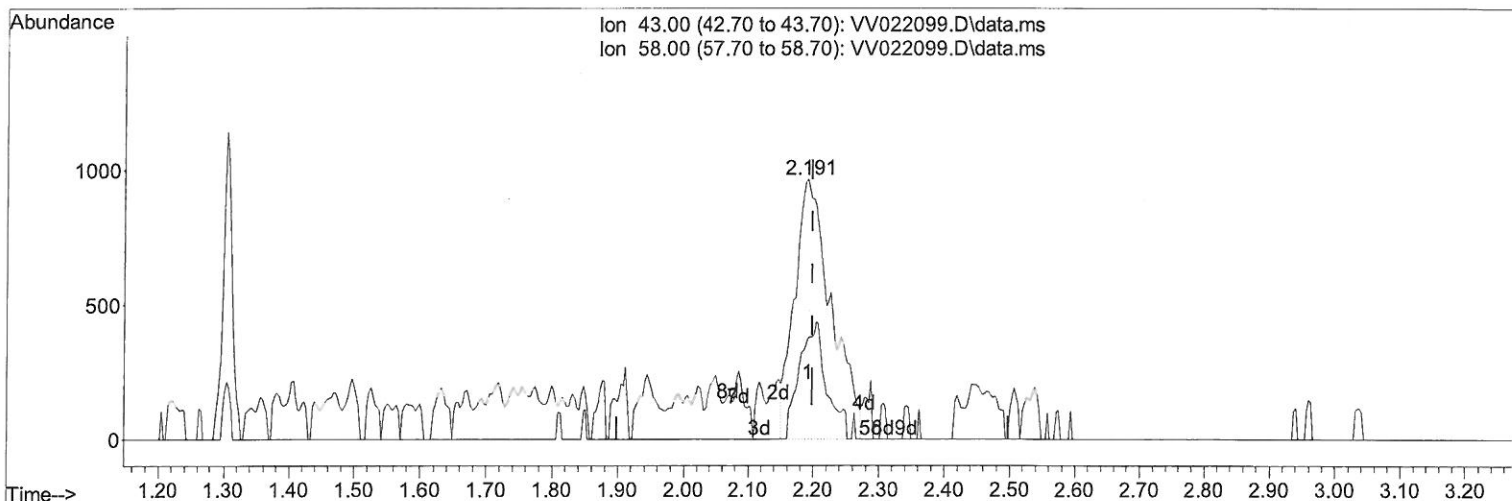

TIC: VV022099.D\data.ms

(13) Acetone (T)

2.191min (-0.006) 2.64 ug/L m

response 3767

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	0.20	16.43#
0.00	0.00	0.00
0.00	0.00	0.00

Handwritten: 7 MD
9/10/21

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\V090721\
 Data File : V022099.D
 Acq On : 07 Sep 2021 13:47
 Operator : SY/MD
 Sample : M3651-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKM2

Manual Integrations
 APPROVED

MMDadoda
 9/8/2021 10:17:10 AM

Quant Time: Sep 08 01:16:40 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Sep 08 01:14:49 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	358360	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	332747	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	150051	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	86633	34.909	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	69.820%		
7) Chloroethane-d5	1.568	69	77028	39.746	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	79.500%		
11) 1,1-Dichloroethene-d2	2.105	63	130381	31.767	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	63.540%		
21) 2-Butanone-d5	3.899	46	182323	107.124	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	107.120%		
24) Chloroform-d	4.352	84	197042	43.544	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	87.080%		
26) 1,2-Dichloroethane-d4	5.034	65	122683	46.028	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	92.060%		
32) Benzene-d6	5.050	84	397102	43.999	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	88.000%		
36) 1,2-Dichloropropane-d6	6.072	67	127676	44.983	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	89.960%		
41) Toluene-d8	7.317	98	353176	41.455	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	82.900%		
43) trans-1,3-Dichloroprop...	7.625	79	54468	40.319	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	80.640%		
47) 2-Hexanone-d5	8.091	63	105883	97.225	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	97.220%		
56) 1,1,2,2-Tetrachloroeth...	10.217	84	168125	46.251	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	92.500%		
66) 1,2-Dichlorobenzene-d4	11.625	152	139809	47.396	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	94.800%		

Target Compounds					Qvalue
13) Acetone	2.191	43	3767m	2.642	ug/L

7 MD
9/10/21

(#) = qualifier out of range (m) = manual integration (+) = signals summed