

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090721\
 Data File : VV022098.D
 Acq On : 07 Sep 2021 13:23
 Operator : SY/MD
 Sample : M3651-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKL9

Manual Integrations
 APPROVED

MMDadoda
 9/8/2021 10:17:07 AM

Quant Time: Sep 08 01:16:27 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Sep 08 01:14:49 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	344802	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	324529	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	149854	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	86852	36.373	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	72.740%		
7) Chloroethane-d5	1.564	69	75981	40.747	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	81.500%		
11) 1,1-Dichloroethene-d2	2.101	63	129114	32.695	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	65.400%		
21) 2-Butanone-d5	3.889	46	169684	103.618	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	103.620%		
24) Chloroform-d	4.346	84	194317	44.630	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	89.260%		
26) 1,2-Dichloroethane-d4	5.031	65	121414	47.343	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	94.680%		
32) Benzene-d6	5.047	84	393425	44.696	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	89.400%		
36) 1,2-Dichloropropane-d6	6.069	67	127692	46.128	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	92.260%		
41) Toluene-d8	7.317	98	351477	42.300	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	84.600%		
43) trans-1,3-Dichloroprop...	7.622	79	53233	40.403	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	80.800%		
47) 2-Hexanone-d5	8.088	63	101965	95.998	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	96.000%		
56) 1,1,2,2-Tetrachloroeth...	10.217	84	162863	45.938	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	91.880%		
66) 1,2-Dichlorobenzene-d4	11.625	152	140712	47.764	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	95.520%		
Target Compounds					Qvalue	
13) Acetone	2.185	43	4290m	3.127	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090721\
Data File : VV022098.D
Acq On : 07 Sep 2021 13:23
Operator : SY/MD
Sample : M3651-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
DBKL9

Manual Integrations
APPROVED

MMDadoda
9/8/2021 10:17:07 AM

Quant Time: Sep 08 01:16:27 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Sep 08 01:14:49 2021
Response via : Initial Calibration

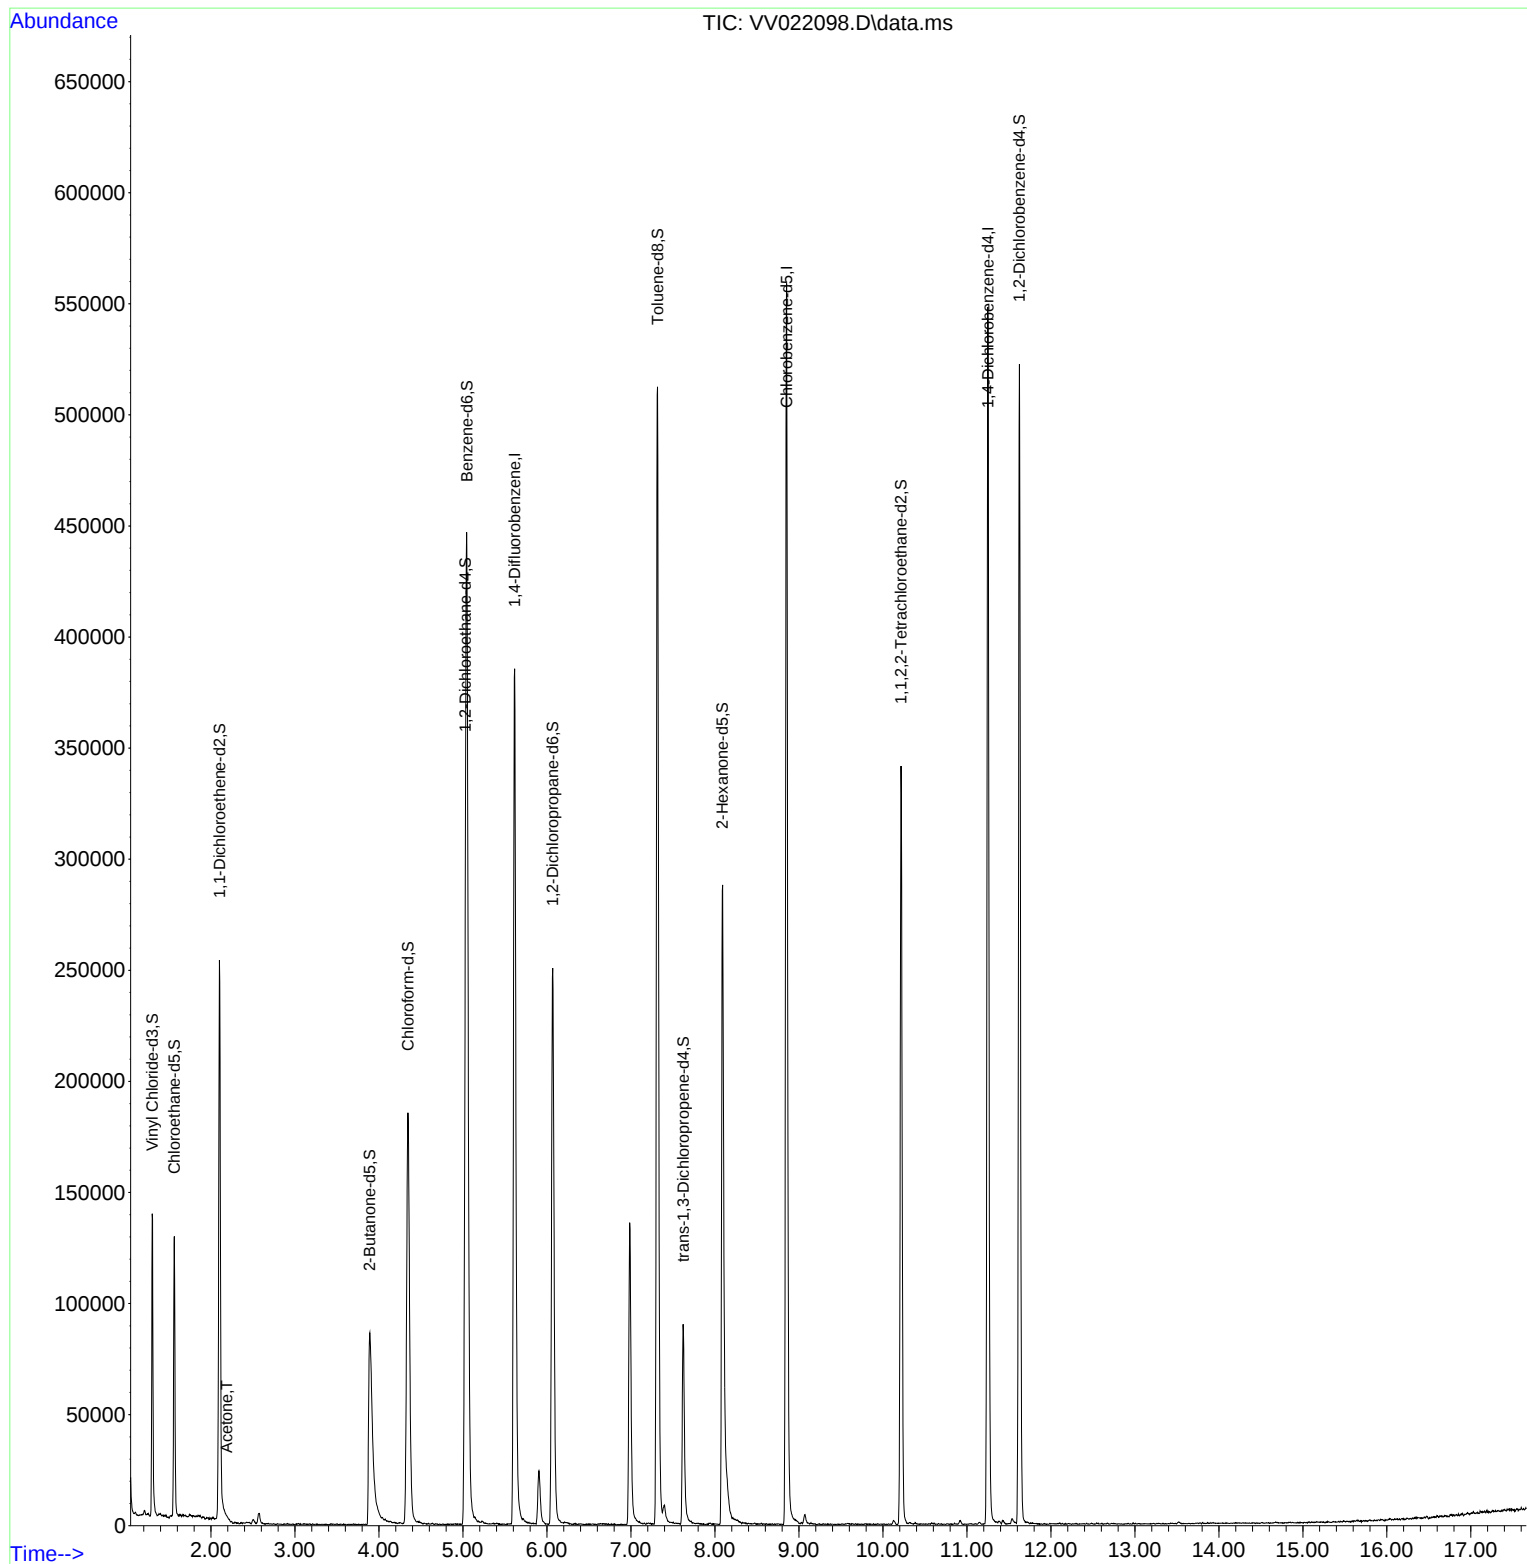

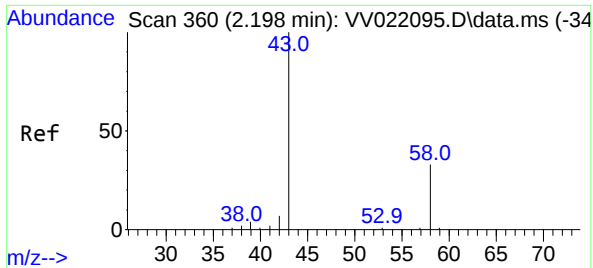

#13
Acetone
Concen: 3.127 ug/L m
RT: 2.185 min Scan# 356
Delta R.T. -0.013 min
Lab File: VV022098.D
Acq: 07 Sep 2021 13:23

Tgt Ion: 43 Resp: 4290
Ion Ratio Lower Upper
43 100
58 17.9 0.0 0.4#

Instrument :
MSVOA_V
ClientSampleId :
DBKL9

Manual Integrations
APPROVED

MMDadoda
9/8/2021 10:17:07 AM

