

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090721\
 Data File : VV022104.D
 Acq On : 07 Sep 2021 15:48
 Operator : SY/MD
 Sample : M3608-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKL3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

Signal : TIC: VV022104.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	103	rVB	121631	128381	11.87%	1.492%
2	1.564	156	163	179	rBV	113571	130595	12.08%	1.518%
3	2.105	322	331	361	rVB	234817	354198	32.76%	4.118%
4	2.320	395	398	403	rBV2	566	519	0.05%	0.006%
5	2.510	450	457	466	rVB6	1639	2690	0.25%	0.031%
6	2.558	470	472	474	rBV2	360	132	0.01%	0.002%
7	2.619	486	491	493	rBV2	357	288	0.03%	0.003%
8	2.748	529	531	532	rBV	341	153	0.01%	0.002%
9	2.773	533	539	541	rBV3	1091	1207	0.11%	0.014%
10	2.847	555	562	566	rBV3	475	639	0.06%	0.007%
11	2.886	570	574	579	rVB3	461	421	0.04%	0.005%
12	2.925	579	586	588	rBV2	329	424	0.04%	0.005%
13	2.944	590	592	595	rVB3	431	178	0.02%	0.002%
14	3.011	610	613	618	rBV2	244	233	0.02%	0.003%
15	3.047	622	624	627	rBV	251	203	0.02%	0.002%
16	3.240	680	684	685	rBV	208	135	0.01%	0.002%
17	3.326	708	711	713	rBV	322	148	0.01%	0.002%
18	3.388	725	730	731	rBV	319	255	0.02%	0.003%
19	3.548	778	780	782	rBV	307	160	0.01%	0.002%
20	3.671	813	818	820	rBV2	254	275	0.03%	0.003%
21	3.735	834	838	841	rVB2	288	243	0.02%	0.003%
22	3.761	841	846	851	rBV	304	301	0.03%	0.003%
23	3.892	877	887	926	rBV	89468	273139	25.26%	3.175%
24	4.278	1005	1007	1011	rBV2	519	434	0.04%	0.005%
25	4.349	1015	1029	1057	rVV	172869	431753	39.93%	5.019%
26	4.584	1100	1102	1108	rVB3	427	377	0.03%	0.004%
27	4.693	1129	1136	1139	rBV2	560	484	0.04%	0.006%
28	4.786	1164	1165	1167	rVB	334	117	0.01%	0.001%
29	4.892	1194	1198	1202	rBV2	278	255	0.02%	0.003%
30	4.908	1202	1203	1207	rVB	247	129	0.01%	0.001%
31	4.934	1207	1211	1214	rBV3	399	286	0.03%	0.003%
32	4.960	1216	1219	1223	rVB	228	174	0.02%	0.002%
33	4.979	1223	1225	1229	rVB2	234	153	0.01%	0.002%
34	5.047	1229	1246	1272	rBV2	425982	1081316	100.00%	12.570%
35	5.310	1326	1328	1330	rBV	610	289	0.03%	0.003%
36	5.384	1348	1351	1353	rVB	245	136	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090721\
 Data File : VV022104.D
 Acq On : 07 Sep 2021 15:48
 Operator : SY/MD
 Sample : M3608-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKL3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

37	5.404	1355	1357	1361	rVV3	460	340	0.03%	0.004%
38	5.442	1364	1369	1370	rBV2	284	195	0.02%	0.002%
39	5.478	1377	1380	1384	rBV3	424	328	0.03%	0.004%
40	5.548	1398	1402	1403	rBV2	955	653	0.06%	0.008%
41	5.619	1412	1424	1454	rBV	376725	767812	71.01%	8.926%
42	5.908	1504	1514	1533	rBV2	17288	36834	3.41%	0.428%
43	6.005	1543	1544	1548	rBV2	304	247	0.02%	0.003%
44	6.072	1551	1565	1595	rBV	243245	498848	46.13%	5.799%
45	6.310	1637	1639	1640	rBV	519	177	0.02%	0.002%
46	6.500	1696	1698	1701	rBV2	286	181	0.02%	0.002%
47	6.574	1719	1721	1724	rBV2	305	138	0.01%	0.002%
48	6.638	1739	1741	1745	rBV2	511	375	0.03%	0.004%
49	6.793	1787	1789	1797	rVB2	318	239	0.02%	0.003%
50	6.822	1797	1798	1802	rBV2	277	190	0.02%	0.002%
51	6.850	1805	1807	1809	rBV	249	155	0.01%	0.002%
52	6.989	1839	1850	1874	rBV	127470	233562	21.60%	2.715%
53	7.169	1904	1906	1909	rVB3	679	316	0.03%	0.004%
54	7.188	1909	1912	1913	rBV2	524	308	0.03%	0.004%
55	7.317	1940	1952	1971	rBV	482954	849233	78.54%	9.872%
56	7.571	2027	2031	2035	rBV4	413	380	0.04%	0.004%
57	7.625	2038	2048	2070	rBV	85459	153271	14.17%	1.782%
58	7.847	2113	2117	2118	rBV	345	220	0.02%	0.003%
59	7.899	2131	2133	2138	rBV3	347	329	0.03%	0.004%
60	7.924	2138	2141	2144	rBV3	336	284	0.03%	0.003%
61	7.982	2156	2159	2162	rBV2	409	251	0.02%	0.003%
62	8.043	2176	2178	2180	rBV2	271	145	0.01%	0.002%
63	8.092	2183	2193	2232	rBV	290685	564548	52.21%	6.563%
64	8.465	2307	2309	2312	rVB	235	113	0.01%	0.001%
65	8.506	2318	2322	2323	rVB2	256	159	0.01%	0.002%
66	8.522	2323	2327	2329	rBV	406	362	0.03%	0.004%
67	8.612	2352	2355	2357	rBV2	313	206	0.02%	0.002%
68	8.744	2393	2396	2397	rBV2	304	144	0.01%	0.002%
69	8.796	2408	2412	2414	rBV2	390	258	0.02%	0.003%
70	8.854	2418	2430	2457	rBV	562672	918438	84.94%	10.677%
71	9.088	2501	2503	2505	rBV2	319	125	0.01%	0.001%
72	9.133	2515	2517	2519	rBV3	392	213	0.02%	0.002%
73	9.210	2537	2541	2542	rBV	483	232	0.02%	0.003%
74	9.297	2565	2568	2569	rBV	368	213	0.02%	0.002%
75	9.432	2606	2610	2612	rBV	222	148	0.01%	0.002%
76	9.474	2621	2623	2626	rVB2	273	120	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090721\
 Data File : VV022104.D
 Acq On : 07 Sep 2021 15:48
 Operator : SY/MD
 Sample : M3608-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKL3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

77	9.545	2642	2645	2646	rBV	286	184	0.02%	0.002%
78	9.979	2776	2780	2784	rBV2	242	205	0.02%	0.002%
79	10.024	2791	2794	2797	rBV2	307	217	0.02%	0.003%
80	10.063	2803	2806	2808	rBV	284	158	0.01%	0.002%
81	10.130	2822	2827	2835	rVB7	1326	1932	0.18%	0.022%
82	10.217	2842	2854	2874	rBV	345221	541988	50.12%	6.301%
83	10.371	2899	2902	2903	rBV	592	313	0.03%	0.004%
84	10.468	2930	2932	2935	rBV2	207	168	0.02%	0.002%
85	10.551	2955	2958	2959	rBV	288	177	0.02%	0.002%
86	10.664	2989	2993	2994	rBV2	326	234	0.02%	0.003%
87	10.886	3058	3062	3063	rBV	284	196	0.02%	0.002%
88	11.043	3107	3111	3112	rBV	441	283	0.03%	0.003%
89	11.124	3133	3136	3138	rBV2	278	208	0.02%	0.002%
90	11.149	3138	3144	3148	rVV3	817	911	0.08%	0.011%
91	11.252	3164	3176	3199	rBV	530215	836922	77.40%	9.729%
92	11.625	3280	3292	3317	rBV	487652	774601	71.64%	9.005%
93	12.191	3464	3468	3475	rBV3	355	513	0.05%	0.006%
94	12.345	3514	3516	3521	rBV	418	304	0.03%	0.004%
95	12.596	3592	3594	3599	rVB2	362	206	0.02%	0.002%
96	12.673	3616	3618	3621	rBV	278	207	0.02%	0.002%
97	12.722	3631	3633	3636	rBV2	239	120	0.01%	0.001%
98	12.747	3636	3641	3643	rBV2	441	421	0.04%	0.005%
99	12.963	3704	3708	3711	rBV2	304	257	0.02%	0.003%
100	13.471	3863	3866	3868	rBV2	294	193	0.02%	0.002%




Sum of corrected areas: 8602028

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090721\
Data File : VV022104.D
Acq On : 07 Sep 2021 15:48
Operator : SY/MD
Sample : M3608-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKL3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

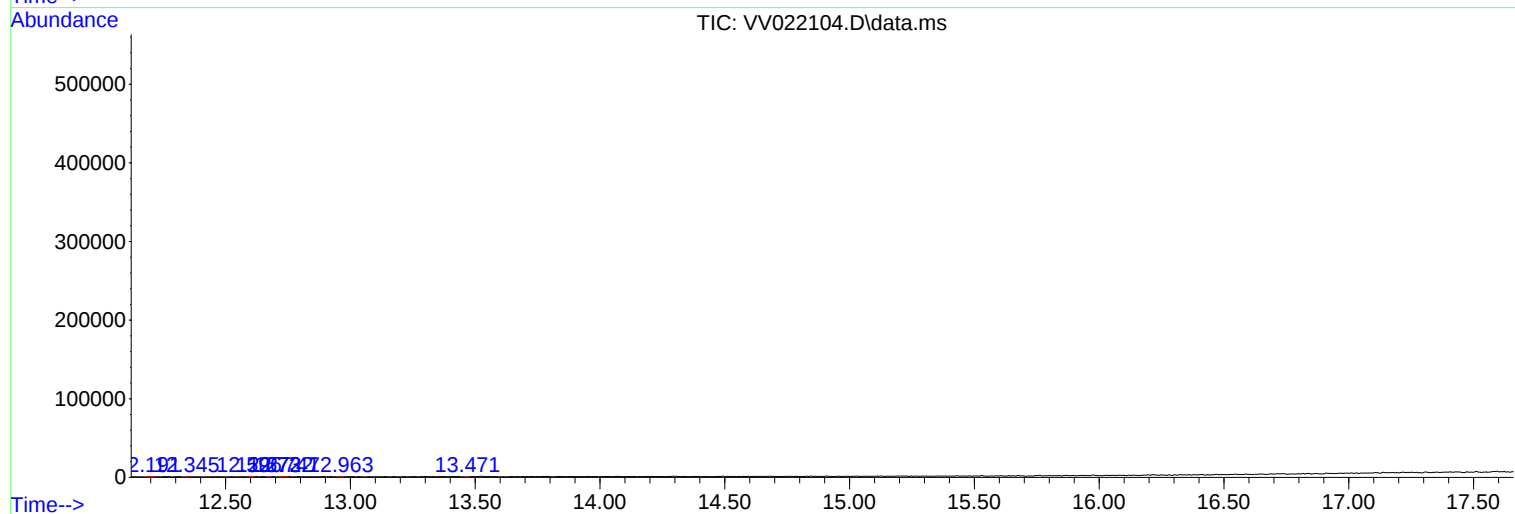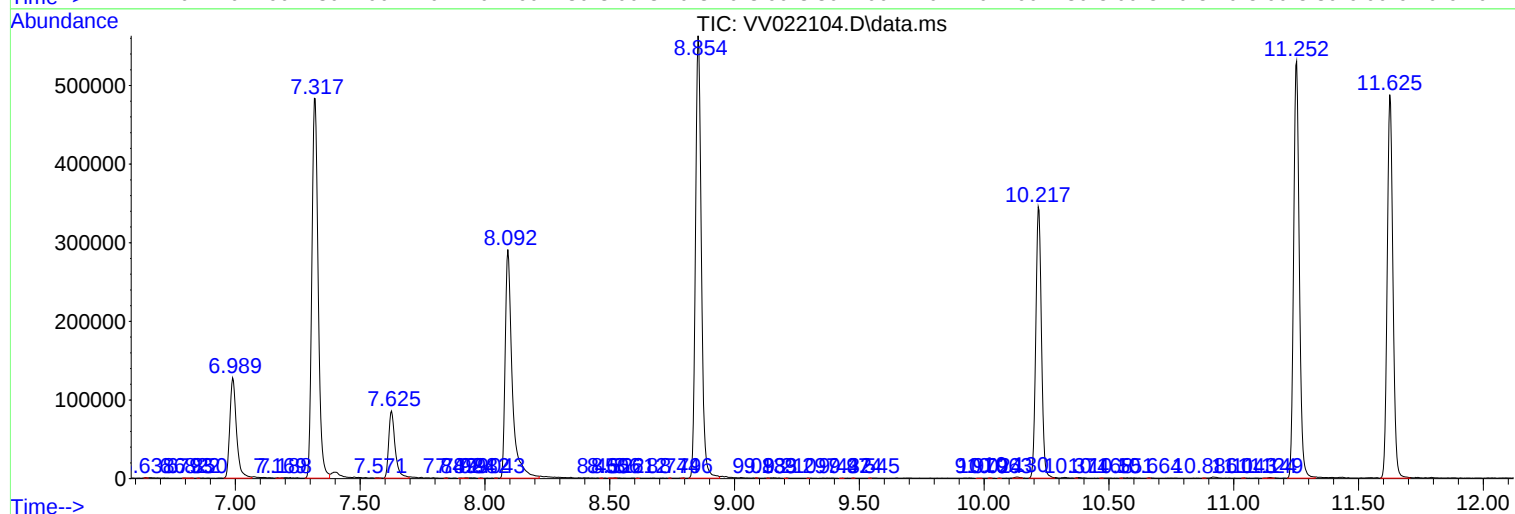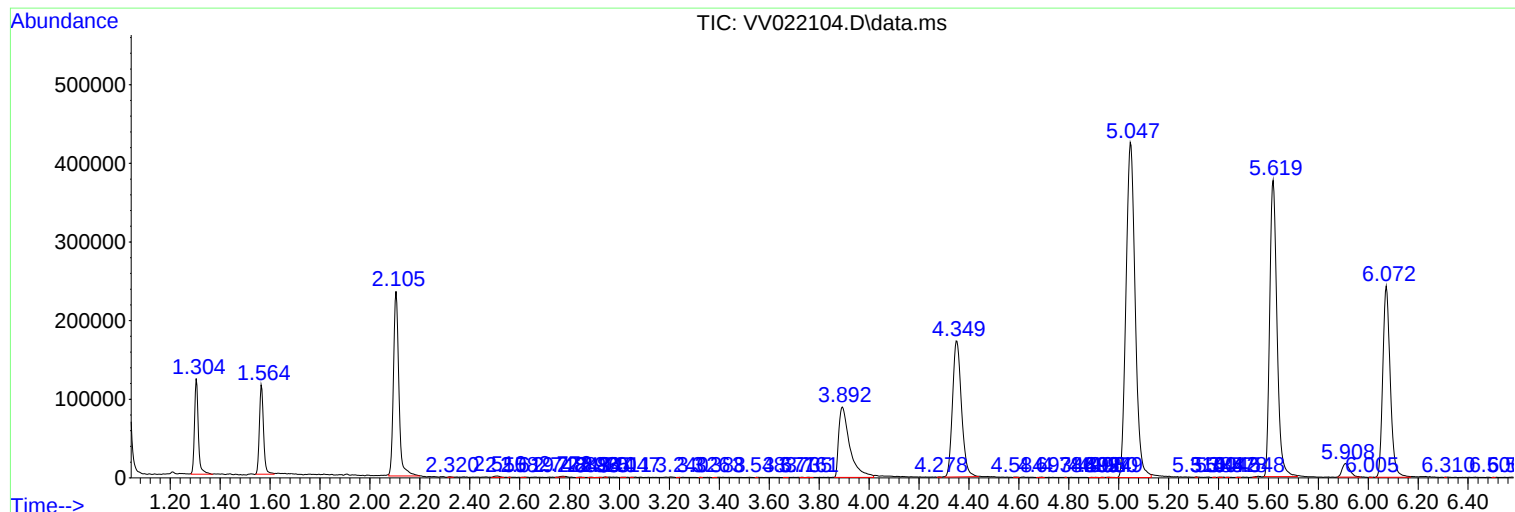

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090721\
Data File : VV022104.D
Acq On : 07 Sep 2021 15:48
Operator : SY/MD
Sample : M3608-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKL3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090721\
Data File : VV022104.D
Acq On : 07 Sep 2021 15:48
Operator : SY/MD
Sample : M3608-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKL3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
