

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090721\
 Data File : VV022113.D
 Acq On : 07 Sep 2021 20:13
 Operator : SY/MD
 Sample : M3651-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKM5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

Signal : TIC: VV022113.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	104	rVB	117773	123502	11.73%	1.478%
2	1.565	156	163	178	rVB	106749	124431	11.82%	1.489%
3	2.105	321	331	344	rBV	222215	321995	30.59%	3.854%
4	2.648	497	500	501	rBV	323	153	0.01%	0.002%
5	2.725	521	524	528	rBV3	562	342	0.03%	0.004%
6	2.770	530	538	551	rVV6	1826	3879	0.37%	0.046%
7	2.909	579	581	584	rVB2	473	222	0.02%	0.003%
8	2.928	584	587	591	rBV2	253	237	0.02%	0.003%
9	2.950	591	594	598	rBV2	362	262	0.02%	0.003%
10	3.031	616	619	622	rBV	250	186	0.02%	0.002%
11	3.050	622	625	626	rBV	284	174	0.02%	0.002%
12	3.150	653	656	658	rBV	349	193	0.02%	0.002%
13	3.256	687	689	692	rVB	308	179	0.02%	0.002%
14	3.343	712	716	718	rBV	334	252	0.02%	0.003%
15	3.378	724	727	730	rBV	232	154	0.01%	0.002%
16	3.577	787	789	793	rVB2	363	138	0.01%	0.002%
17	3.744	836	841	842	rBV	231	144	0.01%	0.002%
18	3.902	879	890	930	rBV2	75397	274134	26.05%	3.281%
19	4.253	995	999	1001	rBV2	569	446	0.04%	0.005%
20	4.352	1013	1030	1062	rBV2	169941	421870	40.08%	5.050%
21	4.670	1127	1129	1130	rBV	440	132	0.01%	0.002%
22	4.793	1165	1167	1171	rVB2	276	141	0.01%	0.002%
23	4.928	1204	1209	1213	rBV3	414	494	0.05%	0.006%
24	4.970	1217	1222	1224	rBV	311	287	0.03%	0.003%
25	5.047	1229	1246	1274	rBV2	415861	1052505	100.00%	12.599%
26	5.310	1327	1328	1331	rVB2	333	131	0.01%	0.002%
27	5.458	1371	1374	1375	rBV2	412	178	0.02%	0.002%
28	5.500	1382	1387	1388	rVV2	541	410	0.04%	0.005%
29	5.551	1398	1403	1406	rVV	320	285	0.03%	0.003%
30	5.619	1412	1424	1450	rBV	368433	746170	70.89%	8.932%
31	5.912	1503	1515	1536	rBV2	16133	34096	3.24%	0.408%
32	5.982	1536	1537	1542	rVB2	479	254	0.02%	0.003%
33	6.018	1545	1548	1550	rBV2	490	229	0.02%	0.003%
34	6.072	1550	1565	1597	rBV	233298	487659	46.33%	5.837%
35	6.297	1631	1635	1638	rVB3	441	341	0.03%	0.004%
36	6.317	1638	1641	1644	rVB2	302	240	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090721\
 Data File : VV022113.D
 Acq On : 07 Sep 2021 20:13
 Operator : SY/MD
 Sample : M3651-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKM5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

37	6.333	1644	1646	1652	rBV2	378	399	0.04%	0.005%
38	6.432	1675	1677	1679	rBV	336	141	0.01%	0.002%
39	6.445	1679	1681	1684	rVB2	322	135	0.01%	0.002%
40	6.484	1690	1693	1699	rVB4	421	412	0.04%	0.005%
41	6.513	1699	1702	1704	rBV	344	183	0.02%	0.002%
42	6.551	1709	1714	1717	rBV3	312	306	0.03%	0.004%
43	6.596	1725	1728	1731	rBV	240	168	0.02%	0.002%
44	6.641	1737	1742	1743	rBV4	513	428	0.04%	0.005%
45	6.712	1758	1764	1767	rBV4	412	416	0.04%	0.005%
46	6.757	1774	1778	1780	rBV	307	148	0.01%	0.002%
47	6.802	1791	1792	1795	rBV2	454	218	0.02%	0.003%
48	6.921	1825	1829	1832	rBV3	205	200	0.02%	0.002%
49	6.989	1837	1850	1875	rBV	119088	221295	21.03%	2.649%
50	7.204	1910	1917	1918	rBV3	631	633	0.06%	0.008%
51	7.243	1927	1929	1934	rVB3	427	385	0.04%	0.005%
52	7.317	1940	1952	1972	rBV	472517	824448	78.33%	9.869%
53	7.625	2038	2048	2070	rBV	80910	143484	13.63%	1.718%
54	7.780	2095	2096	2098	rBV2	276	152	0.01%	0.002%
55	7.802	2101	2103	2105	rBV	273	158	0.02%	0.002%
56	7.870	2121	2124	2128	rVB2	396	278	0.03%	0.003%
57	7.889	2128	2130	2133	rBV	340	201	0.02%	0.002%
58	7.902	2133	2134	2137	rBV	390	189	0.02%	0.002%
59	7.944	2140	2147	2152	rBV3	910	1132	0.11%	0.014%
60	7.982	2156	2159	2161	rBV	374	208	0.02%	0.002%
61	8.092	2183	2193	2234	rBV	287041	565848	53.76%	6.773%
62	8.429	2294	2298	2299	rBV2	458	296	0.03%	0.004%
63	8.510	2321	2323	2326	rVB3	454	256	0.02%	0.003%
64	8.539	2326	2332	2334	rBV3	194	229	0.02%	0.003%
65	8.596	2348	2350	2352	rBV	290	181	0.02%	0.002%
66	8.674	2372	2374	2379	rVB	393	233	0.02%	0.003%
67	8.767	2399	2403	2406	rBV2	298	250	0.02%	0.003%
68	8.854	2418	2430	2456	rBV	553140	885295	84.11%	10.597%
69	9.053	2489	2492	2498	rVB4	767	577	0.05%	0.007%
70	9.137	2516	2518	2519	rBV	603	319	0.03%	0.004%
71	9.207	2533	2540	2543	rBV3	408	466	0.04%	0.006%
72	9.400	2598	2600	2603	rVB2	439	219	0.02%	0.003%
73	9.426	2603	2608	2611	rBV2	310	260	0.02%	0.003%
74	9.487	2622	2627	2628	rBV	208	174	0.02%	0.002%
75	9.731	2700	2703	2705	rBV	204	140	0.01%	0.002%
76	9.834	2732	2735	2737	rBV	266	151	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090721\
 Data File : VV022113.D
 Acq On : 07 Sep 2021 20:13
 Operator : SY/MD
 Sample : M3651-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKM5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

77	10.030	2789	2796	2801	rBV2	458	472	0.04%	0.006%
78	10.072	2805	2809	2813	rBV2	131	146	0.01%	0.002%
79	10.133	2821	2828	2837	rVB4	1755	2480	0.24%	0.030%
80	10.217	2842	2854	2875	rBV	334849	529038	50.26%	6.333%
81	10.387	2905	2907	2911	rVB3	730	352	0.03%	0.004%
82	10.468	2928	2932	2935	rVB2	248	184	0.02%	0.002%
83	10.503	2939	2943	2946	rBV2	514	407	0.04%	0.005%
84	10.535	2951	2953	2959	rVB2	385	251	0.02%	0.003%
85	10.574	2962	2965	2966	rBV2	365	217	0.02%	0.003%
86	10.600	2971	2973	2974	rBV	488	183	0.02%	0.002%
87	10.725	3008	3012	3015	rBV3	429	338	0.03%	0.004%
88	11.005	3097	3099	3104	rVB2	313	183	0.02%	0.002%
89	11.252	3161	3176	3197	rBV	506856	803635	76.35%	9.620%
90	11.471	3242	3244	3252	rVB3	485	412	0.04%	0.005%
91	11.625	3280	3292	3309	rBV	481473	749708	71.23%	8.974%
92	11.860	3364	3365	3368	rBV	375	219	0.02%	0.003%
93	12.088	3432	3436	3440	rBV2	335	338	0.03%	0.004%
94	12.259	3486	3489	3491	rBV2	292	216	0.02%	0.003%
95	12.889	3682	3685	3687	rBV	446	270	0.03%	0.003%
96	12.953	3702	3705	3707	rBV	485	249	0.02%	0.003%
97	13.011	3721	3723	3724	rBV	339	147	0.01%	0.002%
98	13.336	3820	3824	3833	rBV2	602	639	0.06%	0.008%
99	13.509	3865	3878	3888	rBV	10440	16593	1.58%	0.199%
100	13.660	3922	3925	3926	rBV	465	276	0.03%	0.003%




Sum of corrected areas: 8354009

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090721\
Data File : VV022113.D
Acq On : 07 Sep 2021 20:13
Operator : SY/MD
Sample : M3651-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKM5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

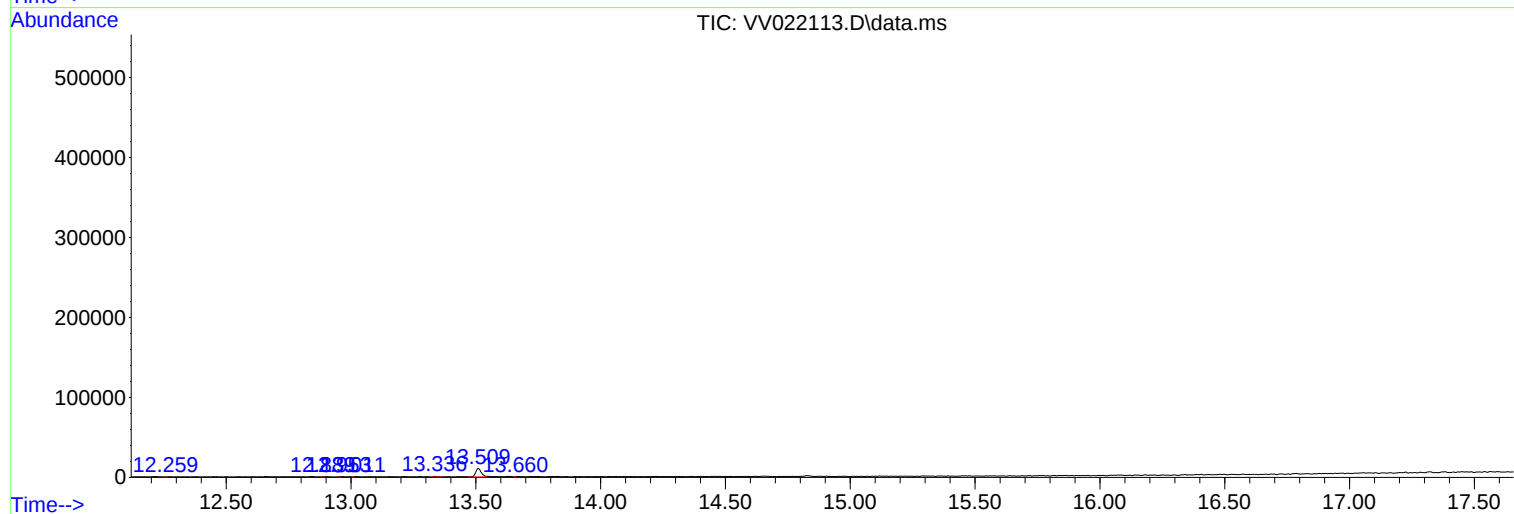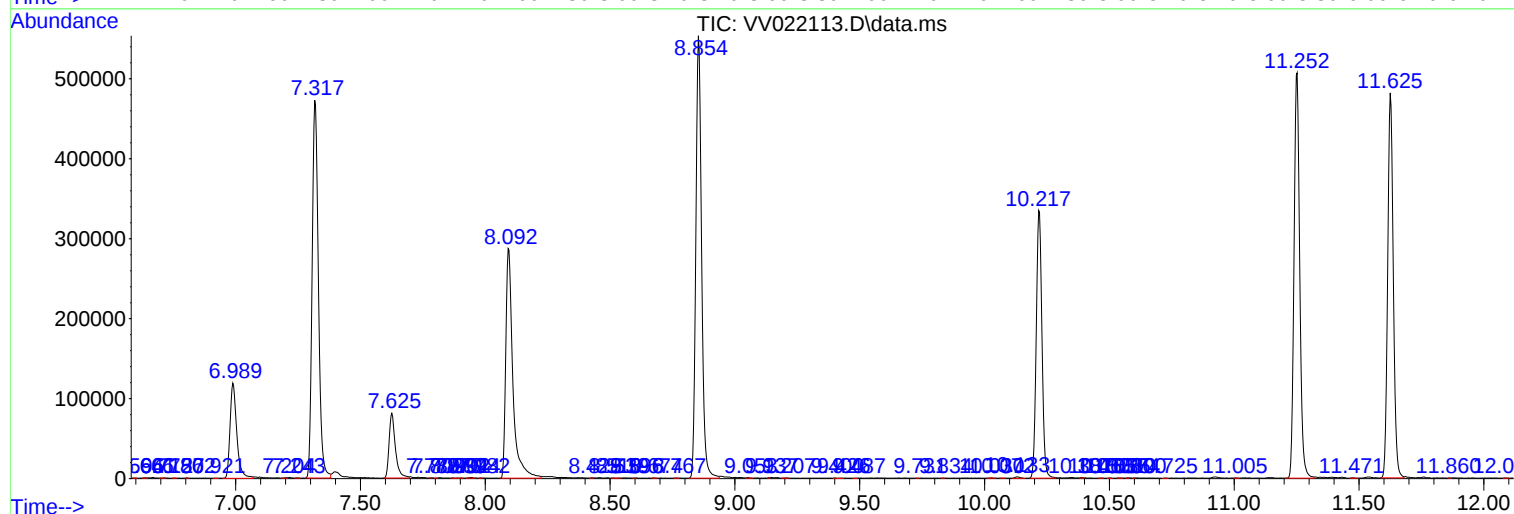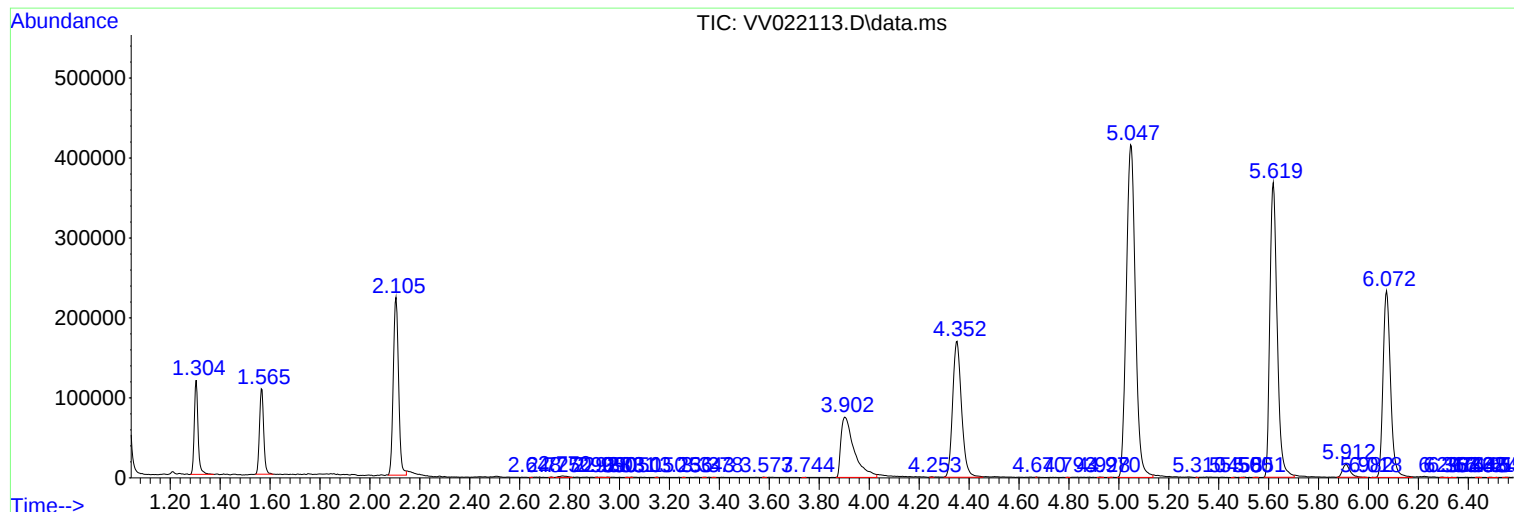

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090721\
Data File : VV022113.D
Acq On : 07 Sep 2021 20:13
Operator : SY/MD
Sample : M3651-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKM5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090721\
Data File : VV022113.D
Acq On : 07 Sep 2021 20:13
Operator : SY/MD
Sample : M3651-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKM5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
