

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090721\
 Data File : VV022115.D
 Acq On : 07 Sep 2021 21:01
 Operator : SY/MD
 Sample : M3651-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKM7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M

Title : VOC Analysis

Signal : TIC: VV022115.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	96	rVB	119704	119156	11.47%	1.452%
2	1.568	156	164	177	rBV	106972	121965	11.74%	1.487%
3	2.105	322	331	347	rBV	216705	312424	30.07%	3.808%
4	2.548	465	469	473	rVV2	618	334	0.03%	0.004%
5	2.568	473	475	479	rVV2	269	184	0.02%	0.002%
6	2.751	528	532	533	rBV2	544	384	0.04%	0.005%
7	2.764	533	536	537	rBV2	1182	673	0.06%	0.008%
8	2.873	568	570	574	rBV2	283	214	0.02%	0.003%
9	2.941	588	591	596	rBV2	256	163	0.02%	0.002%
10	2.960	596	597	600	rBV	234	115	0.01%	0.001%
11	2.989	604	606	608	rBV	263	135	0.01%	0.002%
12	3.037	619	621	624	rVB3	381	205	0.02%	0.002%
13	3.066	627	630	631	rBV	336	169	0.02%	0.002%
14	3.108	641	643	645	rVB	405	150	0.01%	0.002%
15	3.143	651	654	655	rBV	383	160	0.02%	0.002%
16	3.233	676	682	685	rBV2	367	399	0.04%	0.005%
17	3.313	705	707	711	rVB	218	143	0.01%	0.002%
18	3.429	742	743	746	rBV	201	109	0.01%	0.001%
19	3.503	761	766	770	rBV2	257	266	0.03%	0.003%
20	3.577	783	789	791	rBV2	455	350	0.03%	0.004%
21	3.596	791	795	801	rVB2	333	379	0.04%	0.005%
22	3.632	802	806	808	rBV2	245	205	0.02%	0.002%
23	3.712	829	831	836	rVB2	196	120	0.01%	0.001%
24	3.735	836	838	841	rVB2	284	156	0.02%	0.002%
25	3.815	860	863	867	rVB2	387	223	0.02%	0.003%
26	3.841	867	871	876	rBV3	350	358	0.03%	0.004%
27	3.902	880	890	936	rBV2	75138	273592	26.33%	3.335%
28	4.352	1014	1030	1059	rBV	165303	413309	39.77%	5.038%
29	4.702	1134	1139	1144	rBV3	391	437	0.04%	0.005%
30	4.722	1144	1145	1150	rVV3	236	164	0.02%	0.002%
31	4.764	1155	1158	1161	rBV2	344	266	0.03%	0.003%
32	4.892	1196	1198	1200	rBV2	256	121	0.01%	0.001%
33	5.047	1228	1246	1281	rBV2	408799	1039160	100.00%	12.667%
34	5.381	1344	1350	1356	rBV5	441	755	0.07%	0.009%
35	5.468	1375	1377	1379	rBV2	299	141	0.01%	0.002%
36	5.535	1396	1398	1400	rBV2	293	142	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090721\
 Data File : VV022115.D
 Acq On : 07 Sep 2021 21:01
 Operator : SY/MD
 Sample : M3651-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKM7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

37	5.551	1400	1403	1407	rBV2	240	246	0.02%	0.003%
38	5.619	1412	1424	1457	rBV	365054	741324	71.34%	9.037%
39	5.908	1504	1514	1531	rBV3	17071	36139	3.48%	0.441%
40	6.027	1549	1551	1552	rBV	393	175	0.02%	0.002%
41	6.072	1552	1565	1588	rVV	231970	473839	45.60%	5.776%
42	6.284	1628	1631	1635	rBV4	447	259	0.02%	0.003%
43	6.310	1636	1639	1641	rBV2	262	148	0.01%	0.002%
44	6.342	1646	1649	1651	rVV2	253	109	0.01%	0.001%
45	6.387	1659	1663	1666	rVB3	429	365	0.04%	0.004%
46	6.407	1666	1669	1670	rBV	248	122	0.01%	0.001%
47	6.632	1737	1739	1742	rBV3	285	176	0.02%	0.002%
48	6.690	1753	1757	1758	rBV2	352	201	0.02%	0.002%
49	6.738	1770	1772	1778	rVB5	523	381	0.04%	0.005%
50	6.767	1778	1781	1785	rBV	199	155	0.01%	0.002%
51	6.895	1818	1821	1825	rBV3	282	242	0.02%	0.003%
52	6.989	1839	1850	1875	rBV	115251	215705	20.76%	2.629%
53	7.185	1909	1911	1912	rBV2	273	111	0.01%	0.001%
54	7.320	1941	1953	1970	rBV	465946	803380	77.31%	9.793%
55	7.625	2038	2048	2067	rBV	78152	138658	13.34%	1.690%
56	7.763	2087	2091	2095	rVB4	665	591	0.06%	0.007%
57	7.828	2108	2111	2113	rBV2	212	124	0.01%	0.002%
58	7.892	2128	2131	2135	rBV2	484	310	0.03%	0.004%
59	7.921	2135	2140	2141	rBV	223	186	0.02%	0.002%
60	8.027	2171	2173	2175	rBV	208	108	0.01%	0.001%
61	8.050	2178	2180	2183	rBV	216	118	0.01%	0.001%
62	8.095	2183	2194	2234	rBV	281188	557284	53.63%	6.793%
63	8.458	2305	2307	2316	rVB4	564	554	0.05%	0.007%
64	8.580	2342	2345	2346	rBV	244	138	0.01%	0.002%
65	8.661	2364	2370	2377	rVB3	537	690	0.07%	0.008%
66	8.709	2382	2385	2388	rBV	251	154	0.01%	0.002%
67	8.853	2419	2430	2452	rBV	543371	884719	85.14%	10.784%
68	9.053	2490	2492	2495	rBV2	307	162	0.02%	0.002%
69	9.114	2508	2511	2515	rBV2	372	266	0.03%	0.003%
70	9.146	2519	2521	2522	rBV	434	181	0.02%	0.002%
71	9.188	2531	2534	2539	rBV3	395	294	0.03%	0.004%
72	9.413	2601	2604	2606	rBV	175	111	0.01%	0.001%
73	9.603	2661	2663	2667	rBV	165	135	0.01%	0.002%
74	9.654	2677	2679	2682	rVB	350	120	0.01%	0.001%
75	9.738	2702	2705	2708	rBV	277	143	0.01%	0.002%
76	9.770	2713	2715	2718	rBV	214	114	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090721\
 Data File : VV022115.D
 Acq On : 07 Sep 2021 21:01
 Operator : SY/MD
 Sample : M3651-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKM7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

77	9.837	2734	2736	2739	rVB2	388	188	0.02%	0.002%
78	9.853	2739	2741	2743	rBV	230	107	0.01%	0.001%
79	9.918	2759	2761	2765	rVB	362	158	0.02%	0.002%
80	9.995	2781	2785	2787	rBV	347	282	0.03%	0.003%
81	10.130	2816	2827	2829	rBV4	1383	1850	0.18%	0.023%
82	10.217	2842	2854	2876	rBV	326643	521741	50.21%	6.360%
83	10.471	2931	2933	2934	rBV2	426	114	0.01%	0.001%
84	10.570	2962	2964	2966	rBV	370	257	0.02%	0.003%
85	10.599	2969	2973	2974	rBV	245	176	0.02%	0.002%
86	10.705	3002	3006	3009	rBV2	136	137	0.01%	0.002%
87	10.754	3019	3021	3023	rBV2	430	198	0.02%	0.002%
88	10.921	3069	3073	3081	rVB5	1589	1901	0.18%	0.023%
89	11.008	3097	3100	3104	rBV2	277	224	0.02%	0.003%
90	11.252	3164	3176	3204	rVV	505336	797522	76.75%	9.722%
91	11.541	3260	3266	3271	rBV6	1142	1240	0.12%	0.015%
92	11.625	3280	3292	3315	rBV	451398	726792	69.94%	8.859%
93	12.053	3422	3425	3426	rBV	379	213	0.02%	0.003%
94	12.236	3480	3482	3486	rVB2	365	194	0.02%	0.002%
95	12.326	3507	3510	3511	rBV	224	139	0.01%	0.002%
96	12.541	3571	3577	3578	rBV	333	325	0.03%	0.004%
97	12.889	3683	3685	3687	rBV2	361	128	0.01%	0.002%
98	13.246	3791	3796	3799	rBV2	516	434	0.04%	0.005%
99	13.512	3875	3879	3888	rVB3	2723	3426	0.33%	0.042%
100	14.030	4037	4040	4044	rBV3	418	408	0.04%	0.005%


Sum of corrected areas: 8203617

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090721\
Data File : VV022115.D
Acq On : 07 Sep 2021 21:01
Operator : SY/MD
Sample : M3651-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKM7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

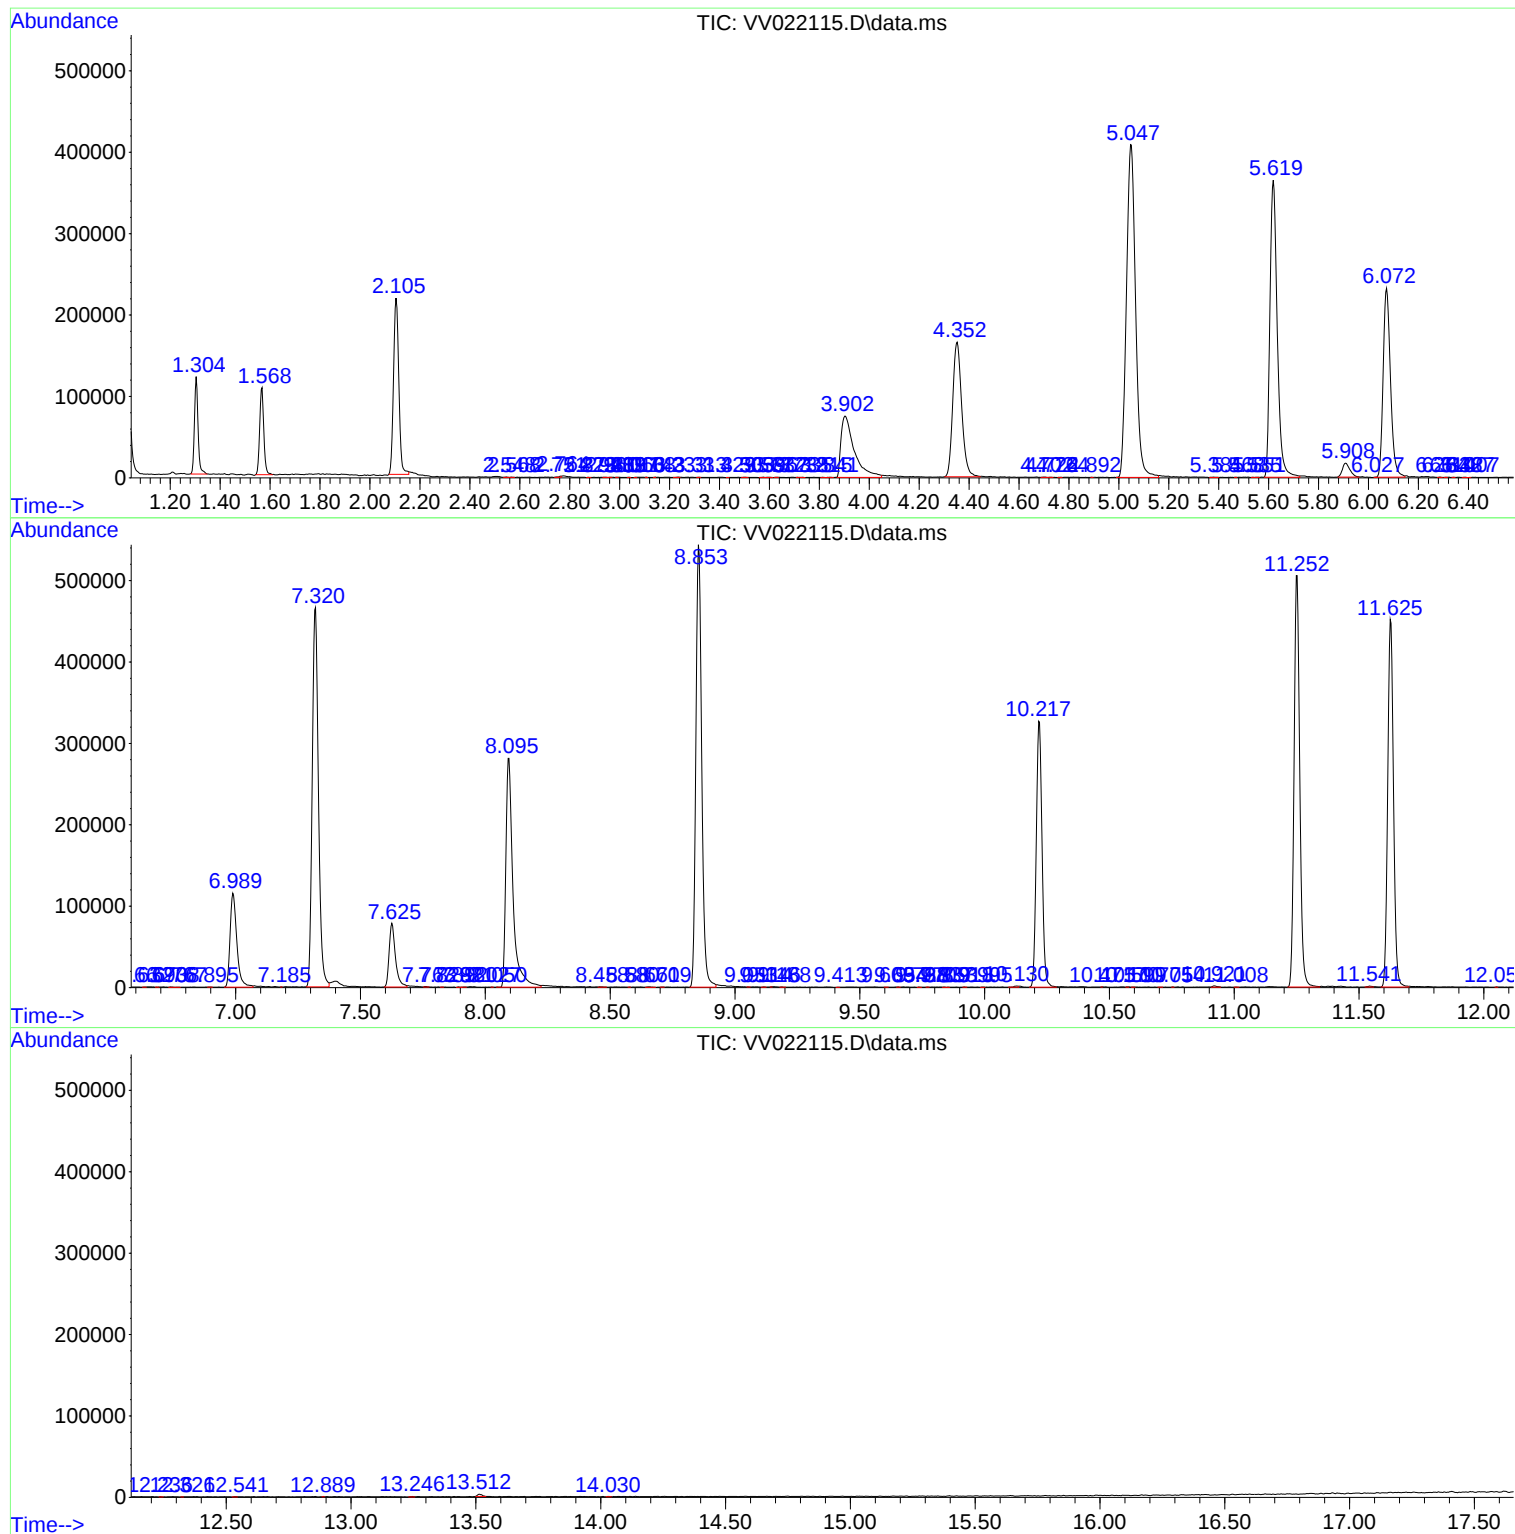

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090721\
Data File : VV022115.D
Acq On : 07 Sep 2021 21:01
Operator : SY/MD
Sample : M3651-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKM7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090721\
Data File : VV022115.D
Acq On : 07 Sep 2021 21:01
Operator : SY/MD
Sample : M3651-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKM7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
