


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090721\
 Data File : VV022094.D
 Acq On : 07 Sep 2021 10:25
 Operator : SY/MD
 Sample : BFB228
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB228

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis
 Last Update : Thu Sep 09 08:27:48 2021

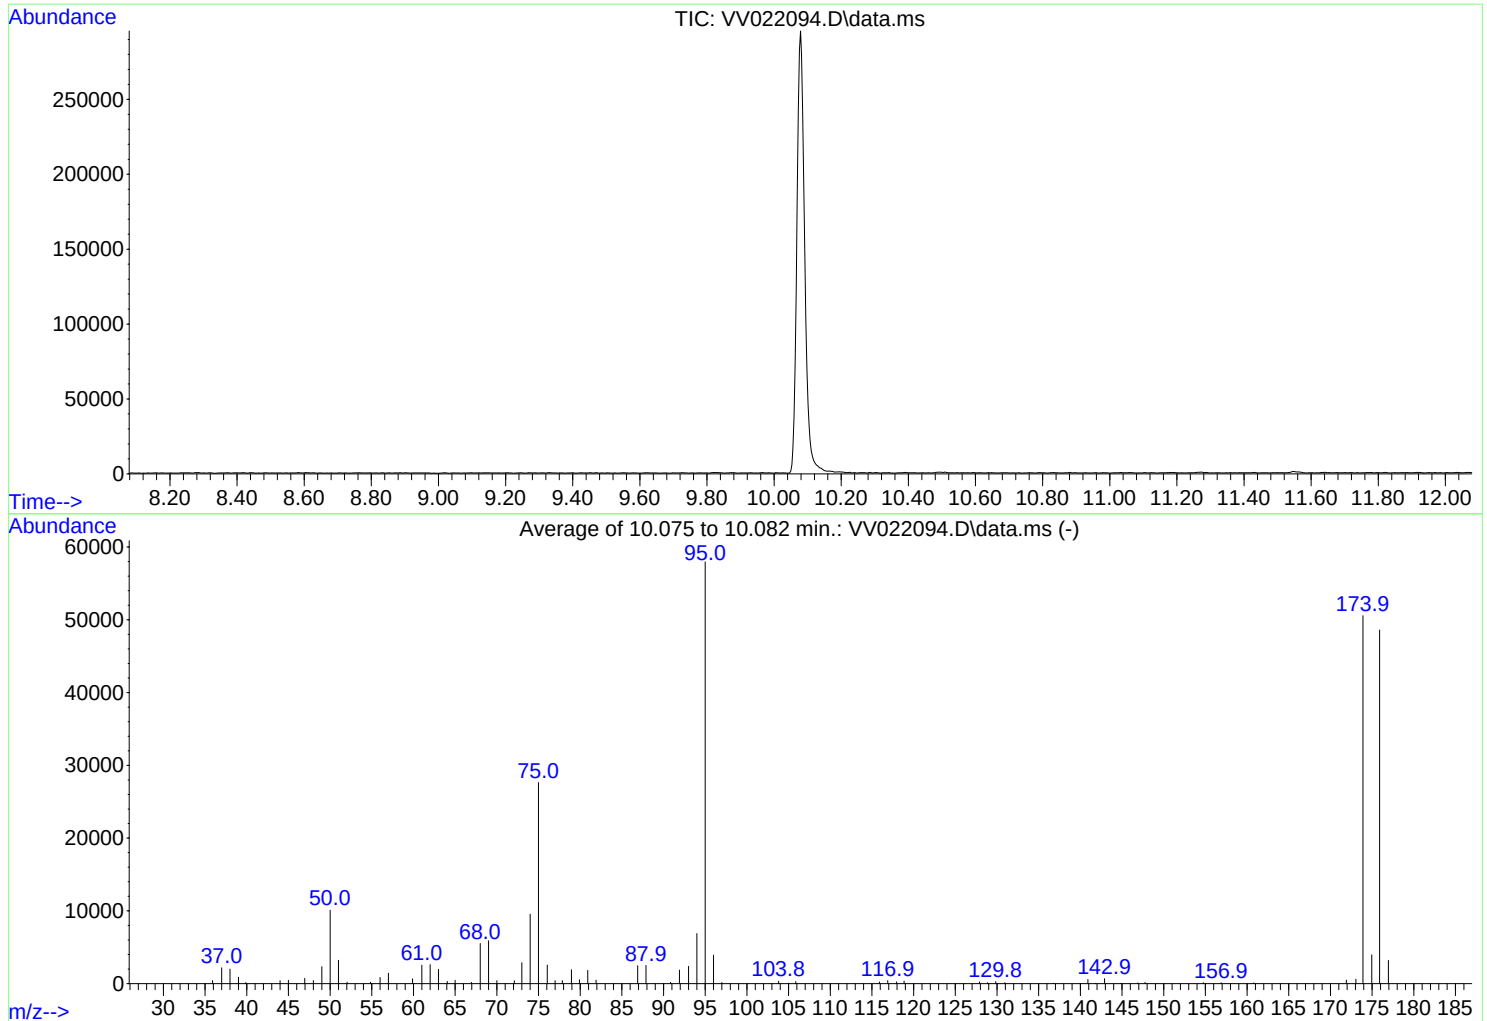

AutoFind: Scans 2810, 2811, 2812; Background Corrected with Scan 2799

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	10097	PASS
75	95	30	80	47.7	27632	PASS
95	95	100	100	100.0	57965	PASS
96	95	5	9	6.8	3918	PASS
173	174	0.00	2	1.2	621	PASS
174	95	50	120	87.2	50568	PASS
175	174	5	9	7.8	3952	PASS
176	174	95	105	96.1	48587	PASS
177	176	5	10	6.5	3181	PASS

m/z	Abundance
39.90	190.0
44.00	337.0

Instrument :
MSVOA_V
ClientSampleId :
BFB228

m/z	Abundance
35.90	394.0
37.00	1964.0
38.00	2014.0
39.00	825.0
40.00	367.0
44.00	720.0
45.00	424.0
47.00	769.0
48.00	374.0
49.00	2240.0
50.00	9677.0
51.00	3023.0
52.00	196.0
54.80	218.0
56.00	800.0
57.00	1370.0
59.90	702.0
61.00	2479.0
62.00	2462.0
63.00	1861.0
64.10	356.0
65.00	399.0
67.00	194.0
68.00	5053.0
69.00	5652.0
70.00	376.0
72.20	400.0
73.00	2685.0
74.00	9258.0
75.00	27016.0
76.00	2228.0
77.00	423.0
77.80	408.0
79.00	1792.0
79.90	512.0
80.90	1769.0
81.90	493.0
86.90	2202.0
87.90	2609.0
90.80	177.0
91.90	1733.0
93.00	2309.0
94.00	6608.0
95.00	56448.0
96.00	3765.0
97.00	148.0
103.80	288.0
105.00	116.0
105.90	282.0
115.90	208.0
116.90	428.0
117.90	211.0
118.90	350.0
127.90	240.0
128.80	116.0
129.80	299.0
130.90	144.0
141.00	590.0
142.90	670.0
144.80	108.0
146.90	114.0
147.70	188.0
154.70	141.0
157.00	117.0
160.80	107.0
171.90	484.0
173.10	646.0
173.90	50736.0
175.00	3981.0
175.90	48304.0
177.00	3145.0

Instrument :
MSVOA_V
ClientSampleId :
BFB228

m/z	Abundance
35.90	424.0
37.00	2233.0
38.00	2031.0
39.00	894.0
40.00	363.0
44.00	749.0
45.00	482.0
46.90	750.0
48.00	450.0
49.00	2398.0
50.00	10562.0
51.00	3314.0
52.10	202.0
54.90	218.0
56.00	850.0
57.00	1480.0
59.90	673.0
61.00	2607.0
62.00	2690.0
63.00	2026.0
64.00	311.0
65.00	502.0
66.90	189.0
68.00	5686.0
69.00	6064.0
70.00	431.0
72.10	424.0
73.00	3025.0
74.00	9831.0
75.00	28424.0
76.00	2669.0
77.00	424.0
77.80	435.0
78.90	1964.0
79.90	547.0
80.90	1859.0
81.90	495.0
86.90	2548.0
87.90	2598.0
90.90	183.0
91.90	1935.0
93.00	2428.0
94.00	7090.0
95.00	60008.0
96.00	4064.0
97.00	141.0
103.80	338.0
105.00	104.0
105.80	305.0
115.90	214.0
116.90	423.0
117.90	262.0
118.90	342.0
127.90	259.0
128.90	136.0
129.80	326.0
131.00	132.0
136.80	102.0
140.90	587.0
142.90	695.0
146.90	126.0
147.70	174.0
154.70	132.0
156.90	142.0
160.80	124.0
171.90	489.0
173.10	638.0
173.90	52368.0
174.90	4054.0
175.90	50168.0
176.90	3306.0

Instrument :
MSVOA_V
ClientSampleId :
BFB228

m/z	Abundance
35.90	433.0
37.00	2355.0
38.00	1950.0
39.00	927.0
39.90	287.0
44.00	766.0
45.00	472.0
46.90	686.0
48.00	457.0
49.00	2330.0
50.00	10051.0
51.00	3295.0
52.10	196.0
54.90	180.0
56.00	827.0
57.00	1439.0
59.90	575.0
61.00	2491.0
62.00	2687.0
63.00	2001.0
64.10	262.0
65.00	509.0
66.90	173.0
68.00	5819.0
69.00	5981.0
70.00	459.0
72.00	398.0
73.00	2945.0
74.00	9513.0
75.00	27456.0
76.10	2768.0
77.00	394.0
77.90	396.0
78.90	2003.0
79.90	536.0
80.90	1823.0
81.90	466.0
86.90	2671.0
87.90	2312.0
90.90	171.0
91.90	1969.0
93.00	2391.0
94.00	6931.0
95.00	57440.0
96.00	3925.0
97.00	152.0
103.80	336.0
105.90	261.0
115.90	226.0
116.90	386.0
118.00	270.0
118.80	354.0
127.90	218.0
128.90	138.0
129.90	259.0
131.00	106.0
136.70	113.0
140.80	571.0
141.80	103.0
142.90	702.0
146.90	111.0
147.90	146.0
154.80	130.0
156.80	153.0
160.80	108.0
171.90	479.0
173.00	579.0
173.90	48600.0
175.00	3822.0
175.90	47288.0
176.90	3093.0

Instrument :
MSVOA_V
ClientSampleId :
BFB228