

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090722\
 Data File : VV027777.D
 Acq On : 07 Sep 2022 13:10
 Operator : SY/MD
 Sample : N4418-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027777.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	101	rVB	65168	73254	15.16%	1.946%
2	1.567	156	164	179	rVB	62223	75842	15.70%	2.015%
3	2.108	322	332	347	rBV	141959	209617	43.38%	5.569%
4	2.506	447	456	468	rBV3	6177	10291	2.13%	0.273%
5	2.767	528	537	550	rBV5	3740	6635	1.37%	0.176%
6	3.902	878	890	905	rBV	22462	68751	14.23%	1.827%
7	4.349	1015	1029	1054	rVB	88312	224743	46.51%	5.971%
8	4.677	1123	1131	1143	rVB7	2395	5474	1.13%	0.145%
9	5.046	1230	1246	1284	rBV3	184000	483202	100.00%	12.837%
10	5.616	1412	1423	1451	rBV	151893	312110	64.59%	8.292%
11	5.918	1506	1517	1530	rBV8	4267	9694	2.01%	0.258%
12	6.069	1548	1564	1580	rBV	109901	229494	47.49%	6.097%
13	6.989	1838	1850	1876	rBV2	43278	87612	18.13%	2.328%
14	7.316	1940	1952	1971	rBV	202284	364100	75.35%	9.673%
15	7.397	1973	1977	1991	rVB4	4974	9162	1.90%	0.243%
16	7.625	2038	2048	2072	rBV2	25137	50395	10.43%	1.339%
17	7.982	2150	2159	2171	rVB4	3820	6723	1.39%	0.179%
18	8.091	2183	2193	2227	rBV	124707	335283	69.39%	8.908%
19	8.850	2418	2429	2459	rBV	230231	395903	81.93%	10.518%
20	9.021	2472	2482	2490	rBV2	4508	6934	1.44%	0.184%
21	9.146	2513	2521	2530	rBV5	3938	6064	1.25%	0.161%
22	9.551	2637	2647	2652	rBV3	4216	7306	1.51%	0.194%
23	9.934	2757	2766	2782	rBV3	3991	6727	1.39%	0.179%
24	10.217	2842	2854	2869	rBV2	67669	111505	23.08%	2.962%
25	10.541	2947	2955	2968	rBV4	4970	6602	1.37%	0.175%
26	10.921	3064	3073	3079	rBV4	4439	5721	1.18%	0.152%
27	11.249	3164	3175	3197	rVV	219822	350354	72.51%	9.308%
28	11.622	3280	3291	3314	rBV	185812	304539	63.03%	8.091%




Sum of corrected areas: 3764037

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090722\
Data File : VV027777.D
Acq On : 07 Sep 2022 13:10
Operator : SY/MD
Sample : N4418-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library :
TIC Integration Parameters: rteint.p

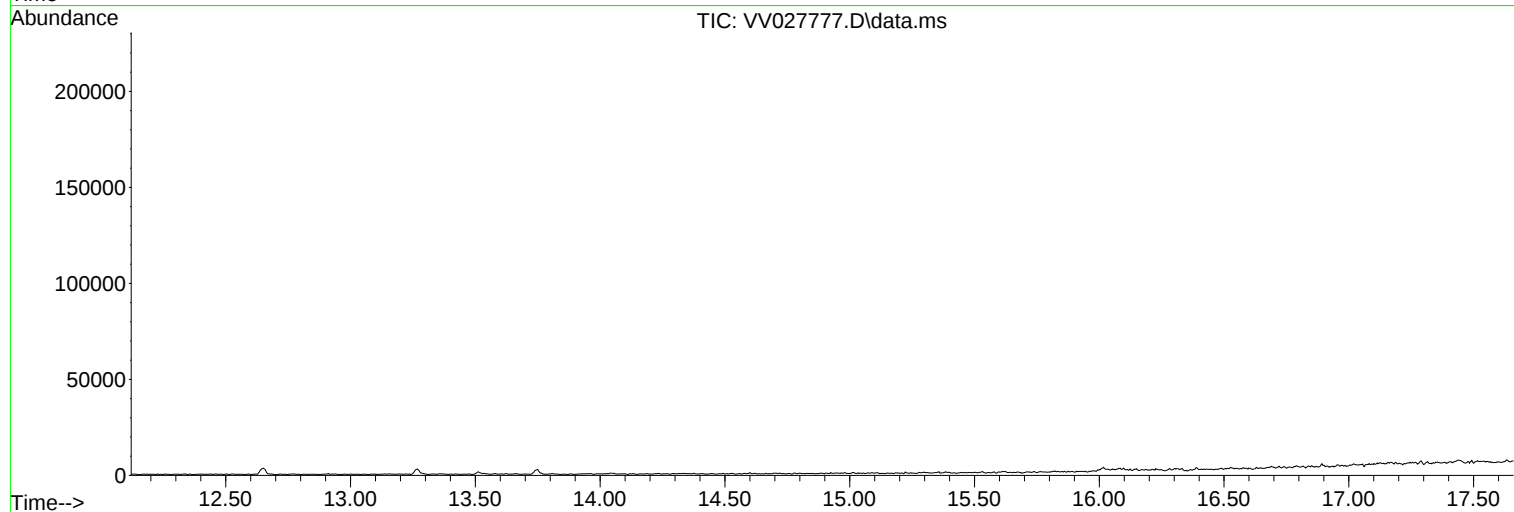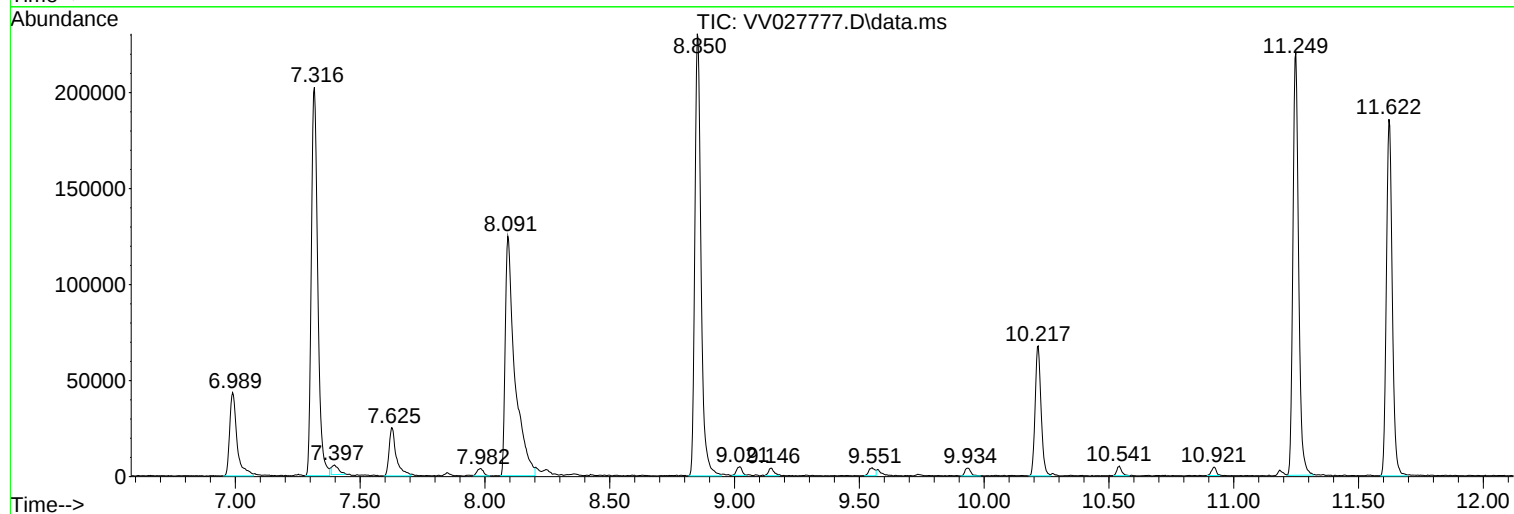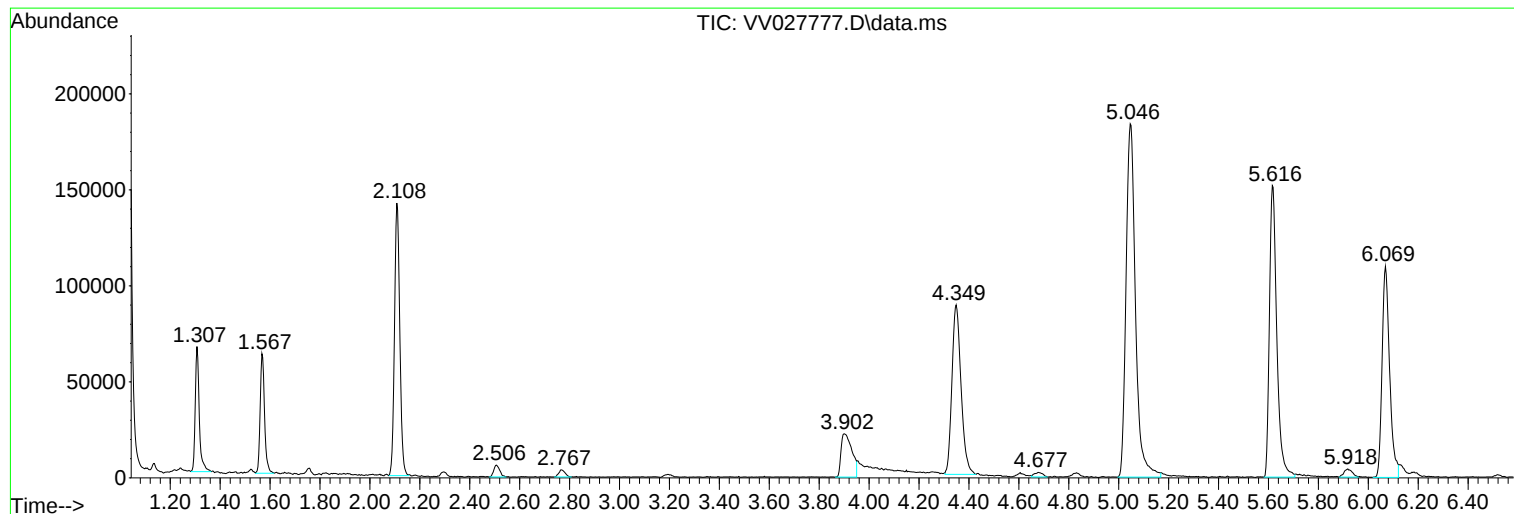

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090722\
Data File : VV027777.D
Acq On : 07 Sep 2022 13:10
Operator : SY/MD
Sample : N4418-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090722\
Data File : VV027777.D
Acq On : 07 Sep 2022 13:10
Operator : SY/MD
Sample : N4418-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc