
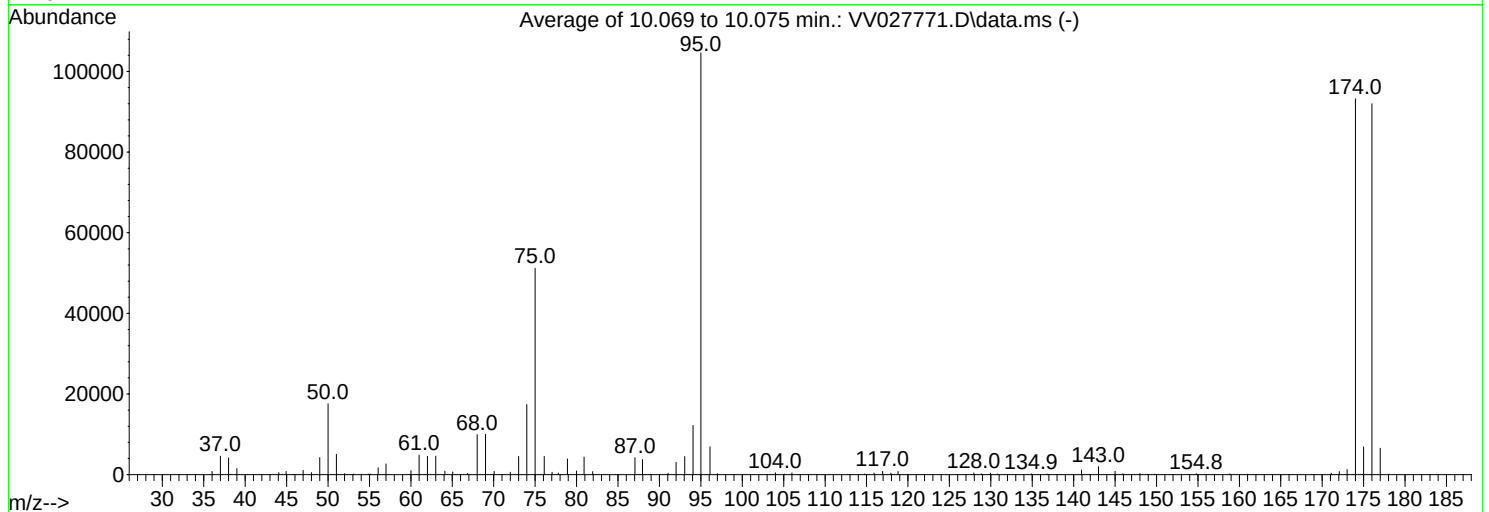


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090722\
 Data File : VV027771.D
 Acq On : 07 Sep 2022 09:57
 Operator : SY/MD
 Sample : BFB367
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB368

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR090622WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Wed Sep 07 06:13:02 2022

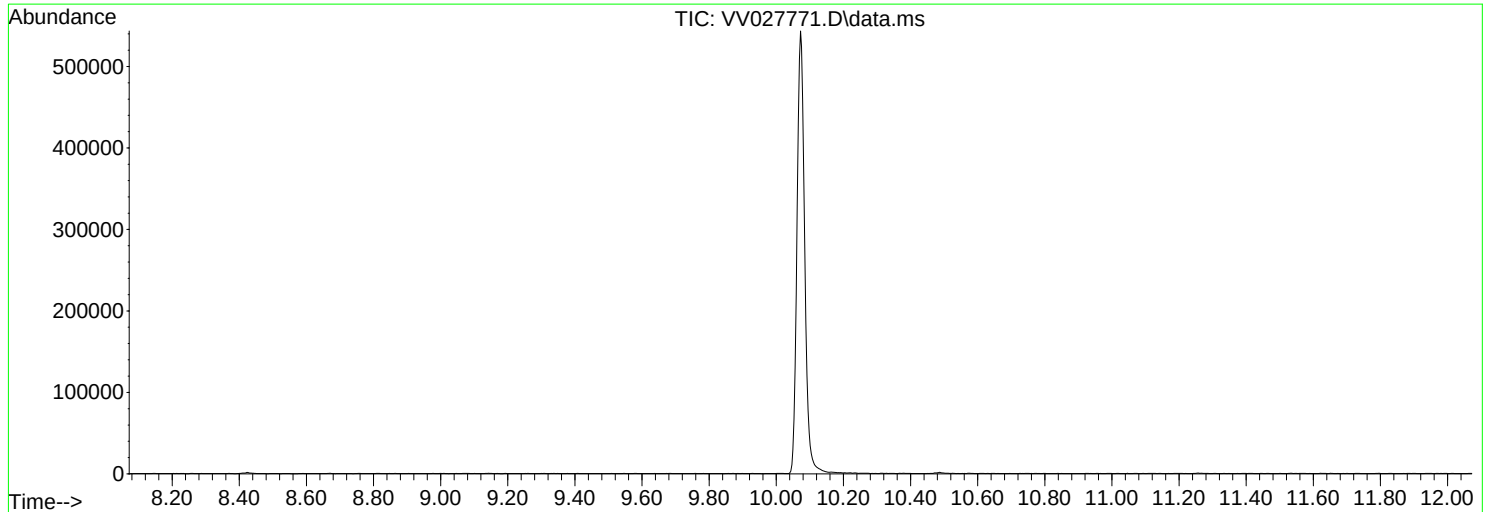

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	17576	PASS
75	95	30	80	48.9	51184	PASS
95	95	100	100	100.0	104621	PASS
96	95	5	9	6.6	6896	PASS
173	174	0.00	2	1.3	1255	PASS
174	95	50	120	89.1	93227	PASS
175	174	5	9	7.4	6869	PASS
176	174	95	105	98.7	91981	PASS
177	176	5	10	7.1	6553	PASS

m/z	Abundance
39.90	304.0
44.00	183.0

Instrument :
MSVOA_V
ClientSampleId :
BFB368

m/z	Abundance
36.00	764.0
37.00	4333.0
38.00	3930.0
39.00	1473.0
40.20	305.0
44.10	727.0
45.00	802.0
45.80	123.0
47.00	1043.0
48.00	467.0
49.00	4243.0
50.00	17352.0
51.00	5077.0
52.00	252.0
53.20	132.0
54.10	108.0
55.20	286.0
56.10	1542.0
57.00	2470.0
58.00	111.0
60.00	982.0
61.00	4589.0
62.00	4429.0
63.00	4632.0
64.10	915.0
65.00	645.0
66.80	325.0
68.00	9276.0
69.00	9696.0
70.10	817.0
72.00	518.0
73.00	4432.0
74.00	16968.0
75.00	50408.0
76.10	4437.0
77.10	581.0
77.80	373.0
78.90	3671.0
80.00	952.0
80.90	4162.0
81.90	687.0
86.00	105.0
87.00	4267.0
87.90	3675.0
88.90	159.0
91.10	408.0
92.00	2877.0
93.00	4235.0
94.10	11969.0
95.00	102960.0
96.10	6657.0
97.00	247.0
103.90	481.0
105.10	133.0
106.10	439.0
114.80	160.0
115.90	374.0
117.00	777.0
117.90	376.0
118.80	754.0
128.10	360.0
128.90	213.0
129.90	343.0
130.80	162.0
134.80	212.0
136.80	181.0
140.90	1068.0
143.00	1909.0
145.00	798.0
146.00	222.0
148.00	260.0
148.90	122.0
149.80	121.0
153.00	171.0
154.80	195.0
157.00	129.0
158.90	170.0
160.70	129.0
171.10	363.0
172.00	663.0
173.00	1166.0
174.00	89248.0
175.00	6719.0
176.00	87784.0
177.00	6238.0
178.10	131.0

Instrument :
MSVOA_V
ClientSampleId :
BFB368

m/z	Abundance
36.00	826.0
37.00	4756.0
38.00	4302.0
39.00	1520.0
39.90	303.0
44.10	718.0
45.00	801.0
45.80	115.0
47.00	1121.0
48.00	512.0
49.00	4400.0
50.00	18144.0
51.00	5209.0
52.00	229.0
53.10	145.0
54.00	141.0
54.80	235.0
55.10	226.0
56.10	1767.0
57.00	2795.0
60.00	1043.0
61.00	5002.0
62.00	4650.0
63.00	4797.0
64.10	883.0
65.10	691.0
66.80	333.0
68.00	10290.0
69.00	10336.0
70.10	833.0
72.00	627.0
73.00	4639.0
74.00	18056.0
75.00	53024.0
76.10	4694.0
77.10	626.0
77.80	425.0
78.90	3956.0
80.00	936.0
80.90	4526.0
82.00	746.0
87.00	4292.0
87.90	3890.0
88.90	159.0
91.10	407.0
92.00	3175.0
93.10	4607.0
94.00	12606.0
95.00	107864.0
96.10	7144.0
97.00	248.0
104.00	477.0
105.00	175.0
106.00	449.0
114.80	166.0
115.90	425.0
116.90	850.0
117.90	429.0
118.80	803.0
127.90	441.0
128.80	214.0
130.00	419.0
130.80	160.0
134.90	215.0
136.80	193.0
141.00	1144.0
141.90	112.0
143.00	2103.0
143.90	110.0
145.00	868.0
146.00	234.0
148.00	254.0
148.90	104.0
149.80	143.0
153.00	148.0
153.80	128.0
154.80	239.0
156.70	113.0
157.10	142.0
158.80	184.0
161.00	158.0
171.10	348.0
172.00	768.0
173.00	1248.0
174.00	96488.0
175.00	7102.0
176.00	95224.0
177.00	6871.0
178.00	158.0

Instrument :
MSVOA_V
ClientSampleId :
BFB368

m/z	Abundance
36.00	771.0
37.00	4590.0
38.00	4313.0
39.00	1484.0
40.00	291.0
44.10	613.0
44.90	743.0
47.00	1012.0
48.00	576.0
49.00	4068.0
50.00	17232.0
51.00	4876.0
52.00	198.0
53.00	180.0
54.00	164.0
54.90	233.0
56.00	1794.0
57.00	2687.0
60.00	1018.0
61.00	4951.0
62.00	4496.0
63.00	4385.0
64.10	821.0
65.10	661.0
66.00	101.0
66.90	291.0
68.00	10214.0
69.00	10022.0
70.00	797.0
72.00	646.0
73.00	4486.0
74.00	17176.0
75.00	50120.0
76.10	4491.0
77.00	574.0
77.80	457.0
78.90	4016.0
80.00	850.0
80.90	4383.0
81.90	777.0
83.00	104.0
87.10	4043.0
88.00	3723.0
90.90	381.0
92.00	3136.0
93.10	4563.0
94.00	12105.0
95.00	103040.0
96.10	6886.0
97.00	223.0
104.10	425.0
105.00	193.0
105.90	438.0
106.80	103.0
114.80	152.0
115.90	523.0
117.00	871.0
118.00	437.0
118.80	797.0
127.90	489.0
128.80	204.0
129.90	448.0
130.80	163.0
135.00	206.0
136.80	159.0
141.00	1197.0
141.90	119.0
143.00	1994.0
143.90	102.0
145.00	833.0
145.90	203.0
148.00	278.0
148.90	110.0
149.80	136.0
153.00	112.0
153.80	135.0
154.80	269.0
157.00	126.0
158.80	197.0
161.00	176.0
171.10	316.0
172.10	848.0
173.00	1352.0
174.00	93944.0
175.00	6787.0
176.00	92936.0
177.00	6551.0
178.00	190.0

Instrument :
MSVOA_V
ClientSampleId :
BFB368