

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090821\
 Data File : VV022120.D
 Acq On : 08 Sep 2021 11:31
 Operator : SY/MD
 Sample : VV0908WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK252

Quant Time: Sep 09 08:28:22 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Sep 09 08:27:48 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	324790	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	303279	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	140363	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	125426	55.764	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	111.520%
7) Chloroethane-d5	1.561	69	101655	57.875	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	115.740%
11) 1,1-Dichloroethene-d2	2.105	63	173070	46.527	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	93.060%
21) 2-Butanone-d5	3.873	46	168681	109.352	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	109.350%
24) Chloroform-d	4.346	84	225203	54.911	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	109.820%
26) 1,2-Dichloroethane-d4	5.027	65	140366	58.106	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	116.220%
32) Benzene-d6	5.047	84	474410	57.672	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	115.340%
36) 1,2-Dichloropropane-d6	6.069	67	146692	56.705	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	113.400%
41) Toluene-d8	7.317	98	425886	54.846	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	109.700%
43) trans-1,3-Dichloroprop...	7.622	79	62513	50.771	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	101.540%
47) 2-Hexanone-d5	8.088	63	103581	104.352	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	104.350%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	178235	53.796	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	107.600%
66) 1,2-Dichlorobenzene-d4	11.625	152	159693	57.873	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	115.740%
Target Compounds						
16) Methylene chloride	2.507	84	2756	1.098	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090821\
Data File : VV022120.D
Acq On : 08 Sep 2021 11:31
Operator : SY/MD
Sample : VV0908WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK252


Quant Time: Sep 09 08:28:22 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Sep 09 08:27:48 2021
Response via : Initial Calibration

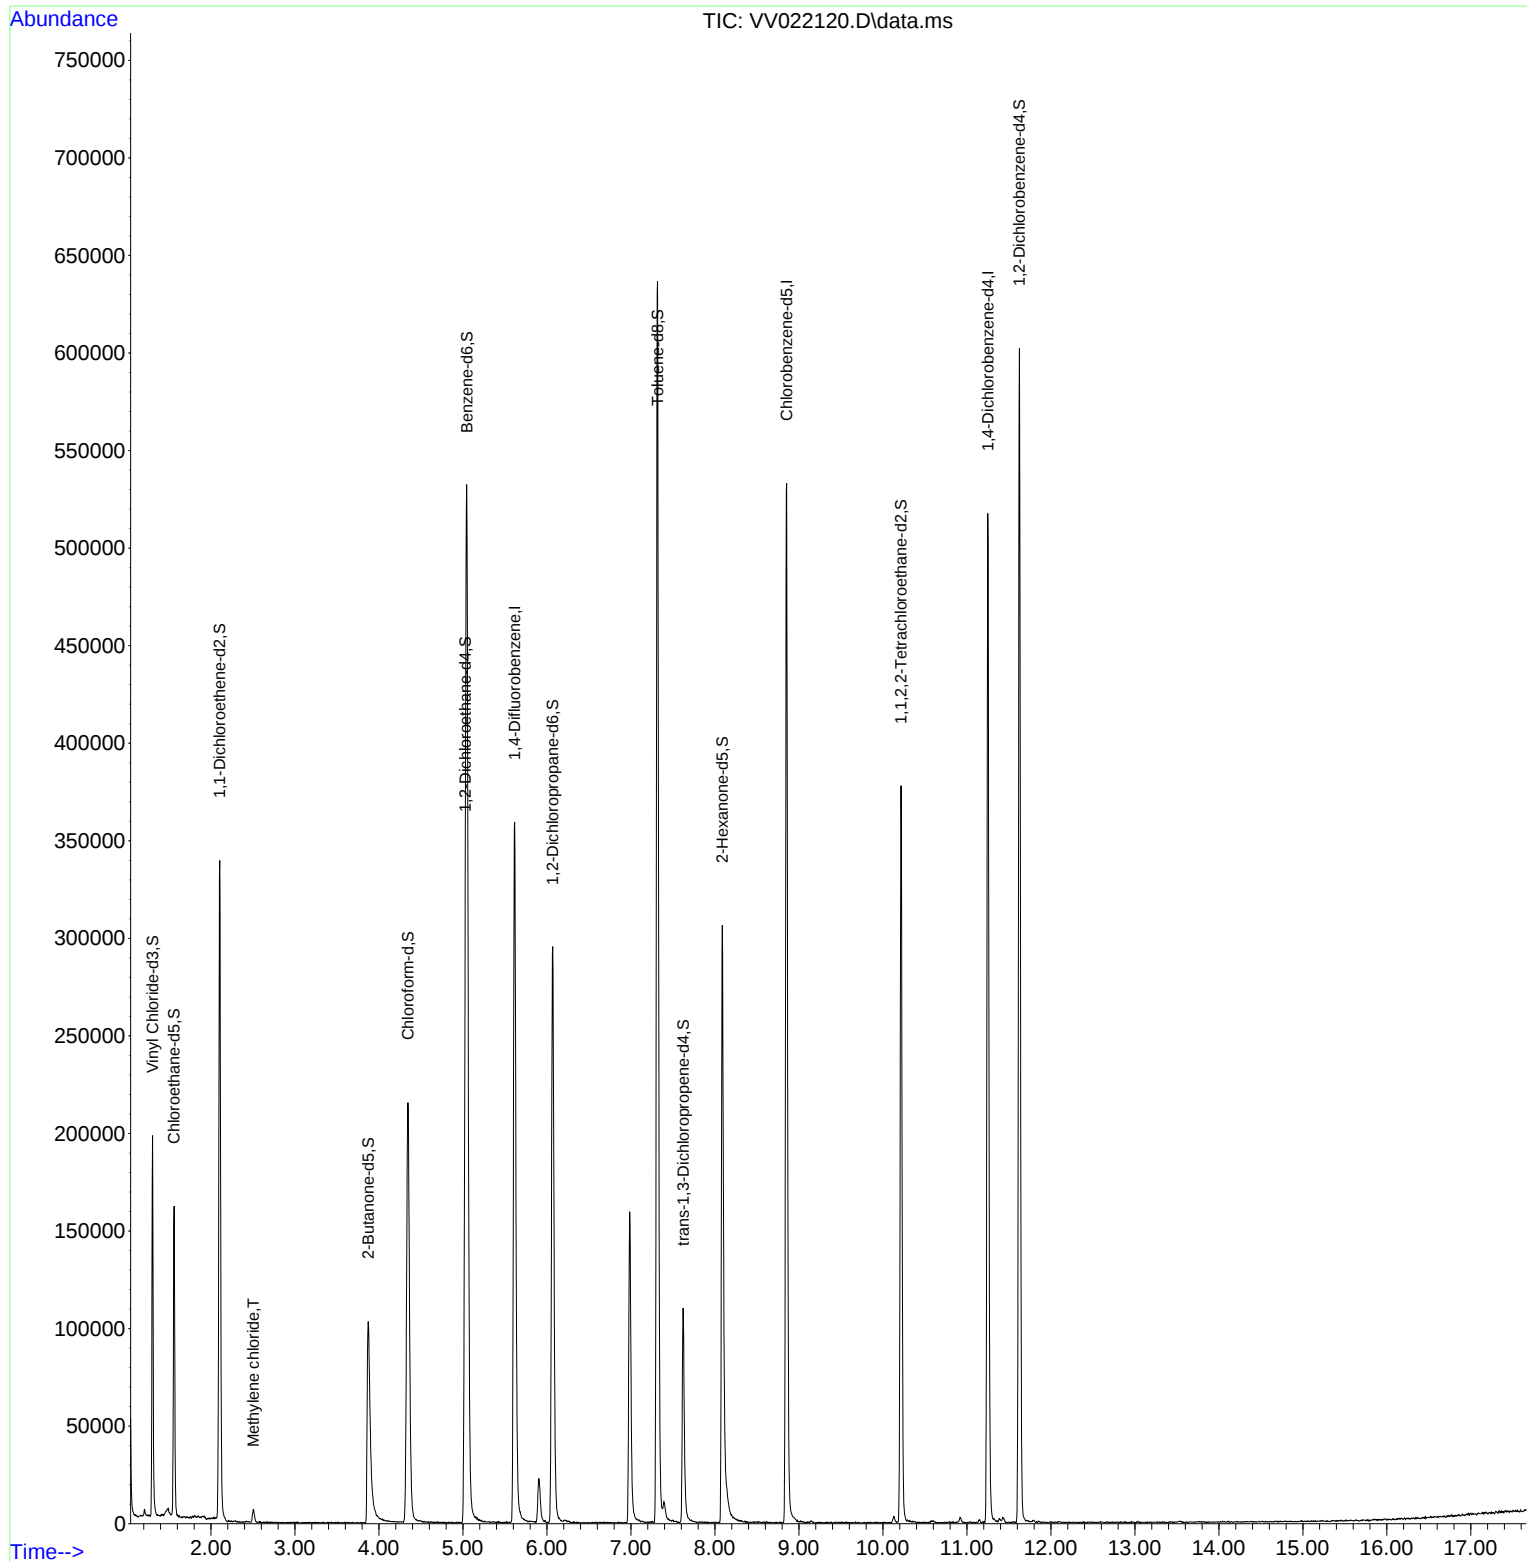

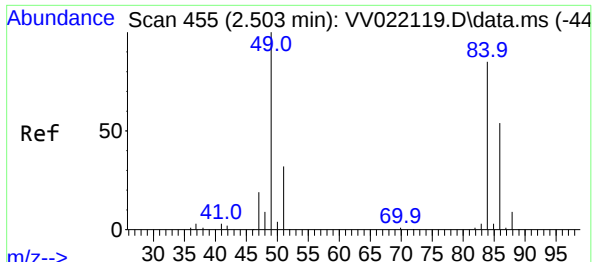

#16
Methylene chloride
Concen: 1.098 ug/L
RT: 2.507 min Scan# 456
Delta R.T. 0.003 min
Lab File: VV022120.D
Acq: 08 Sep 2021 11:31

Instrument :
MSVOA_V
ClientSampleId :
VBLK252

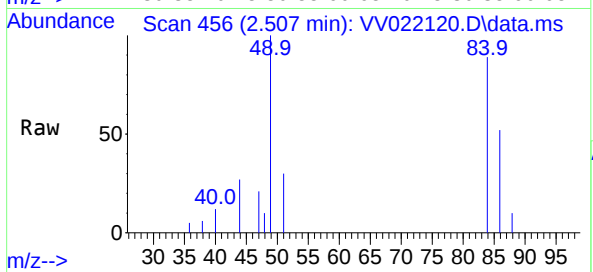

Tgt Ion:	84	Resp:	2756
Ion	Ratio	Lower	Upper
84	100		
86	58.9	44.8	83.2
49	112.7	80.2	149.0

