

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090821\
 Data File : VV022121.D
 Acq On : 08 Sep 2021 11:58
 Operator : SY/MD
 Sample : M3608-23
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Sep 09 08:28:32 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Sep 09 08:27:48 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	329900	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	306778	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	143472	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	119007	52.091	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	104.180%
7) Chloroethane-d5	1.565	69	95301	53.417	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	106.840%
11) 1,1-Dichloroethene-d2	2.102	63	167208	44.255	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	88.500%
21) 2-Butanone-d5	3.902	46	177174	113.079	ug/L	0.03
Spiked Amount	100.000	Range	40 - 130	Recovery	=	113.080%
24) Chloroform-d	4.349	84	219096	52.595	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	105.180%
26) 1,2-Dichloroethane-d4	5.031	65	139402	56.813	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	113.620%
32) Benzene-d6	5.050	84	463139	55.660	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	111.320%
36) 1,2-Dichloropropane-d6	6.069	67	144267	55.131	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	110.260%
41) Toluene-d8	7.317	98	416189	52.986	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	105.980%
43) trans-1,3-Dichloroprop...	7.622	79	61747	49.576	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	99.160%
47) 2-Hexanone-d5	8.092	63	108584	108.145	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	108.150%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	177794	53.051	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	106.100%
66) 1,2-Dichlorobenzene-d4	11.625	152	157152	55.718	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	111.440%
Target Compounds						
					Qvalue	
16) Methylene chloride	2.507	84	2834	1.112	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090821\
Data File : VV022121.D
Acq On : 08 Sep 2021 11:58
Operator : SY/MD
Sample : M3608-23
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Time: Sep 09 08:28:32 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Sep 09 08:27:48 2021
Response via : Initial Calibration

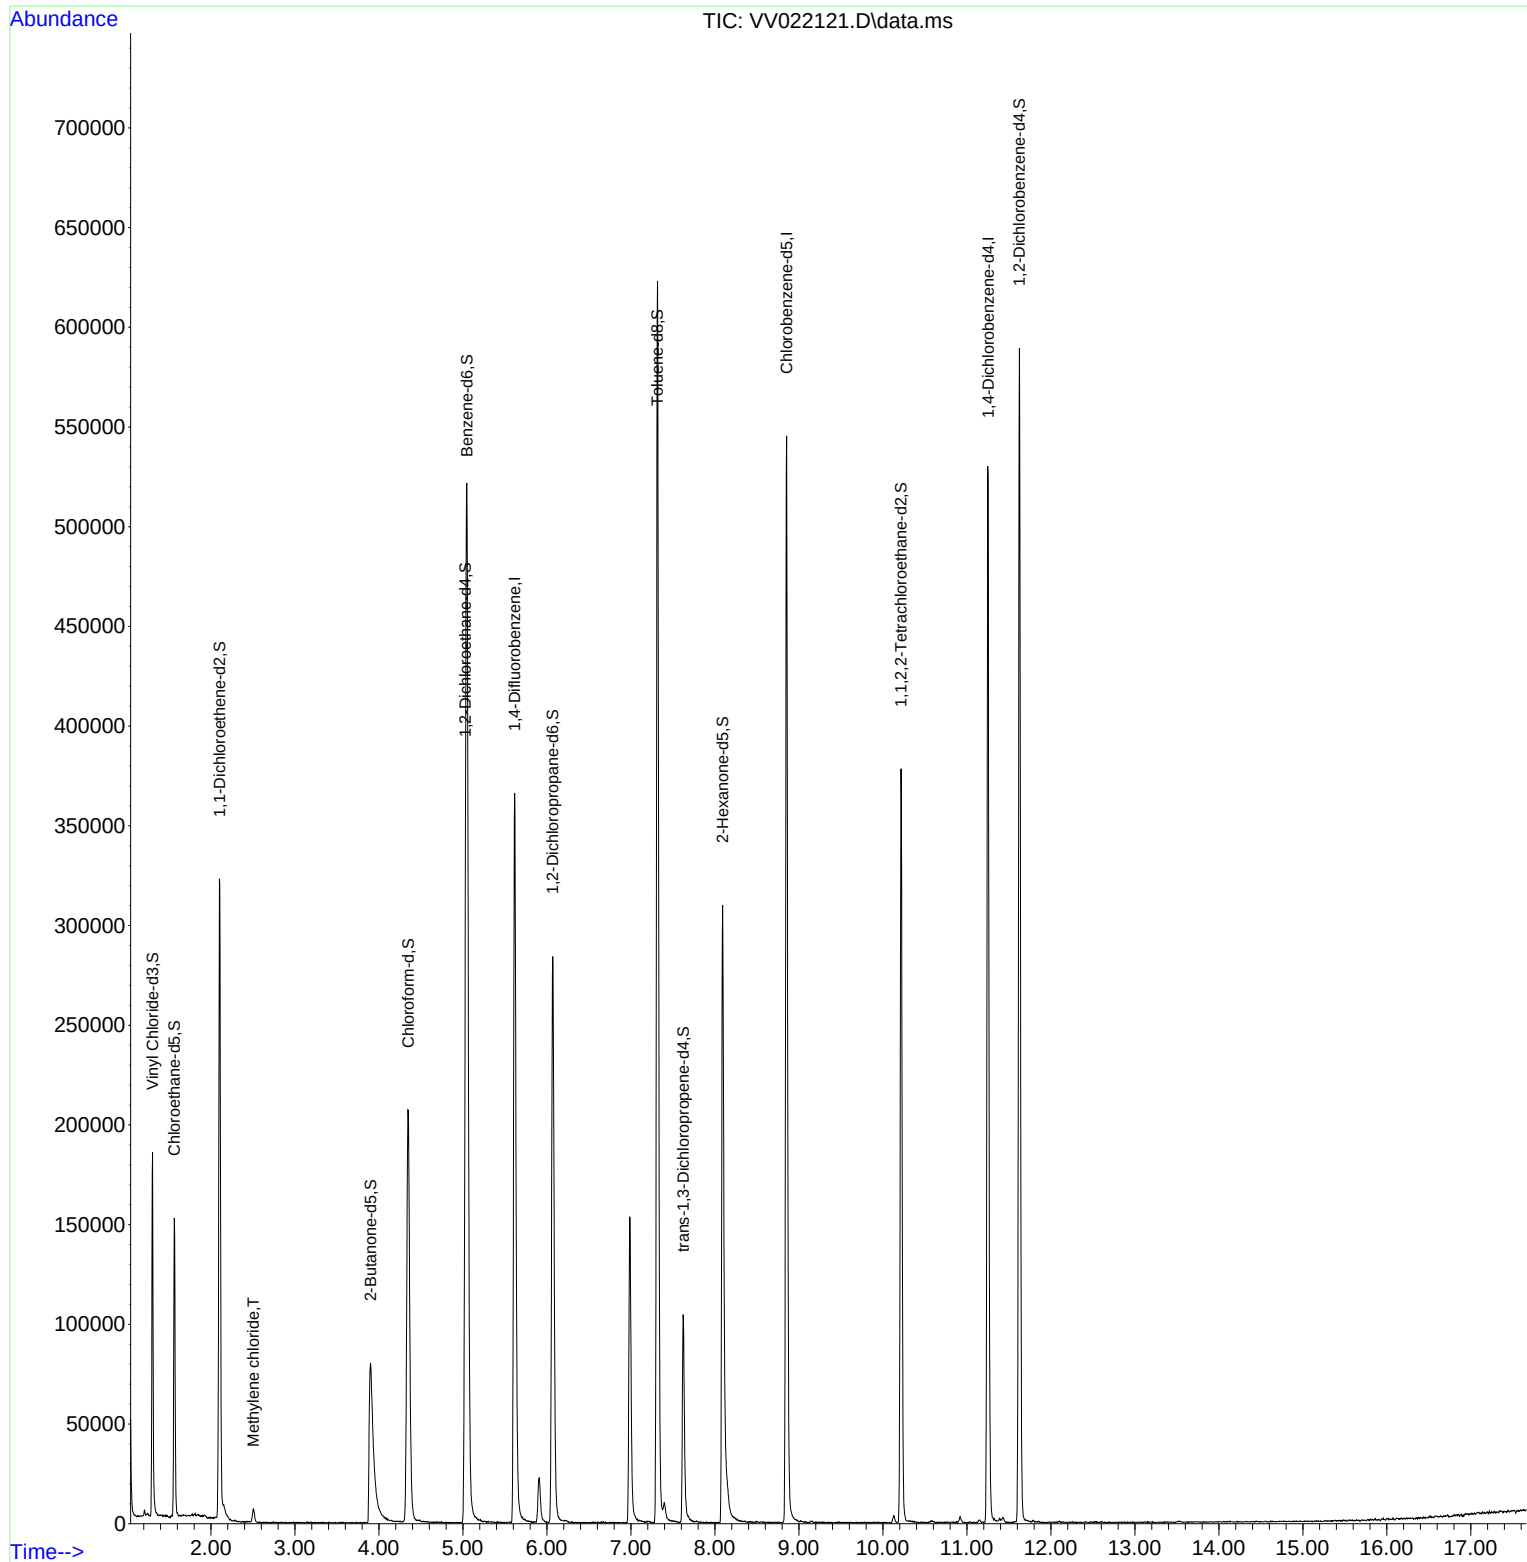

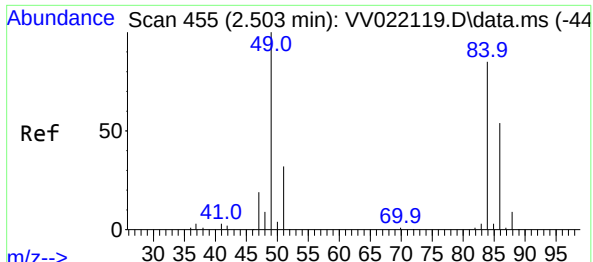

#16
Methylene chloride
Concen: 1.112 ug/L
RT: 2.507 min Scan# 456
Delta R.T. 0.003 min
Lab File: VV022121.D
Acq: 08 Sep 2021 11:58

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Tgt Ion:	84	Resp:	2834
Ion	Ratio	Lower	Upper
84	100		
86	64.1	44.8	83.2
49	110.6	80.2	149.0

