

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090821\
 Data File : VV022124.D
 Acq On : 08 Sep 2021 13:09
 Operator : SY/MD
 Sample : M3651-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKN1

Quant Time: Sep 09 08:29:04 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Sep 09 08:27:48 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	303546	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	289320	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	139788	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	116553	55.446	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	110.900%	
7) Chloroethane-d5	1.565	69	92677	56.456	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	112.920%	
11) 1,1-Dichloroethene-d2	2.102	63	163183	46.939	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	93.880%	
21) 2-Butanone-d5	3.889	46	189029	131.120	ug/L	0.02
Spiked Amount	100.000	Range 40 - 130	Recovery	=	131.120%#	
24) Chloroform-d	4.352	84	214748	56.027	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	112.060%	
26) 1,2-Dichloroethane-d4	5.034	65	134100	59.397	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	118.800%	
32) Benzene-d6	5.050	84	455695	58.070	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	116.140%	
36) 1,2-Dichloropropane-d6	6.072	67	142568	57.769	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	115.540%	
41) Toluene-d8	7.317	98	405877	54.791	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	109.580%	
43) trans-1,3-Dichloroprop...	7.625	79	60065	51.136	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	102.280%	
47) 2-Hexanone-d5	8.092	63	127975	135.149	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	135.150%#	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	187853	59.434	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	118.860%	
66) 1,2-Dichlorobenzene-d4	11.625	152	157906	57.461	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	114.920%	
Target Compounds					Qvalue	
13) Acetone	2.179	43	3238	2.681	ug/L #	72


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090821\
Data File : VV022124.D
Acq On : 08 Sep 2021 13:09
Operator : SY/MD
Sample : M3651-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKN1

Quant Time: Sep 09 08:29:04 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Sep 09 08:27:48 2021
Response via : Initial Calibration

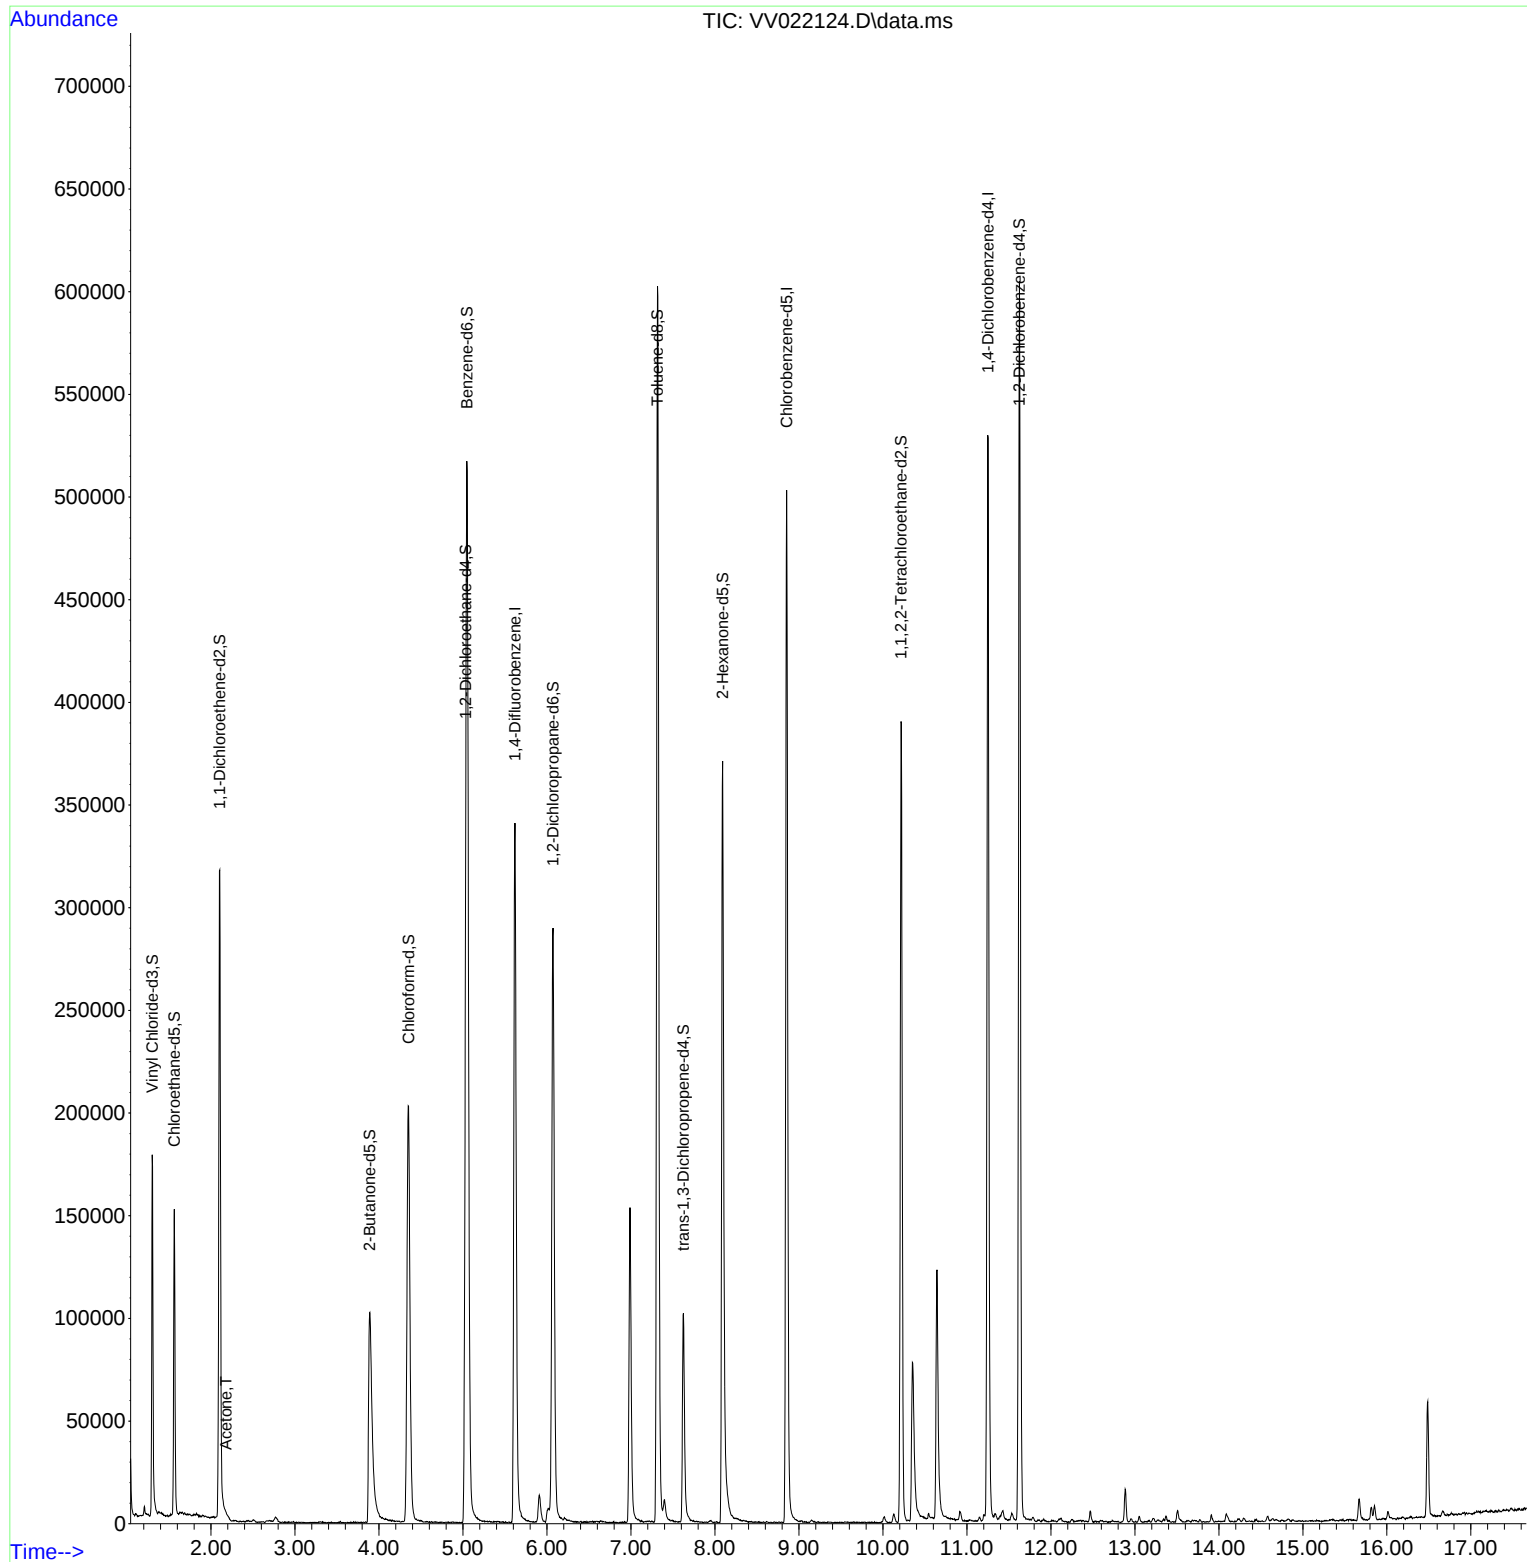

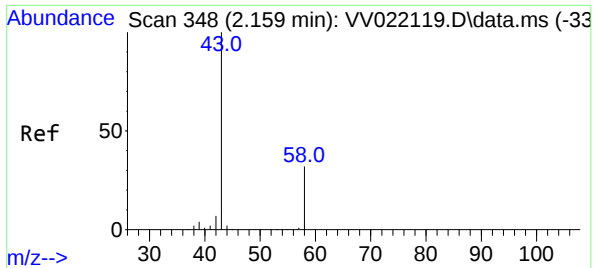

#13

Acetone

Concen: 2.681 ug/L


RT: 2.179 min Scan# 354

Delta R.T. 0.019 min

Lab File: VV022124.D

Acq: 08 Sep 2021 13:09

Instrument :
MSVOA_V
ClientSampleId :
DBKN1

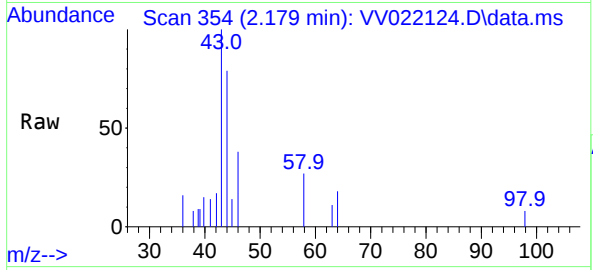

Tgt Ion: 43 Resp: 3238

Ion	Ratio	Lower	Upper
43	100		
58	35.6	0.0	0.4#

