

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090821\
 Data File : VV022125.D
 Acq On : 08 Sep 2021 13:33
 Operator : SY/MD
 Sample : M3651-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKN2

Quant Time: Sep 09 08:29:22 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Sep 09 08:27:48 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	322038	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	303644	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	143556	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	112964	50.653	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	101.300%	
7) Chloroethane-d5	1.561	69	92279	52.986	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	105.980%	
11) 1,1-Dichloroethene-d2	2.104	63	157402	42.676	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	85.360%	
21) 2-Butanone-d5	3.876	46	161740	105.749	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	105.750%	
24) Chloroform-d	4.349	84	209008	51.398	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	102.800%	
26) 1,2-Dichloroethane-d4	5.034	65	130799	54.608	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	109.220%	
32) Benzene-d6	5.050	84	434115	52.710	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	105.420%	
36) 1,2-Dichloropropane-d6	6.072	67	136098	52.546	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	105.100%	
41) Toluene-d8	7.316	98	390707	50.255	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	100.520%	
43) trans-1,3-Dichloroprop...	7.625	79	56735	46.022	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	92.040%	
47) 2-Hexanone-d5	8.088	63	105369	106.026	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	106.030%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	177307	53.451	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	106.900%	
66) 1,2-Dichlorobenzene-d4	11.625	152	150695	53.397	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	106.800%	
Target Compounds					Qvalue	
13) Acetone	2.159	43	4617	3.603	ug/L	# 74
42) Toluene	7.400	91	7642	0.801	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090821\
Data File : VV022125.D
Acq On : 08 Sep 2021 13:33
Operator : SY/MD
Sample : M3651-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKN2

Quant Time: Sep 09 08:29:22 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Sep 09 08:27:48 2021
Response via : Initial Calibration




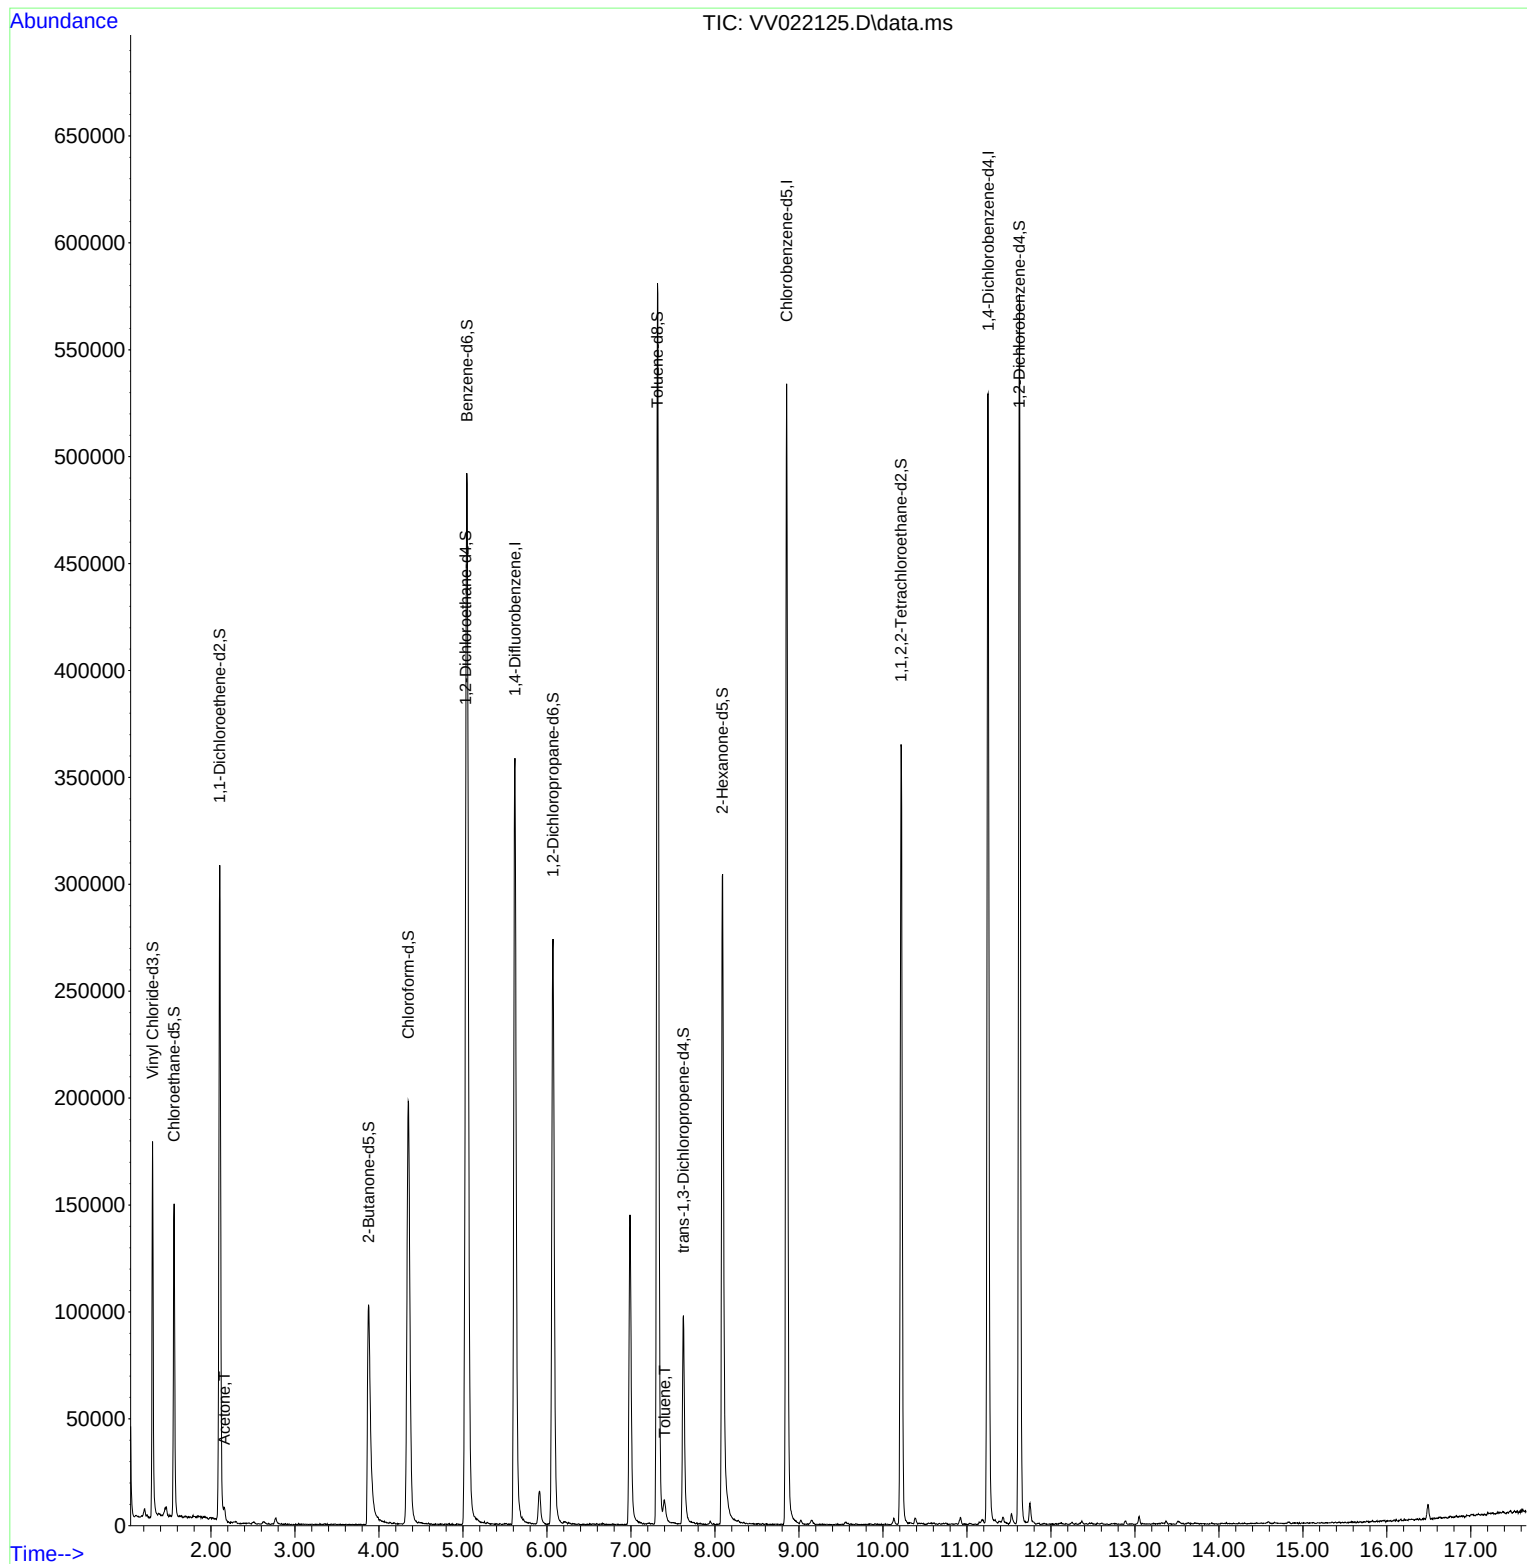


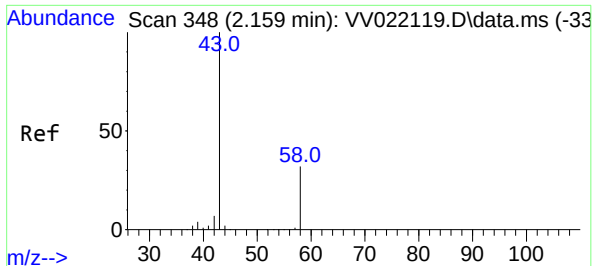

#13
Acetone
Concen: 3.603 ug/L
RT: 2.159 min Scan# 348
Delta R.T. -0.000 min
Lab File: VV022125.D
Acq: 08 Sep 2021 13:33

Instrument :
MSVOA_V
ClientSampleId :
DBKN2

Tgt Ion: 43 Resp: 4617
Ion Ratio Lower Upper
43 100
58 34.0 0.0 0.4#

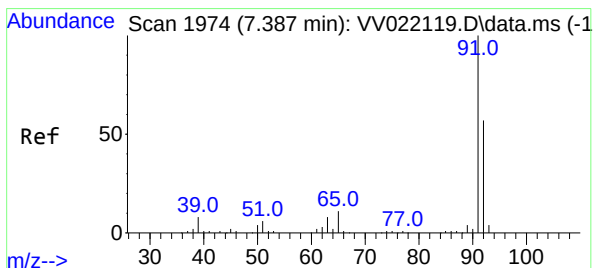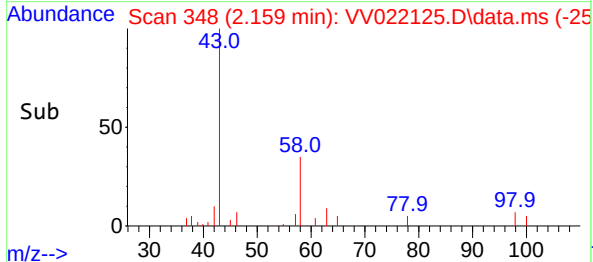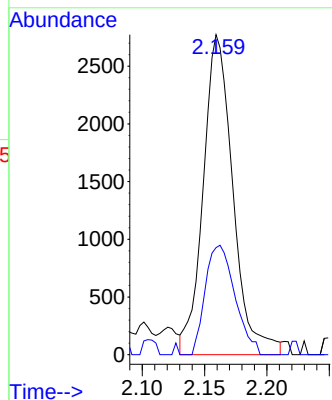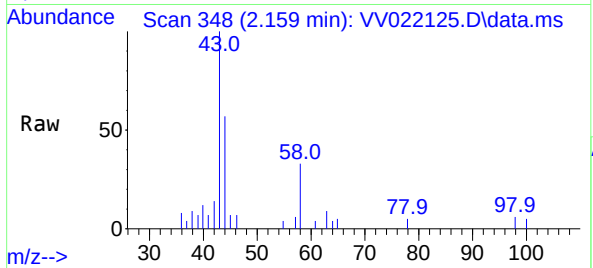

#42
Toluene
Concen: 0.801 ug/L
RT: 7.400 min Scan# 1978
Delta R.T. 0.013 min
Lab File: VV022125.D
Acq: 08 Sep 2021 13:33

Tgt Ion: 91 Resp: 7642
Ion Ratio Lower Upper
91 100
92 54.2 40.3 74.8

