

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090821\
 Data File : VV022127.D
 Acq On : 08 Sep 2021 14:22
 Operator : SY/MD
 Sample : M3651-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKN4

Quant Time: Sep 09 08:29:36 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Sep 09 08:27:48 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	318103	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	300082	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	136785	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	108656	49.324	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	98.640%	
7) Chloroethane-d5	1.561	69	90865	52.819	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	105.640%	
11) 1,1-Dichloroethene-d2	2.105	63	153284	42.074	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	84.140%	
21) 2-Butanone-d5	3.876	46	154930	102.549	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	102.550%	
24) Chloroform-d	4.349	84	203582	50.683	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	101.360%	
26) 1,2-Dichloroethane-d4	5.034	65	128688	54.392	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	108.780%	
32) Benzene-d6	5.050	84	426537	52.405	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	104.800%	
36) 1,2-Dichloropropane-d6	6.072	67	134669	52.612	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	105.220%	
41) Toluene-d8	7.317	98	380491	49.522	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	99.040%	
43) trans-1,3-Dichloroprop...	7.625	79	55370	45.448	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	90.900%	
47) 2-Hexanone-d5	8.088	63	97811	99.589	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	99.590%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	168230	51.317	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	102.640%	
66) 1,2-Dichlorobenzene-d4	11.625	152	144072	53.578	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	107.160%	
Target Compounds						
13) Acetone	2.159	43	4249	3.357	ug/L	Qvalue # 78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090821\
Data File : VV022127.D
Acq On : 08 Sep 2021 14:22
Operator : SY/MD
Sample : M3651-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKN4

Quant Time: Sep 09 08:29:36 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Sep 09 08:27:48 2021
Response via : Initial Calibration

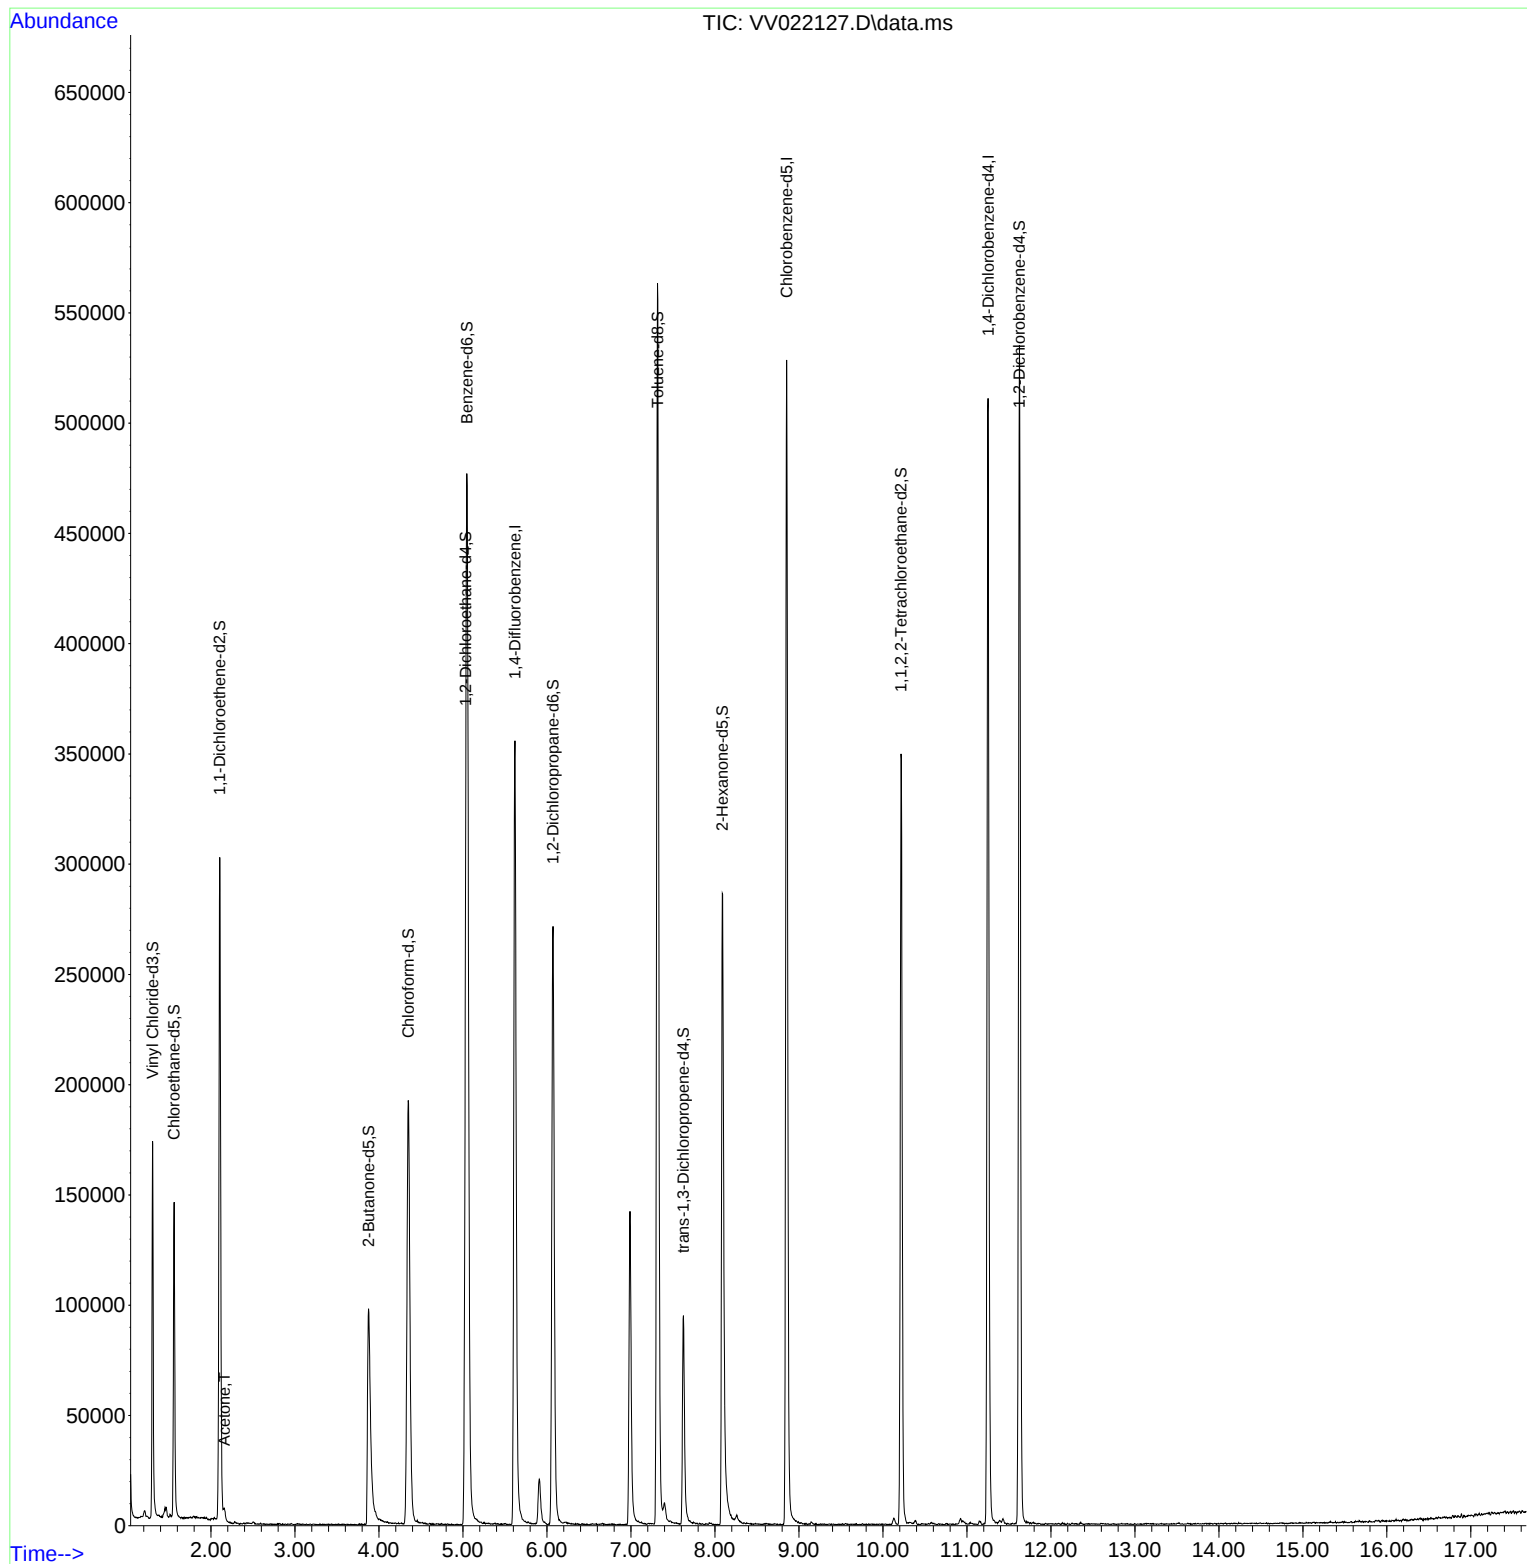

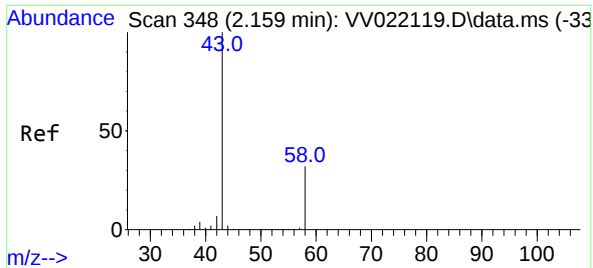

#13

Acetone

Concen: 3.357 ug/L

RT: 2.159 min Scan# 348

Delta R.T. -0.000 min

Lab File: VV022127.D

Acq: 08 Sep 2021 14:22

Instrument :
MSVOA_V
ClientSampleId :
DBKN4

Tgt Ion: 43 Resp: 4249

Ion	Ratio	Lower	Upper
43	100		
58	28.6	0.0	0.4#

