

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090821\
 Data File : VV022123.D
 Acq On : 08 Sep 2021 12:46
 Operator : SY/MD
 Sample : M3651-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKM9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M

Title : VOC Analysis

Signal : TIC: VV022123.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	100	rVB	98784	101548	10.35%	1.282%
2	1.558	155	161	182	rVB	94625	111991	11.41%	1.414%
3	2.105	321	331	345	rBV	192300	286491	29.20%	3.618%
4	2.407	423	425	428	rBV2	490	214	0.02%	0.003%
5	2.445	434	437	441	rBV2	591	479	0.05%	0.006%
6	2.478	445	447	450	rVB2	465	226	0.02%	0.003%
7	2.510	450	457	458	rBV2	952	1059	0.11%	0.013%
8	2.619	489	491	496	rVB2	385	219	0.02%	0.003%
9	2.699	511	516	517	rBV2	334	227	0.02%	0.003%
10	2.751	530	532	537	rBV2	488	322	0.03%	0.004%
11	2.838	556	559	564	rBV2	438	289	0.03%	0.004%
12	2.889	571	575	580	rBV2	379	409	0.04%	0.005%
13	2.944	588	592	595	rBV3	270	244	0.02%	0.003%
14	3.175	662	664	665	rVV3	479	172	0.02%	0.002%
15	3.468	751	755	761	rVB	515	392	0.04%	0.005%
16	3.584	789	791	795	rVV3	301	201	0.02%	0.003%
17	3.619	798	802	804	rBV	275	200	0.02%	0.003%
18	3.677	817	820	823	rBV	357	190	0.02%	0.002%
19	3.786	851	854	856	rVB2	289	177	0.02%	0.002%
20	3.873	872	881	913	rBV	99693	259553	26.45%	3.278%
21	4.262	1000	1002	1007	rVB2	405	174	0.02%	0.002%
22	4.349	1014	1029	1052	rBV	159438	394797	40.24%	4.986%
23	4.625	1113	1115	1120	rVB2	400	330	0.03%	0.004%
24	4.706	1137	1140	1144	rVB	294	192	0.02%	0.002%
25	4.799	1166	1169	1172	rVB2	425	258	0.03%	0.003%
26	4.828	1176	1178	1181	rVB2	328	171	0.02%	0.002%
27	4.902	1198	1201	1204	rVV2	346	249	0.03%	0.003%
28	4.931	1207	1210	1212	rBV2	349	200	0.02%	0.003%
29	5.047	1227	1246	1275	rBV2	384752	981165	100.00%	12.391%
30	5.368	1343	1346	1350	rBV3	255	235	0.02%	0.003%
31	5.384	1350	1351	1357	rVB2	547	247	0.03%	0.003%
32	5.616	1410	1423	1450	rBV	353543	722951	73.68%	9.130%
33	5.908	1503	1514	1532	rBV3	12308	26432	2.69%	0.334%
34	5.998	1539	1542	1545	rBV2	269	225	0.02%	0.003%
35	6.072	1552	1565	1593	rBV	221292	460006	46.88%	5.809%
36	6.494	1693	1696	1699	rBV	247	187	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090821\
 Data File : VV022123.D
 Acq On : 08 Sep 2021 12:46
 Operator : SY/MD
 Sample : M3651-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKM9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

37	6.699	1756	1760	1761	rBV3	283	189	0.02%	0.002%
38	6.844	1802	1805	1807	rVV2	379	209	0.02%	0.003%
39	6.989	1838	1850	1882	rBV	114783	214265	21.84%	2.706%
40	7.194	1912	1914	1916	rBV3	350	233	0.02%	0.003%
41	7.317	1941	1952	1970	rBV	436906	763464	77.81%	9.641%
42	7.625	2034	2048	2072	rBV	78296	138421	14.11%	1.748%
43	7.860	2118	2121	2125	rBV	234	222	0.02%	0.003%
44	7.934	2139	2144	2145	rBV	529	420	0.04%	0.005%
45	7.985	2151	2160	2170	rVB6	3767	6264	0.64%	0.079%
46	8.056	2176	2182	2183	rBV3	372	303	0.03%	0.004%
47	8.088	2183	2192	2232	rBV	285759	540442	55.08%	6.825%
48	8.439	2298	2301	2304	rBV3	412	279	0.03%	0.004%
49	8.474	2309	2312	2315	rVB	580	277	0.03%	0.003%
50	8.490	2315	2317	2321	rBV3	361	194	0.02%	0.002%
51	8.577	2338	2344	2346	rBV3	434	467	0.05%	0.006%
52	8.612	2353	2355	2360	rVB2	525	263	0.03%	0.003%
53	8.648	2363	2366	2370	rBV2	380	275	0.03%	0.003%
54	8.686	2375	2378	2381	rBV	356	167	0.02%	0.002%
55	8.712	2381	2386	2388	rBV2	350	288	0.03%	0.004%
56	8.773	2400	2405	2408	rBV	344	324	0.03%	0.004%
57	8.854	2417	2430	2450	rBV	521602	860794	87.73%	10.870%
58	9.288	2561	2565	2567	rBV2	291	195	0.02%	0.002%
59	9.490	2624	2628	2629	rBV	223	162	0.02%	0.002%
60	9.526	2636	2639	2644	rVB2	356	317	0.03%	0.004%
61	9.561	2647	2650	2653	rVB3	417	251	0.03%	0.003%
62	9.635	2669	2673	2675	rBV2	276	171	0.02%	0.002%
63	9.738	2700	2705	2710	rVB2	400	387	0.04%	0.005%
64	9.815	2725	2729	2732	rVB	253	172	0.02%	0.002%
65	10.124	2821	2825	2827	rBV3	843	733	0.07%	0.009%
66	10.217	2842	2854	2879	rBV	340606	532572	54.28%	6.726%
67	10.304	2879	2881	2882	rBV2	475	174	0.02%	0.002%
68	10.455	2923	2928	2932	rBV3	370	290	0.03%	0.004%
69	10.558	2955	2960	2961	rBV2	267	240	0.02%	0.003%
70	10.622	2976	2980	2983	rBV2	264	223	0.02%	0.003%
71	10.722	3001	3011	3013	rBV3	447	619	0.06%	0.008%
72	10.754	3019	3021	3026	rVB3	402	270	0.03%	0.003%
73	10.780	3026	3029	3031	rBV	456	215	0.02%	0.003%
74	10.825	3038	3043	3047	rVV2	397	399	0.04%	0.005%
75	10.866	3051	3056	3059	rVB2	261	219	0.02%	0.003%
76	10.911	3065	3070	3073	rBV4	926	1021	0.10%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090821\
 Data File : VV022123.D
 Acq On : 08 Sep 2021 12:46
 Operator : SY/MD
 Sample : M3651-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKM9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

77	11.133	3136	3139	3141	rBV3	393	229	0.02%	0.003%
78	11.252	3163	3176	3196	rBV	495558	776964	79.19%	9.812%
79	11.484	3245	3248	3251	rBV2	204	208	0.02%	0.003%
80	11.545	3264	3267	3277	rVB5	906	1262	0.13%	0.016%
81	11.625	3277	3292	3316	rBV	451979	715627	72.94%	9.037%
82	11.783	3337	3341	3343	rBV2	752	484	0.05%	0.006%
83	11.825	3351	3354	3358	rVB3	289	238	0.02%	0.003%
84	11.847	3358	3361	3362	rBV	495	233	0.02%	0.003%
85	11.879	3367	3371	3373	rBV	295	203	0.02%	0.003%
86	11.895	3374	3376	3380	rVB3	354	212	0.02%	0.003%
87	11.988	3402	3405	3407	rBV	473	273	0.03%	0.003%
88	12.043	3418	3422	3427	rVB3	427	457	0.05%	0.006%
89	12.117	3442	3445	3449	rVB2	380	240	0.02%	0.003%
90	12.207	3469	3473	3475	rBV2	269	217	0.02%	0.003%
91	12.246	3480	3485	3491	rVV4	535	618	0.06%	0.008%
92	12.593	3591	3593	3598	rVB2	458	322	0.03%	0.004%
93	12.956	3701	3706	3709	rBV2	367	406	0.04%	0.005%
94	13.008	3720	3722	3729	rBV2	253	258	0.03%	0.003%
95	13.075	3741	3743	3749	rVV2	336	205	0.02%	0.003%
96	13.332	3819	3823	3827	rBV2	366	318	0.03%	0.004%
97	13.670	3926	3928	3931	rBV2	334	213	0.02%	0.003%
98	13.750	3951	3953	3958	rBV2	288	210	0.02%	0.003%
99	13.902	3998	4000	4002	rBV	386	178	0.02%	0.002%
100	14.107	4061	4064	4067	rBV2	373	275	0.03%	0.003%




Sum of corrected areas: 7918662

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090821\
Data File : VV022123.D
Acq On : 08 Sep 2021 12:46
Operator : SY/MD
Sample : M3651-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKM9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

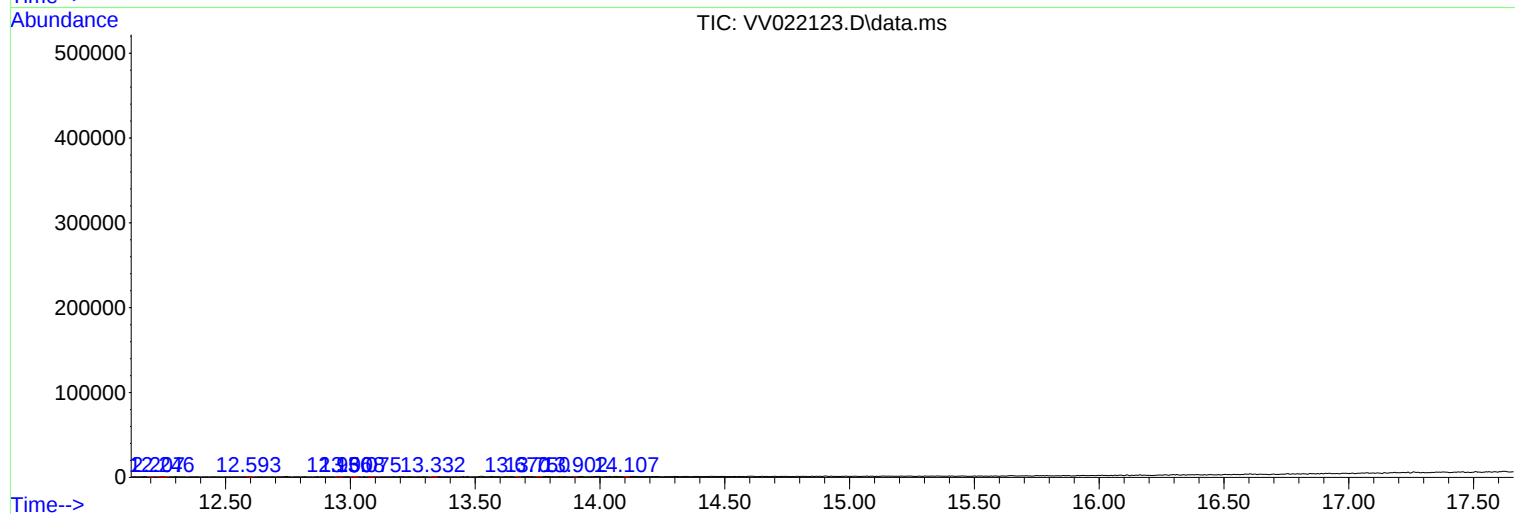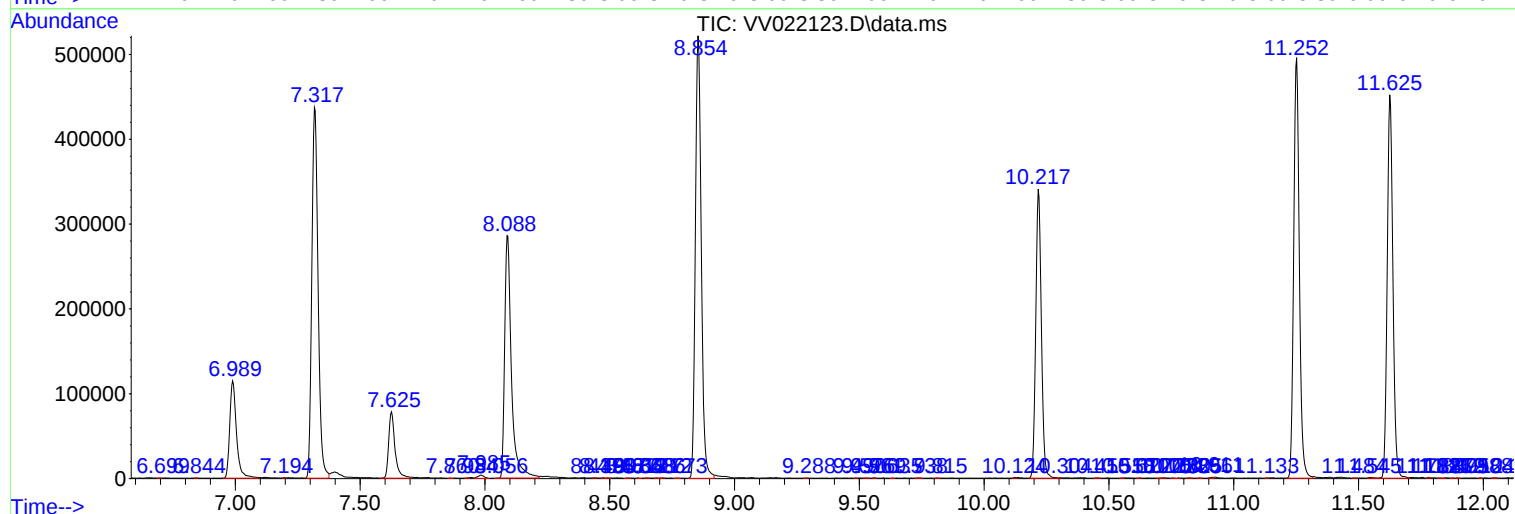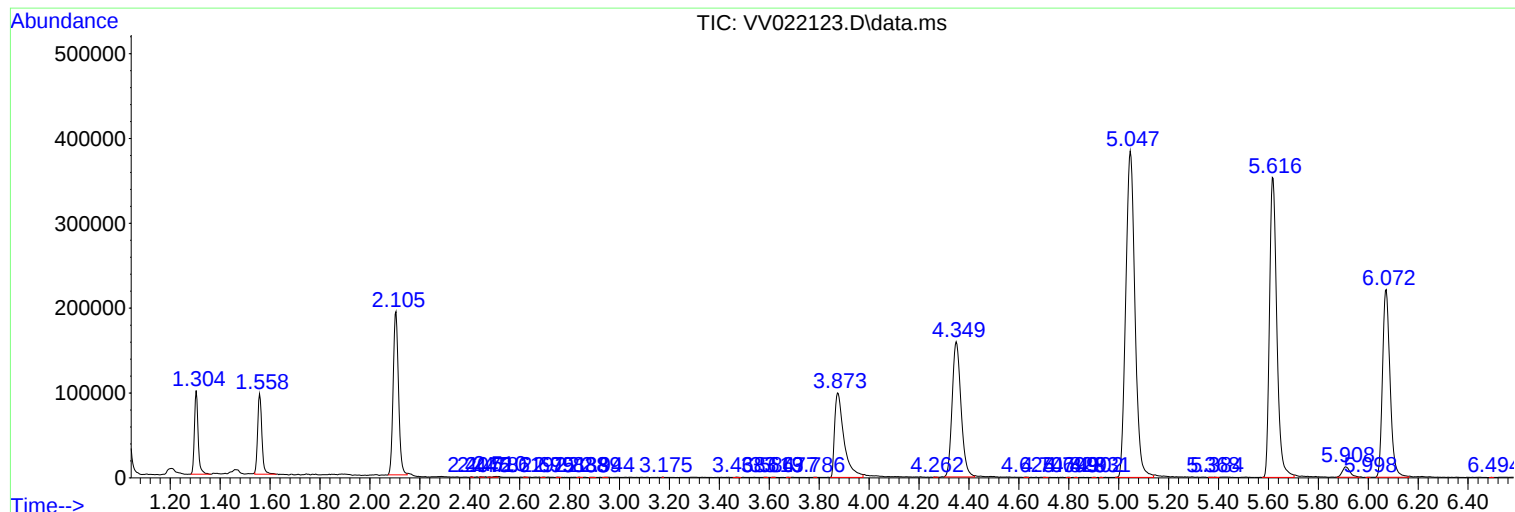

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090821\
Data File : VV022123.D
Acq On : 08 Sep 2021 12:46
Operator : SY/MD
Sample : M3651-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKM9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090821\
Data File : VV022123.D
Acq On : 08 Sep 2021 12:46
Operator : SY/MD
Sample : M3651-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKM9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------