


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090821\
 Data File : VV022118.D
 Acq On : 08 Sep 2021 09:14
 Operator : SY/MD
 Sample : BFB229
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB229

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis
 Last Update : Thu Sep 09 08:27:48 2021

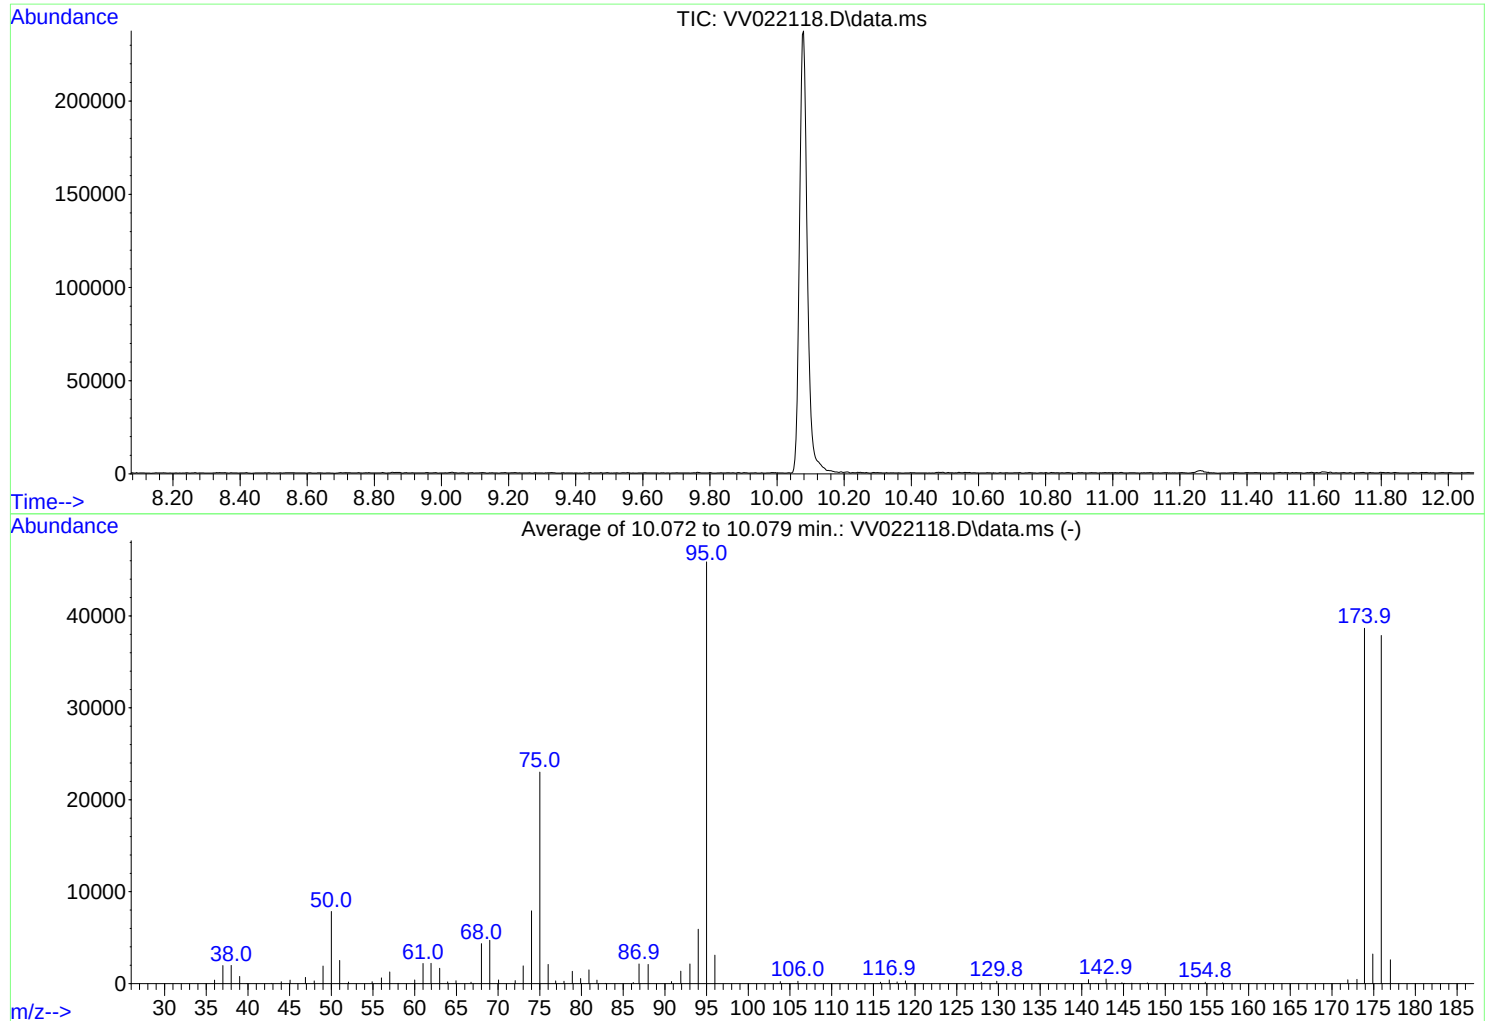

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2799

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	7850	PASS
75	95	30	80	50.1	23011	PASS
95	95	100	100	100.0	45885	PASS
96	95	5	9	6.7	3093	PASS
173	174	0.00	2	1.2	466	PASS
174	95	50	120	84.2	38651	PASS
175	174	5	9	8.3	3222	PASS
176	174	95	105	98.0	37867	PASS
177	176	5	10	6.9	2597	PASS

Scan 2799 (10.040 min): VV022118.D\data.ms
BFB229

m/z	Abundance
39.90	183.0
44.10	296.0

Instrument :
MSVOA_V
ClientSampleId :
BFB229

m/z	Abundance
36.00	383.0
37.00	2009.0
38.00	1954.0
39.00	789.0
39.90	220.0
42.80	109.0
43.90	572.0
45.10	386.0
46.90	683.0
48.00	289.0
49.00	1937.0
50.00	8255.0
51.00	2575.0
52.00	156.0
54.90	212.0
56.00	631.0
57.00	1322.0
60.00	433.0
61.00	2231.0
61.90	2248.0
63.00	1776.0
63.90	212.0
64.90	351.0
66.80	149.0
68.00	4452.0
69.00	4724.0
70.00	457.0
72.10	326.0
73.00	1911.0
74.00	8193.0
75.00	23352.0
76.00	2097.0
76.90	362.0
77.90	283.0
78.90	1386.0
79.90	579.0
80.90	1650.0
81.80	362.0
82.90	104.0
86.20	204.0
86.90	2410.0
88.00	2115.0
90.80	249.0
91.90	1478.0
93.00	2159.0
94.00	6053.0
95.00	47440.0
96.00	3252.0
103.90	222.0
105.90	293.0
115.90	187.0
116.90	448.0
117.90	216.0
118.80	287.0
127.90	204.0
129.80	231.0
130.90	105.0
134.80	130.0
140.80	504.0
142.90	498.0
145.10	130.0
146.00	151.0
147.90	147.0
154.90	158.0
171.90	424.0
173.00	483.0
173.90	40792.0
174.90	3313.0
175.90	40336.0
177.00	2856.0

Instrument :
MSVOA_V
ClientSampleId :
BFB229

m/z	Abundance
36.00	400.0
37.00	2047.0
38.00	2040.0
39.00	847.0
39.90	194.0
43.90	517.0
45.10	407.0
46.90	700.0
47.90	303.0
49.00	1980.0
50.00	8103.0
51.00	2632.0
52.10	170.0
54.90	216.0
56.00	644.0
57.00	1307.0
60.00	394.0
61.00	2295.0
61.90	2292.0
63.00	1687.0
64.00	179.0
65.00	311.0
66.80	164.0
68.00	4536.0
69.00	4949.0
70.00	407.0
72.00	342.0
73.00	1973.0
74.00	8161.0
75.00	23840.0
76.00	2188.0
76.90	295.0
77.90	262.0
78.90	1356.0
79.90	571.0
80.90	1554.0
81.90	381.0
86.20	143.0
86.90	2223.0
88.00	2184.0
90.80	246.0
91.90	1405.0
93.00	2251.0
94.00	6134.0
95.00	47624.0
96.00	3173.0
103.80	238.0
106.00	285.0
115.90	161.0
116.90	426.0
117.80	192.0
118.90	302.0
127.90	146.0
129.80	282.0
140.80	437.0
142.90	512.0
144.80	143.0
147.80	119.0
154.80	166.0
156.90	131.0
171.90	414.0
173.00	484.0
173.90	39856.0
174.90	3398.0
175.90	39208.0
177.00	2680.0

Instrument :
MSVOA_V
ClientSampleId :
BFB229

m/z	Abundance
36.00	373.0
37.00	1871.0
38.00	1945.0
39.00	734.0
39.90	208.0
44.00	417.0
45.00	377.0
46.90	633.0
47.90	293.0
49.00	1830.0
50.00	7193.0
51.00	2392.0
52.10	180.0
54.90	201.0
56.00	626.0
57.00	1191.0
58.00	116.0
60.00	375.0
61.00	2058.0
62.00	2071.0
63.00	1560.0
64.00	179.0
65.00	264.0
66.70	173.0
68.00	4082.0
69.00	4490.0
70.10	360.0
72.00	310.0
73.00	1912.0
74.00	7428.0
75.00	21840.0
76.00	1977.0
76.90	231.0
77.90	226.0
78.90	1296.0
79.90	501.0
80.90	1307.0
81.90	392.0
86.90	1799.0
88.00	1951.0
90.80	199.0
91.90	1171.0
93.00	2011.0
94.00	5560.0
95.00	42592.0
96.00	2854.0
103.80	241.0
106.00	200.0
115.80	138.0
116.90	334.0
117.80	161.0
118.90	321.0
128.00	101.0
129.80	272.0
140.80	362.0
141.70	117.0
142.90	522.0
144.80	169.0
154.70	159.0
156.90	142.0
171.90	417.0
173.00	430.0
173.90	35304.0
174.90	2954.0
175.90	34056.0
177.00	2255.0

Instrument :
MSVOA_V
ClientSampleId :
BFB229